

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
 Data File : P0065976.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2020 2:03
 Operator : DD\AJ
 Sample : L1017-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TR-04-012420

Manual Integrations
 APPROVED

mohammad
 1/28/2020 2:41:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 04:12:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.432	914699	1091326	39.447m	41.087
2) SA Decachlor...	9.654	8.332	658580	802043	15.821	16.504

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
Data File : P0065976.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2020 2:03
Operator : DD\AJ
Sample : L1017-07
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TR-04-012420


Manual Integrations
APPROVED

mohammad
1/28/2020 2:41:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 04:12:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

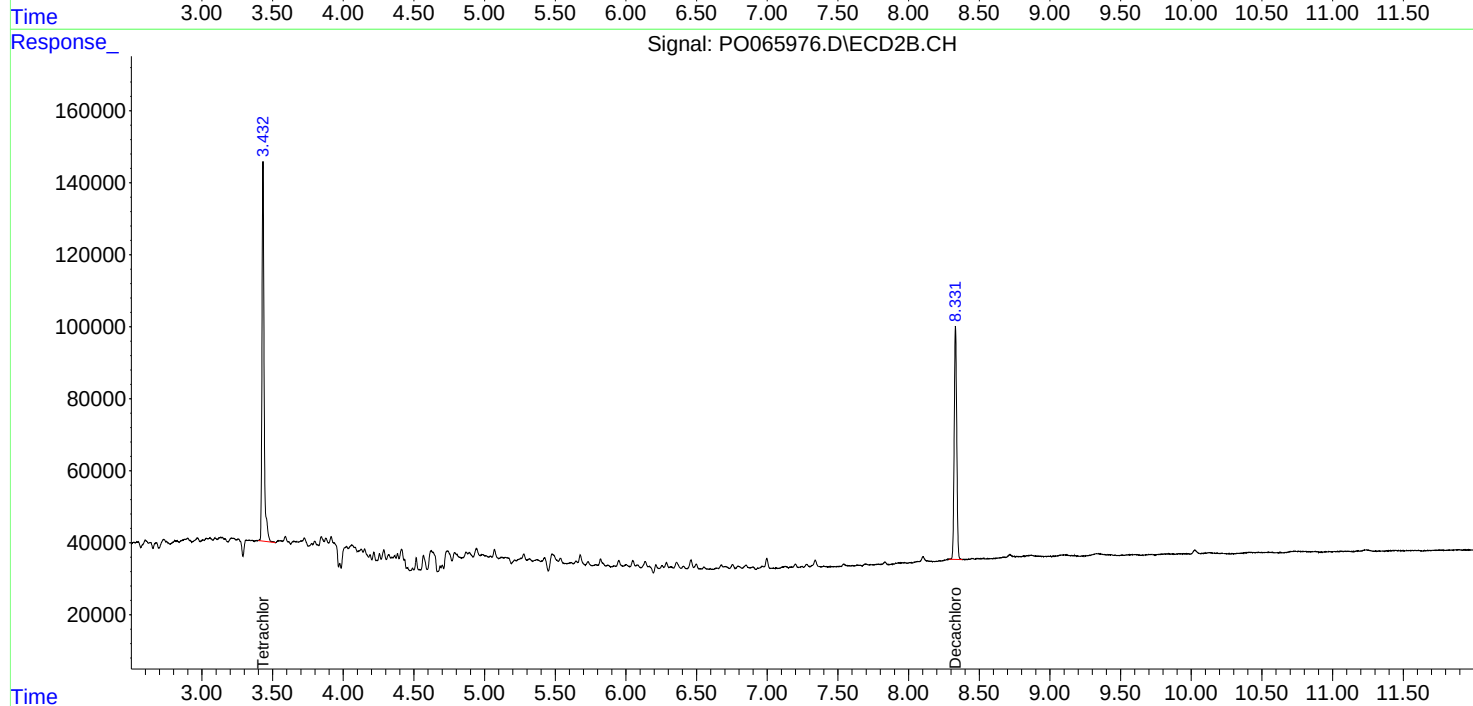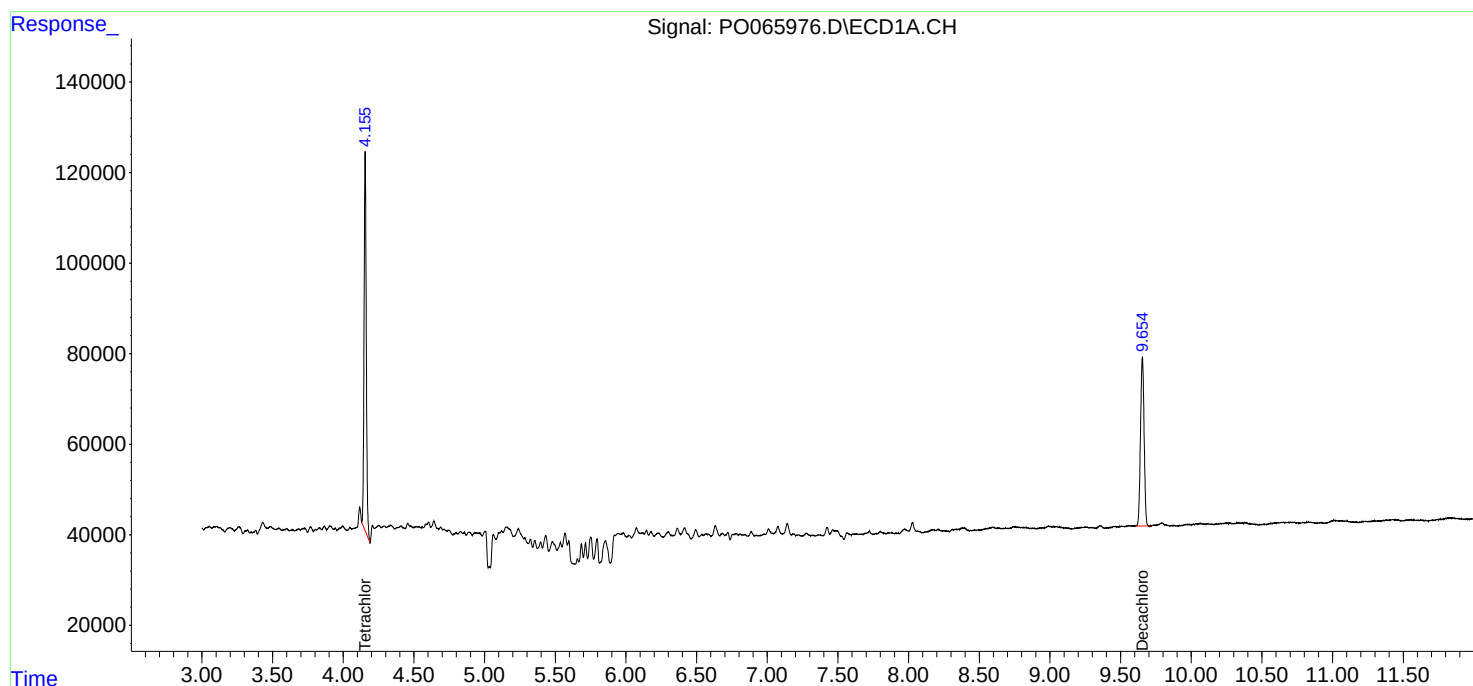

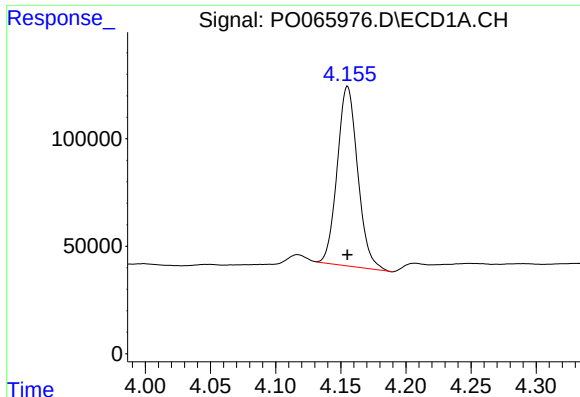


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 914699
Conc: 39.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TR-04-012420


Manual Integrations
APPROVED

mohammad
1/28/2020 2:41:04 PM

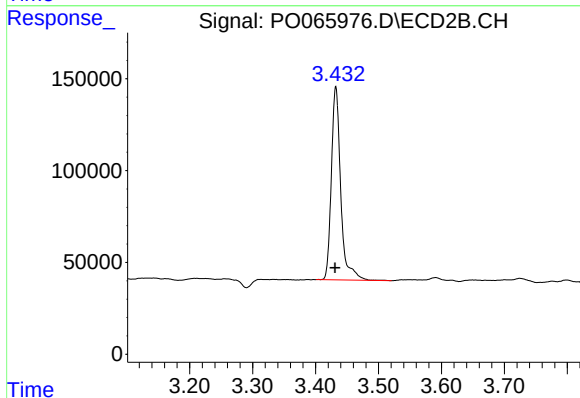


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.001 min
Response: 1091326
Conc: 41.09 ng/ml

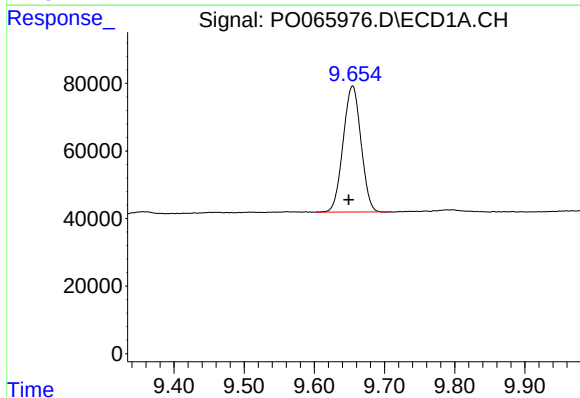

#2 Decachlorobiphenyl

R.T.: 9.654 min
Delta R.T.: 0.006 min
Response: 658580
Conc: 15.82 ng/ml

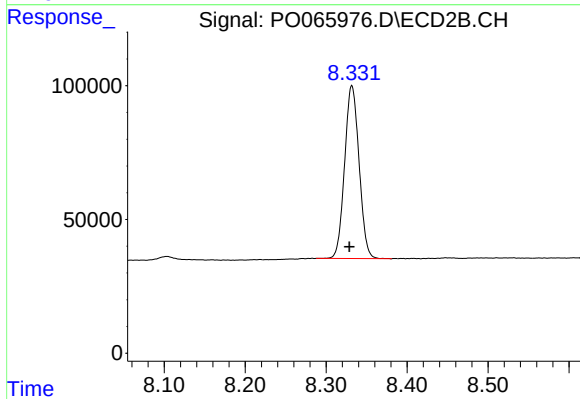

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: 0.003 min
Response: 802043
Conc: 16.50 ng/ml