

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
 Data File : P0065983.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2020 4:00
 Operator : DD\AJ
 Sample : L1245-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20200066-AMENDED-COMP-4

Manual Integrations
 APPROVED

mohammad
 1/28/2020 2:41:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 05:20:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.156	3.433	879682	1073269	37.937m	40.407m
2) SA Decachlor...	9.654	8.332	640283	781348	15.381	16.078

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
Data File : P0065983.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2020 4:00
Operator : DD\AJ
Sample : L1245-04
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20200066-AMENDED-COMP-4


Manual Integrations
APPROVED

mohammad
1/28/2020 2:41:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 05:20:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

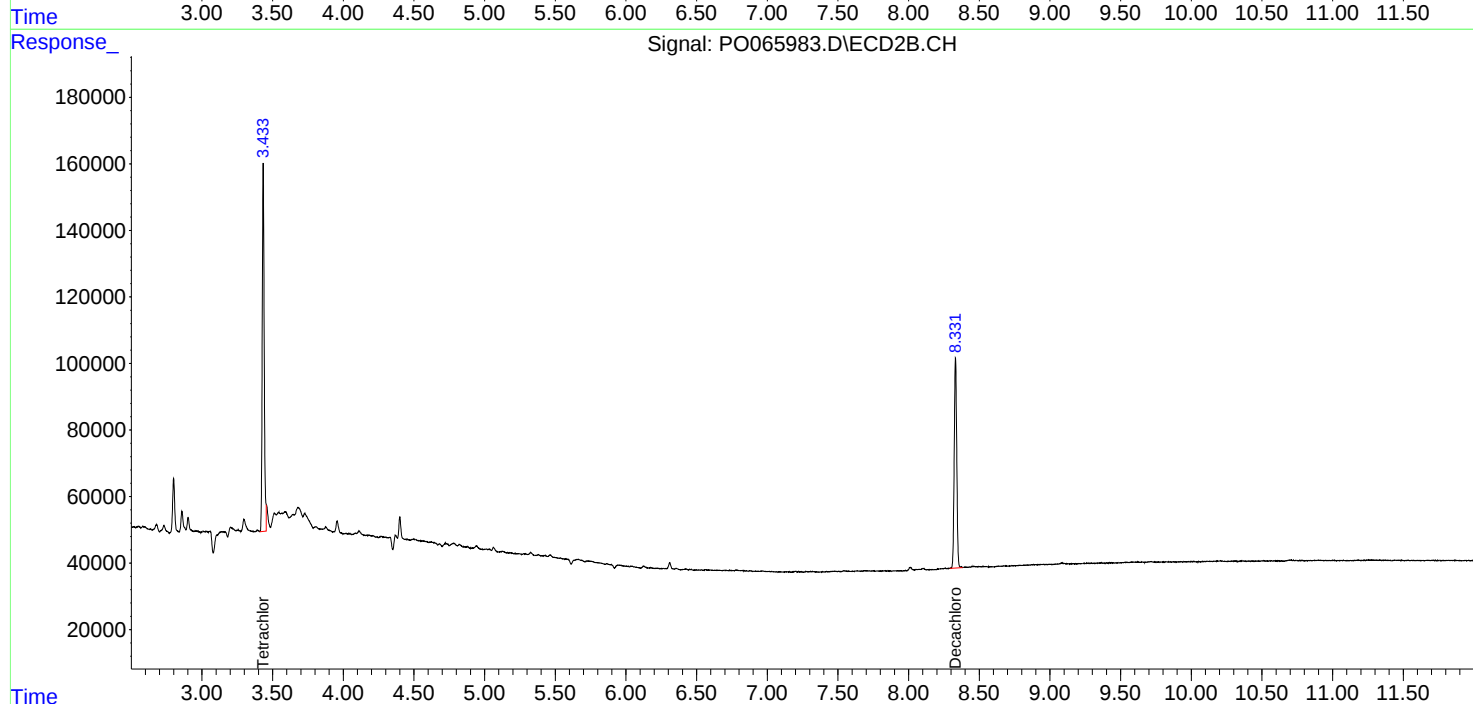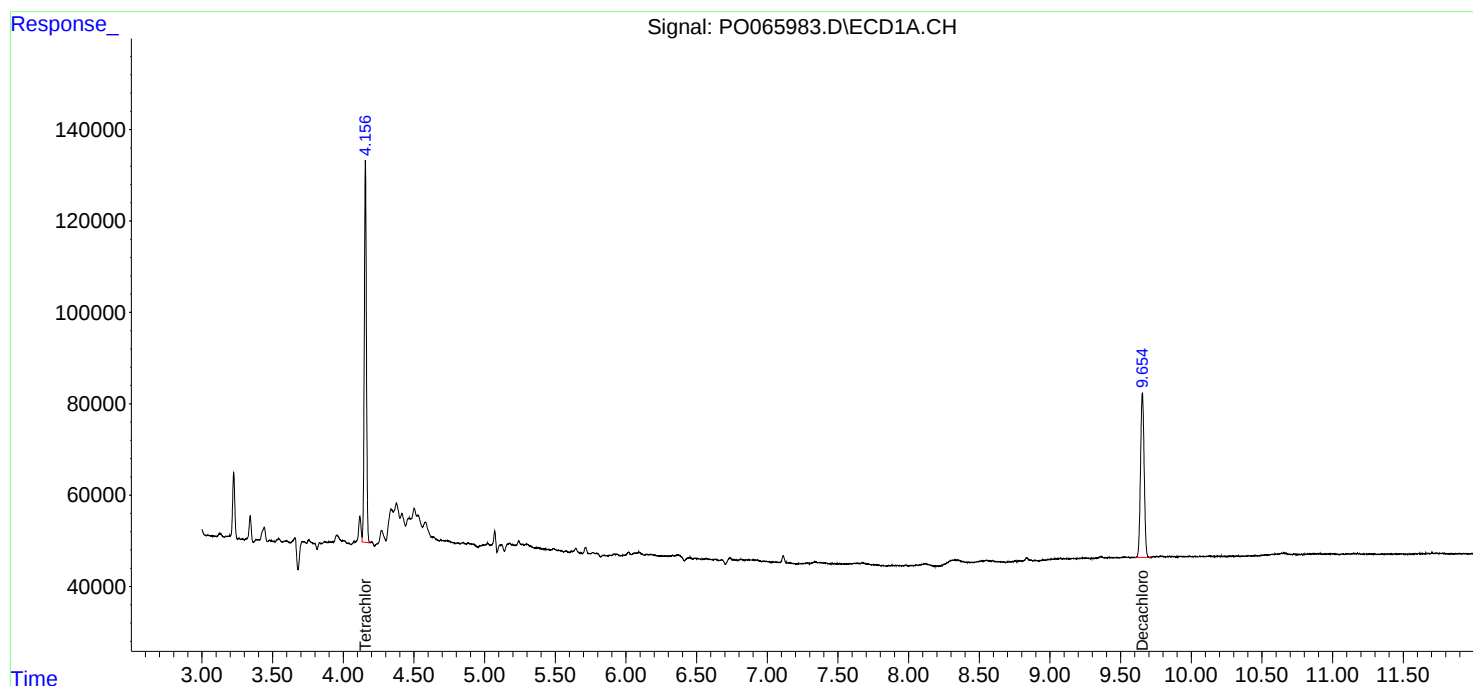

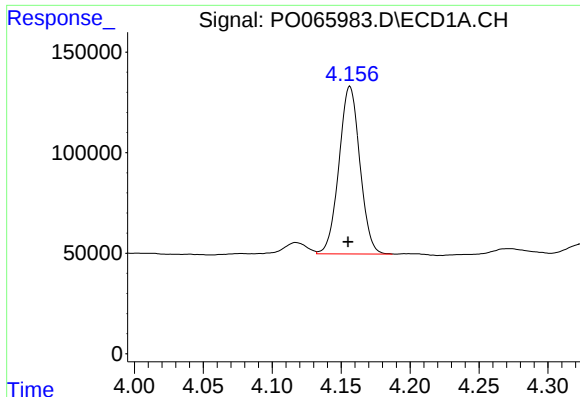


#1 Tetrachloro-m-xylene

R.T.: 4.156 min
Delta R.T.: 0.000 min
Response: 879682
Conc: 37.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
20200066-AMENDED-COMP-4


Manual Integrations
APPROVED

mohammad
1/28/2020 2:41:10 PM

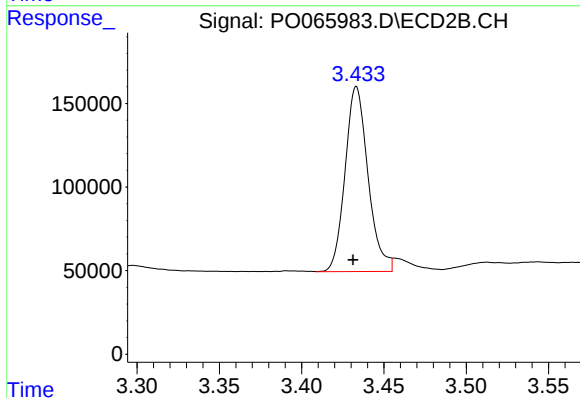


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.002 min
Response: 1073269
Conc: 40.41 ng/ml m

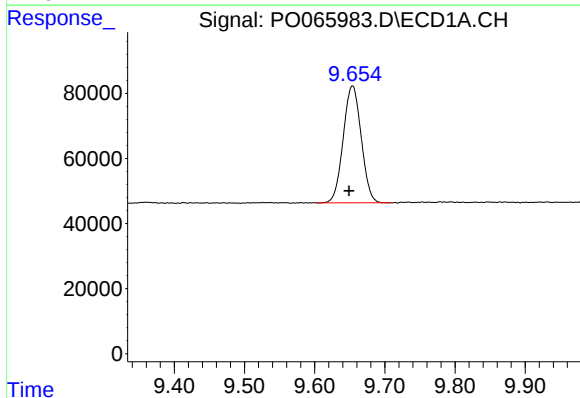

#2 Decachlorobiphenyl

R.T.: 9.654 min
Delta R.T.: 0.005 min
Response: 640283
Conc: 15.38 ng/ml

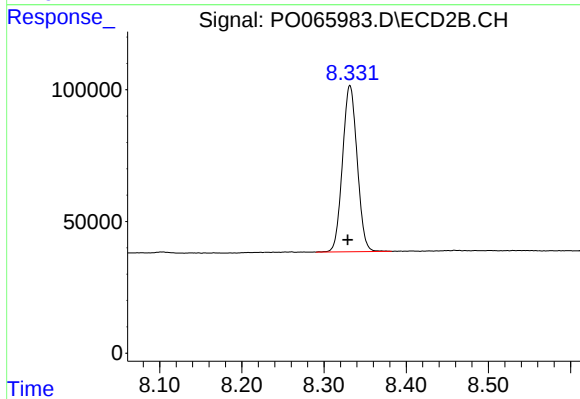

#2 Decachlorobiphenyl

R.T.: 8.332 min
Delta R.T.: 0.003 min
Response: 781348
Conc: 16.08 ng/ml