

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012821\
 Data File : P0075309.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2021 4:35
 Operator : AJ/MA
 Sample : M1247-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 250EM-018-0002

Manual Integrations
 APPROVED

Ankita
 1/29/2021 1:13:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 08:06:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 07:43:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.995	2302646	1115606	22.753	23.212
2) SA Decachlor...	10.937	9.244	2338672	1134615	24.255	23.386
Target Compounds						
36) L8 AR-1262-1	8.571	7.341	115005	56790	13.179m	26.036 #
37) L8 AR-1262-2	9.129	7.887	184618	61285	12.209	7.991 #
38) L8 AR-1262-3	9.438	8.173	242215	114982	23.186	34.745 #
39) L8 AR-1262-4	9.533	8.238	248535	117552	33.626	20.473 #
40) L8 AR-1262-5	10.196	8.730	103569	62486	19.971	22.715

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012821\
Data File : P0075309.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2021 4:35
Operator : AJ/MA
Sample : M1247-07
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
250EM-018-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 08:06:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 07:43:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

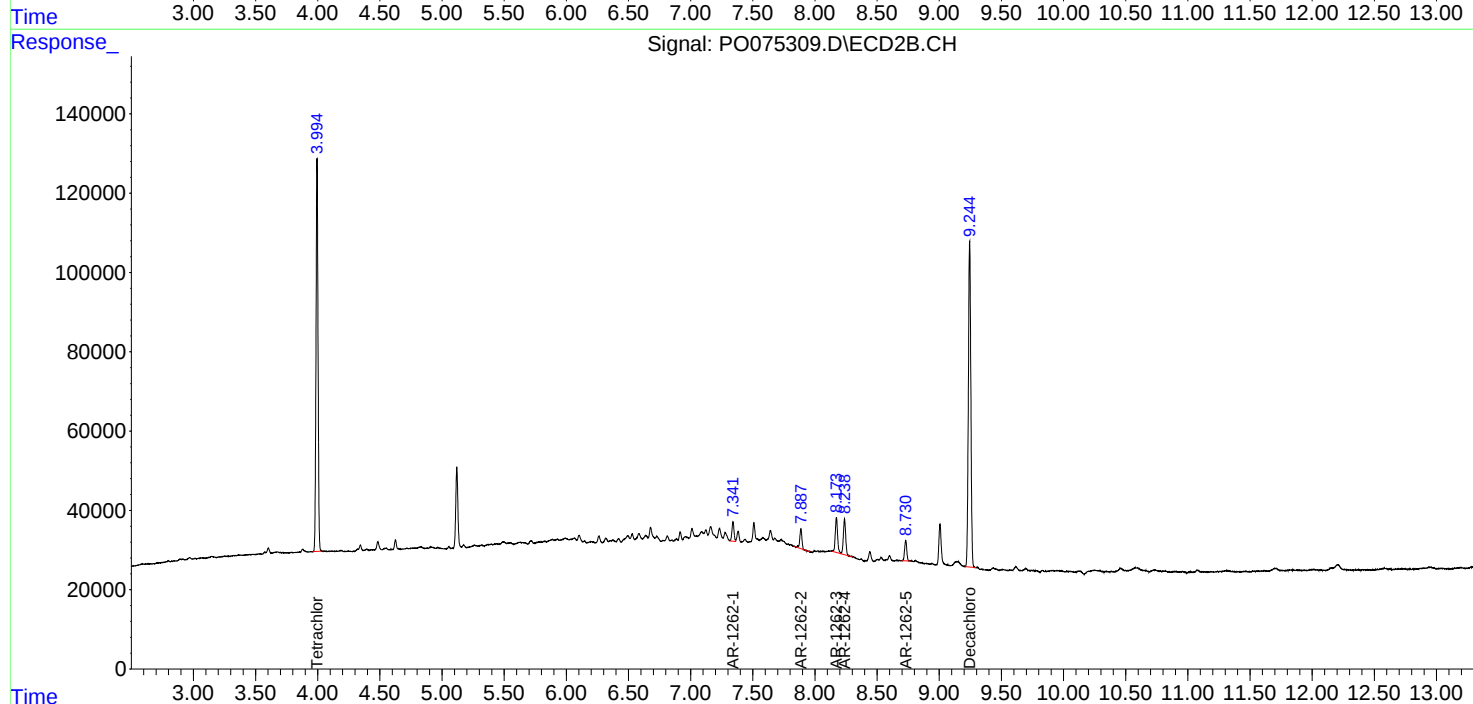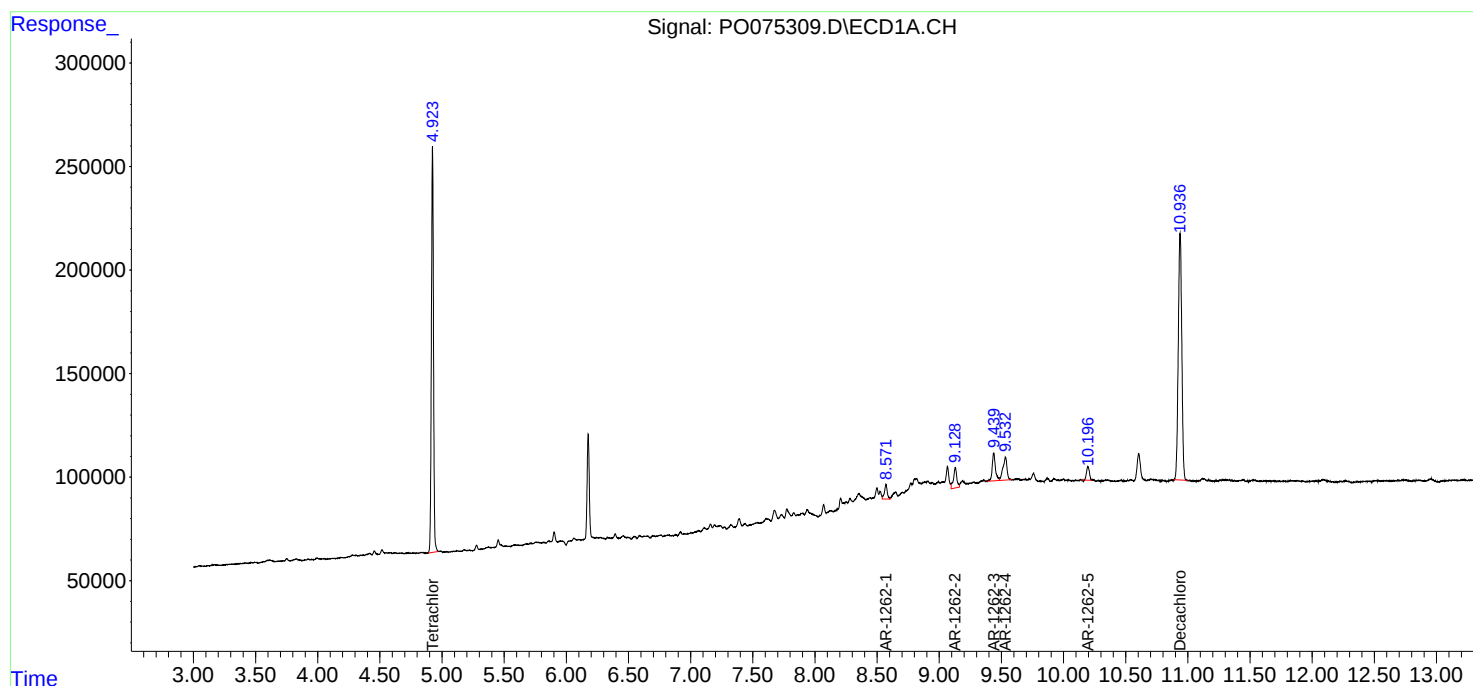

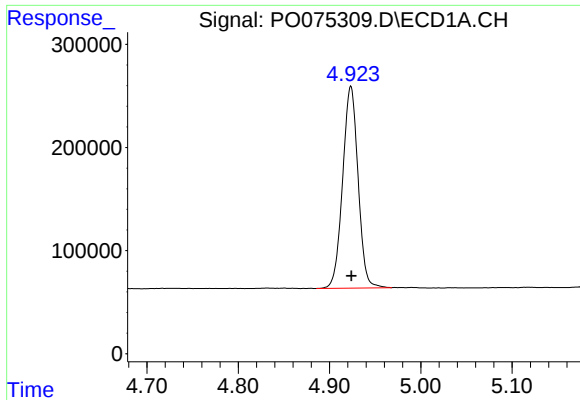


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 2302646
Conc: 22.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-018-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:38 PM

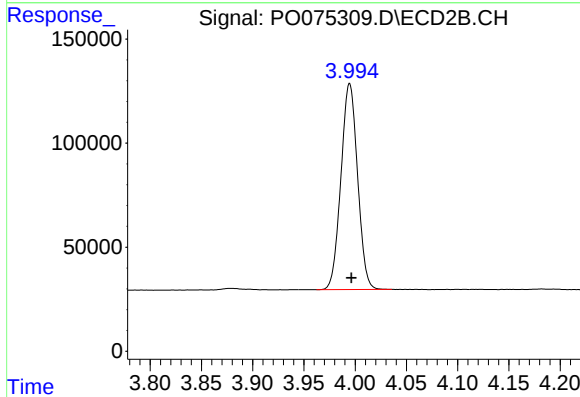


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.002 min
Response: 1115606
Conc: 23.21 ng/ml

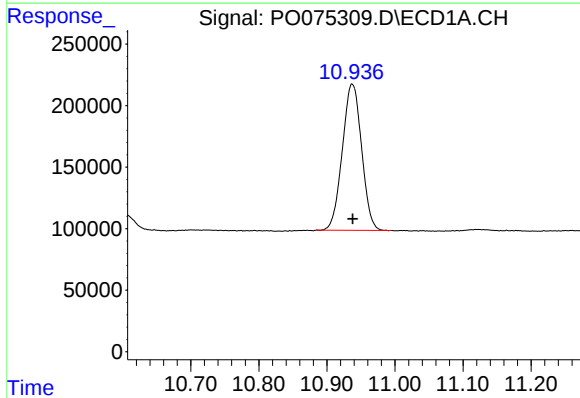


#2 Decachlorobiphenyl

R.T.: 10.937 min
Delta R.T.: 0.000 min
Response: 2338672
Conc: 24.25 ng/ml

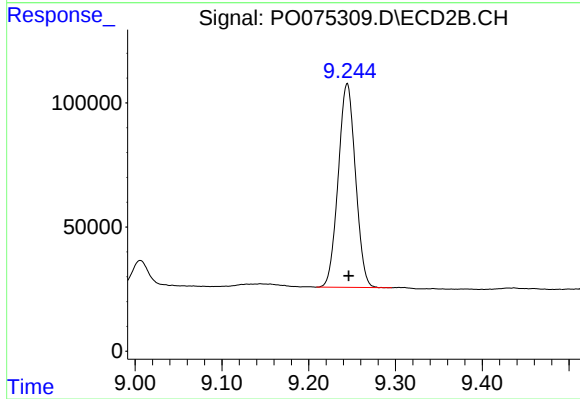

#2 Decachlorobiphenyl

R.T.: 9.244 min
Delta R.T.: -0.002 min
Response: 1134615
Conc: 23.39 ng/ml

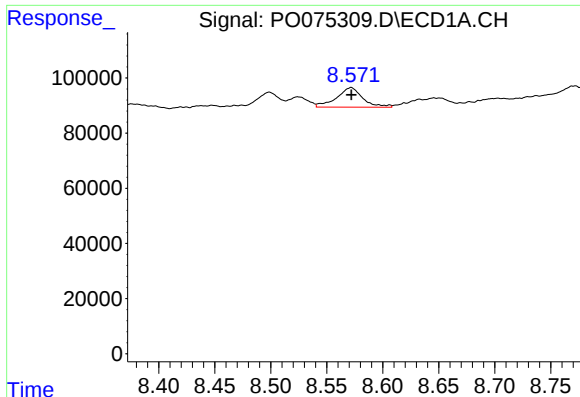


#36 AR-1262-1

R.T.: 8.571 min
Delta R.T.: 0.000 min
Response: 115005
Conc: 13.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
250EM-018-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:38 PM

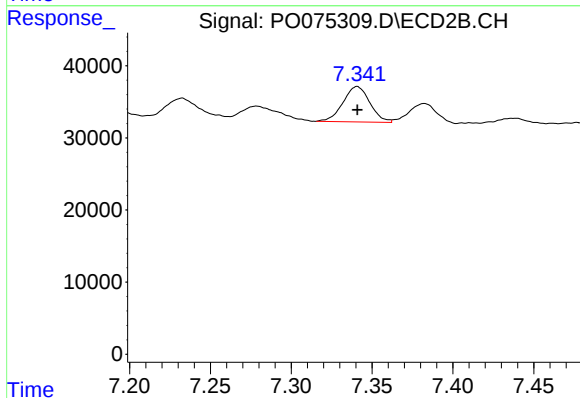


#36 AR-1262-1

R.T.: 7.341 min
Delta R.T.: 0.000 min
Response: 56790
Conc: 26.04 ng/ml

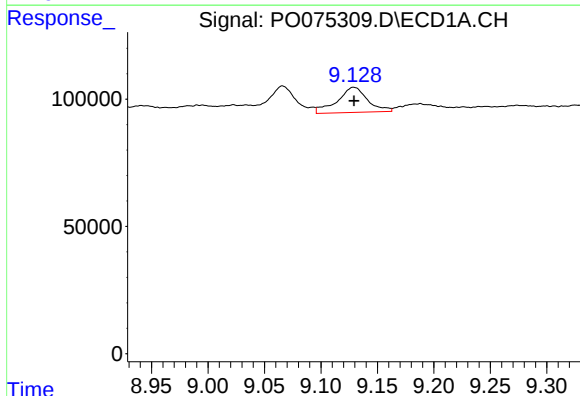


#37 AR-1262-2

R.T.: 9.129 min
Delta R.T.: 0.000 min
Response: 184618
Conc: 12.21 ng/ml

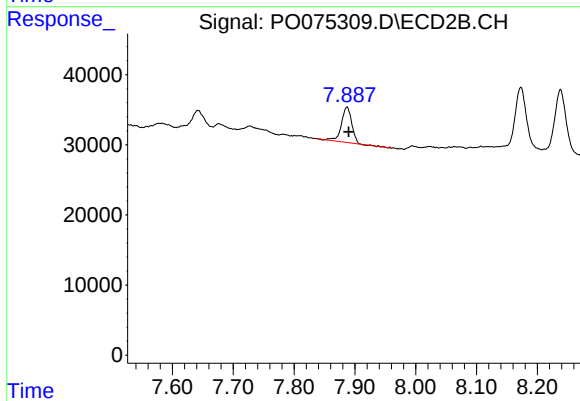

#37 AR-1262-2

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 61285
Conc: 7.99 ng/ml

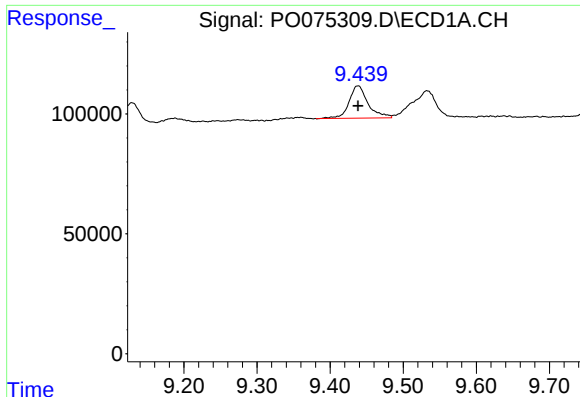


#38 AR-1262-3

R.T.: 9.438 min
Delta R.T.: 0.000 min
Response: 242215
Conc: 23.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-018-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:38 PM

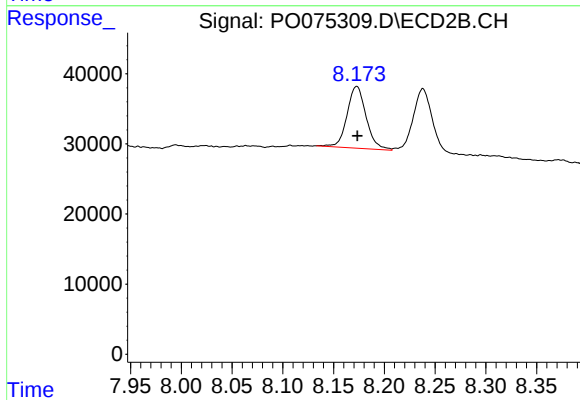


#38 AR-1262-3

R.T.: 8.173 min
Delta R.T.: 0.000 min
Response: 114982
Conc: 34.74 ng/ml

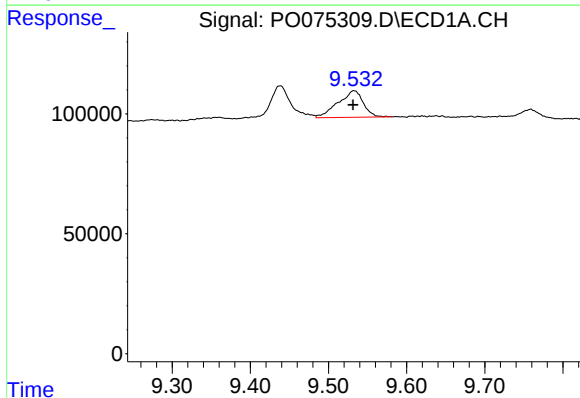


#39 AR-1262-4

R.T.: 9.533 min
Delta R.T.: 0.001 min
Response: 248535
Conc: 33.63 ng/ml

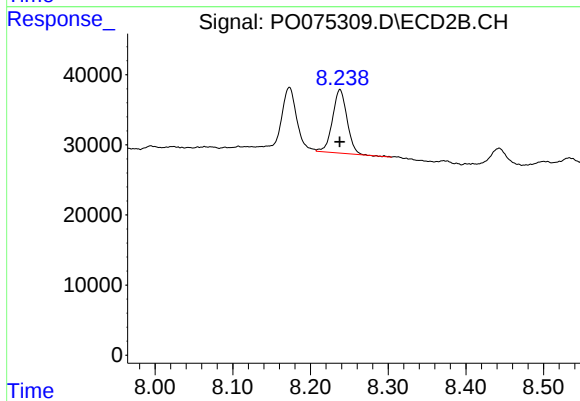

#39 AR-1262-4

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 117552
Conc: 20.47 ng/ml

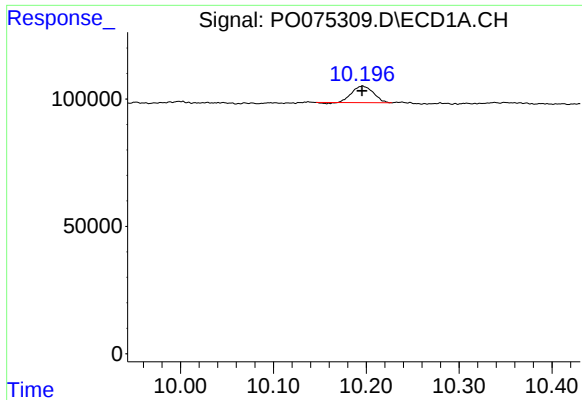


#40 AR-1262-5

R.T.: 10.196 min
Delta R.T.: 0.000 min
Response: 103569
Conc: 19.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-018-0002

Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:38 PM

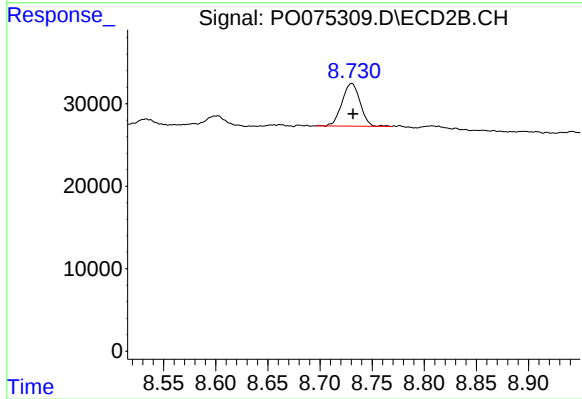

#40 AR-1262-5

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 62486
Conc: 22.71 ng/ml