

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012821\
 Data File : P0075312.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2021 5:27
 Operator : AJ/MA
 Sample : M1247-11
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 250EM-020-0002

Manual Integrations
 APPROVED

Ankita
 1/29/2021 1:13:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 08:07:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 07:43:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.997	2155126	1067636	21.295	22.214
2) SA Decachlor...	10.939	9.246	2320178	1176458	24.063	24.248
Target Compounds						
36) L8 AR-1262-1	8.574	7.343	202435	24995	23.198	11.459 #
37) L8 AR-1262-2	9.131	7.889	238709	113166	15.786	14.756
38) L8 AR-1262-3	9.440	8.174	439897	246927	42.108	74.616m#
39) L8 AR-1262-4	9.535	8.239	453508	245905	61.358	42.827 #
40) L8 AR-1262-5	10.198	8.732	280114	158393	54.014	57.579

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012821\
Data File : P0075312.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2021 5:27
Operator : AJ/MA
Sample : M1247-11
Misc :
ALS Vial : 63 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
250EM-020-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 08:07:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 07:43:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

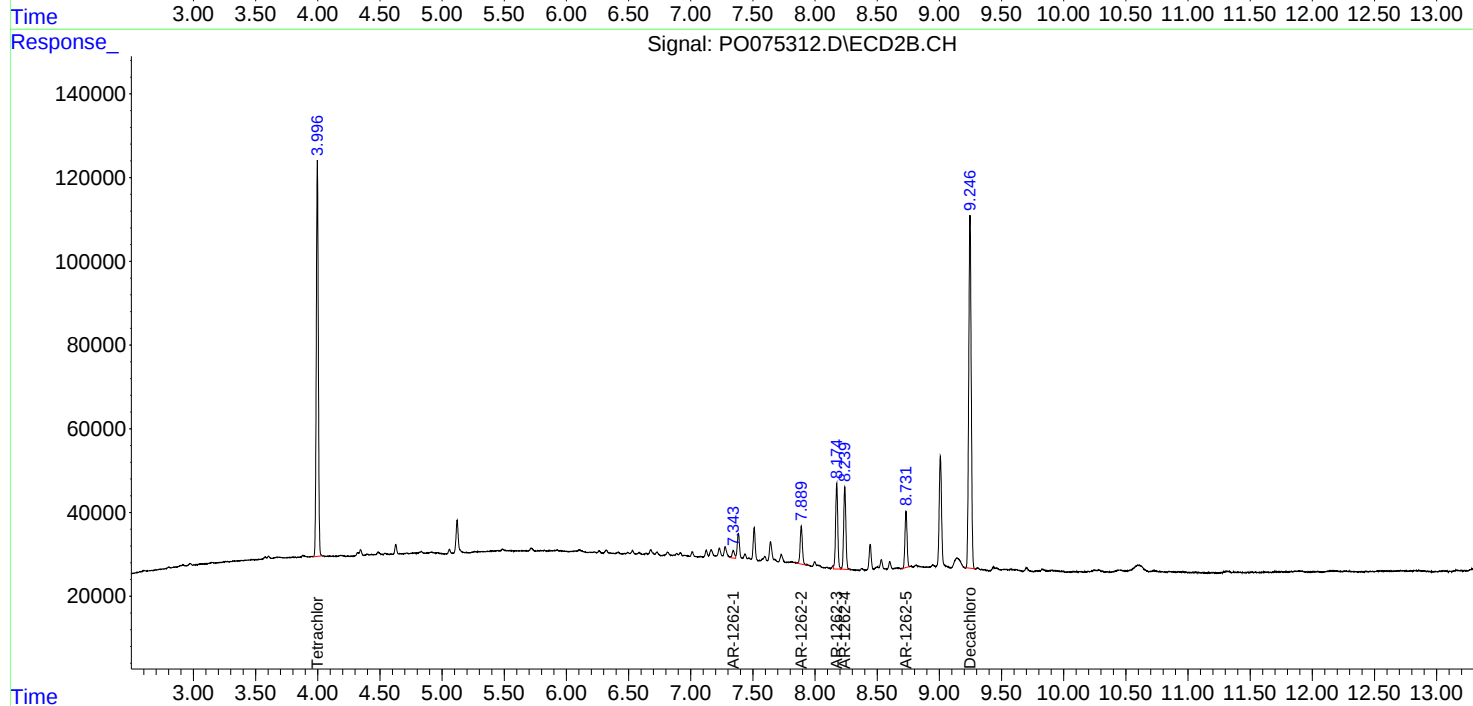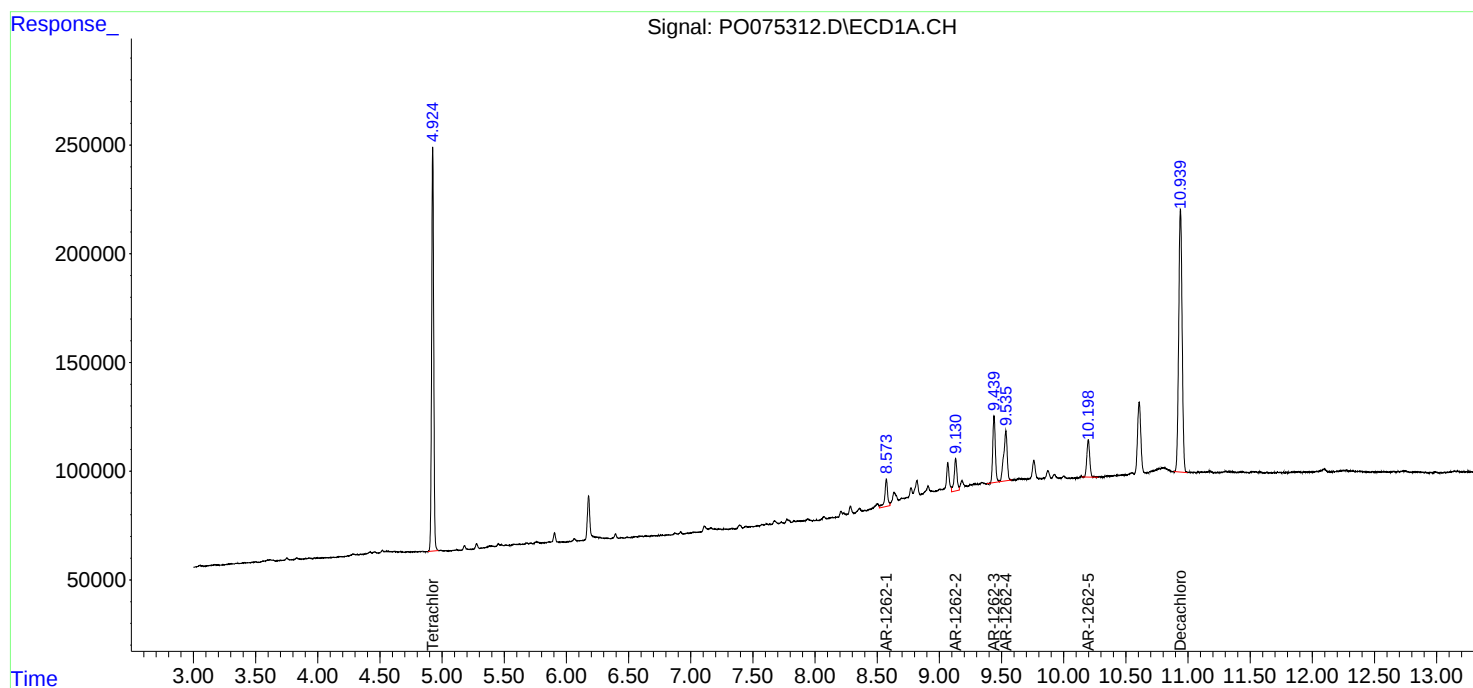

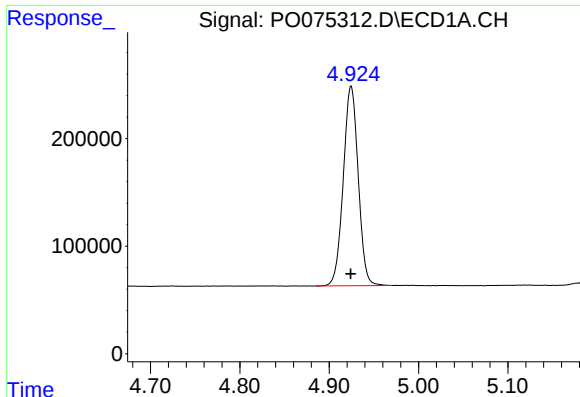


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: 0.000 min
Response: 2155126
Conc: 21.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-020-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:40 PM

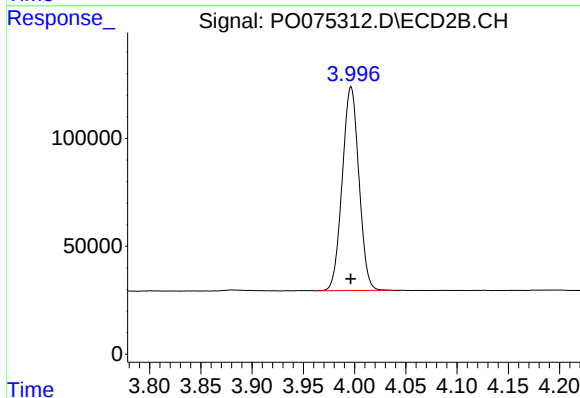


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: 0.000 min
Response: 1067636
Conc: 22.21 ng/ml

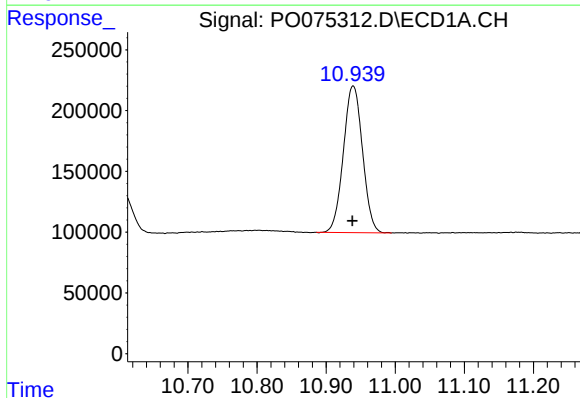


#2 Decachlorobiphenyl

R.T.: 10.939 min
Delta R.T.: 0.001 min
Response: 2320178
Conc: 24.06 ng/ml

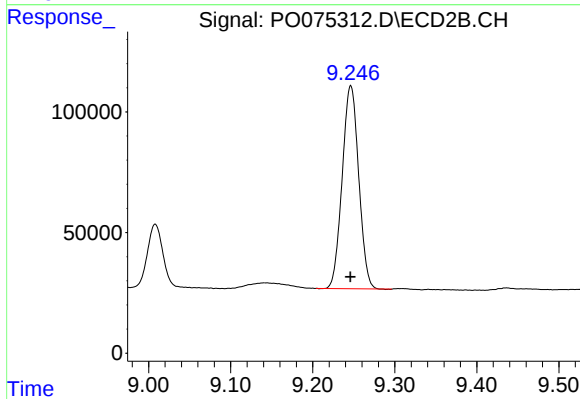

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: 0.000 min
Response: 1176458
Conc: 24.25 ng/ml

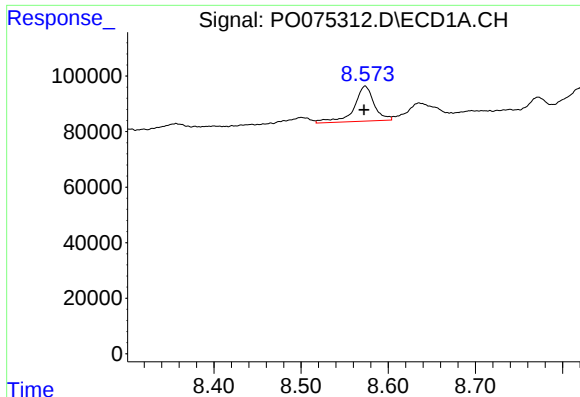


#36 AR-1262-1

R.T.: 8.574 min
Delta R.T.: 0.002 min
Response: 202435
Conc: 23.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-020-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:40 PM

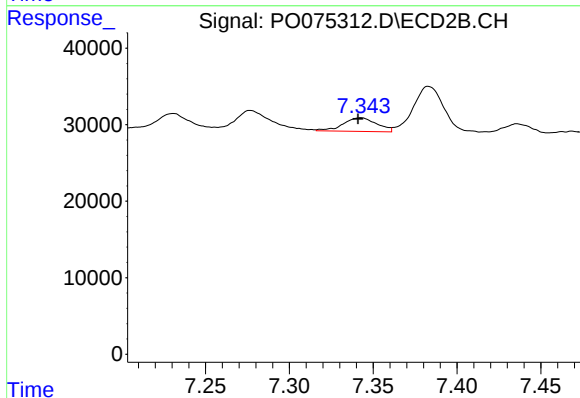


#36 AR-1262-1

R.T.: 7.343 min
Delta R.T.: 0.002 min
Response: 24995
Conc: 11.46 ng/ml

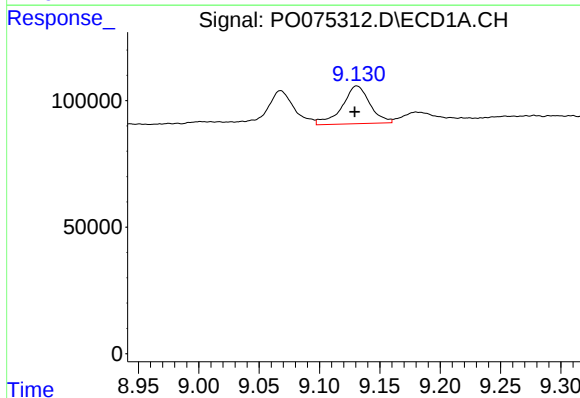


#37 AR-1262-2

R.T.: 9.131 min
Delta R.T.: 0.002 min
Response: 238709
Conc: 15.79 ng/ml

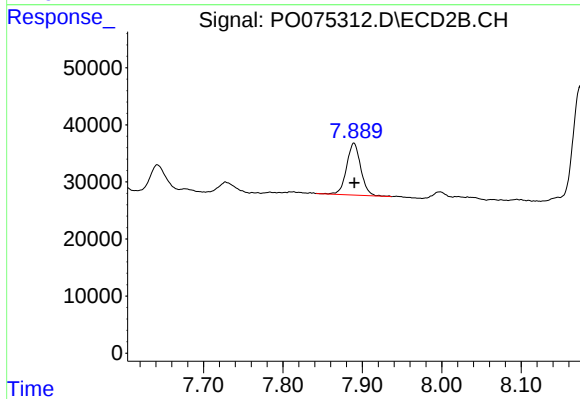

#37 AR-1262-2

R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 113166
Conc: 14.76 ng/ml

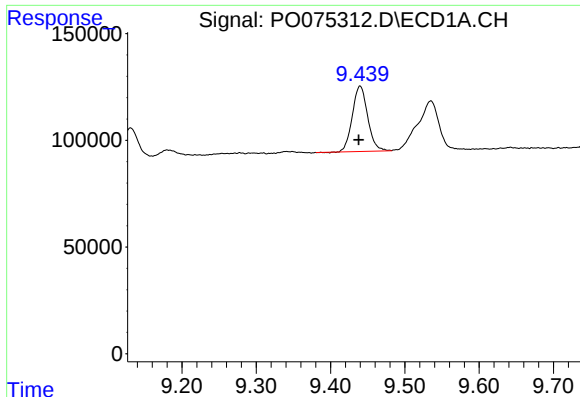


#38 AR-1262-3

R.T.: 9.440 min
Delta R.T.: 0.002 min
Response: 439897
Conc: 42.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-020-0002


Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:40 PM

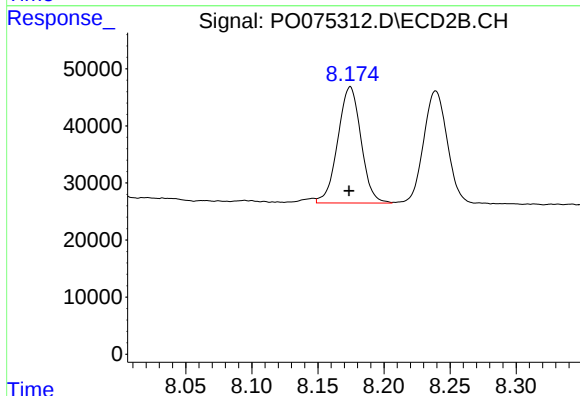


#38 AR-1262-3

R.T.: 8.174 min
Delta R.T.: 0.000 min
Response: 246927
Conc: 74.62 ng/ml m

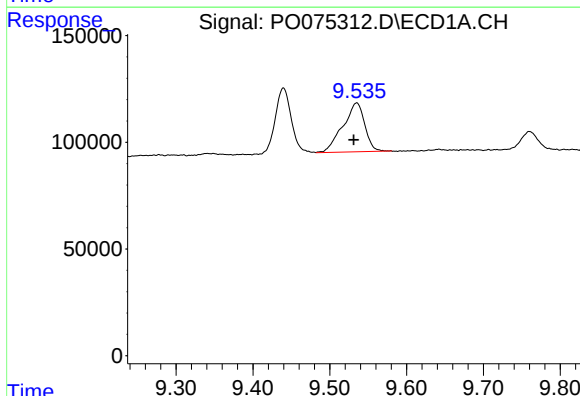


#39 AR-1262-4

R.T.: 9.535 min
Delta R.T.: 0.004 min
Response: 453508
Conc: 61.36 ng/ml

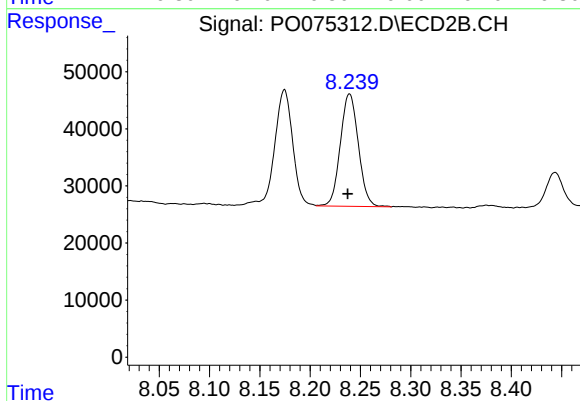

#39 AR-1262-4

R.T.: 8.239 min
Delta R.T.: 0.002 min
Response: 245905
Conc: 42.83 ng/ml

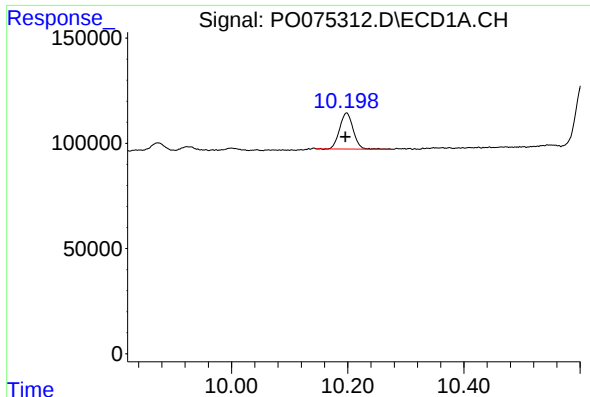


#40 AR-1262-5

R.T.: 10.198 min
Delta R.T.: 0.002 min
Response: 280114
Conc: 54.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-020-0002

Manual Integrations
APPROVED

Ankita
1/29/2021 1:13:40 PM

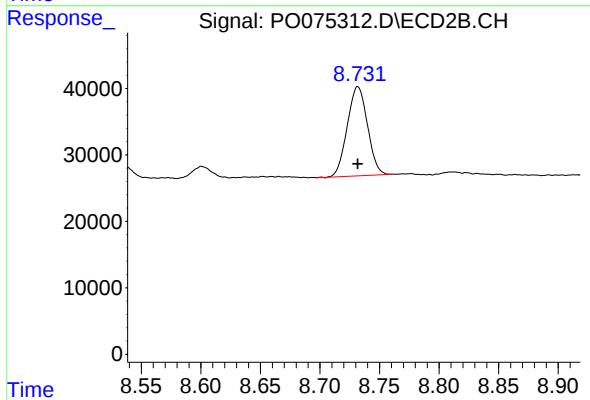

#40 AR-1262-5

R.T.: 8.732 min
Delta R.T.: 0.000 min
Response: 158393
Conc: 57.58 ng/ml