

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012822\
 Data File : P0084456.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2022 13:39
 Operator : AJ\MA
 Sample : N1299-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260791102-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 22:54:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 28 07:54:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.517	5.301	93844	54908	1.628m	2.948m#
2) SA Decachlor...	13.748	11.299	186886	50487	2.228	1.750m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012822\
Data File : P0084456.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2022 13:39
Operator : AJ\MA
Sample : N1299-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC260791102-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 22:54:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012622.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 28 07:54:18 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

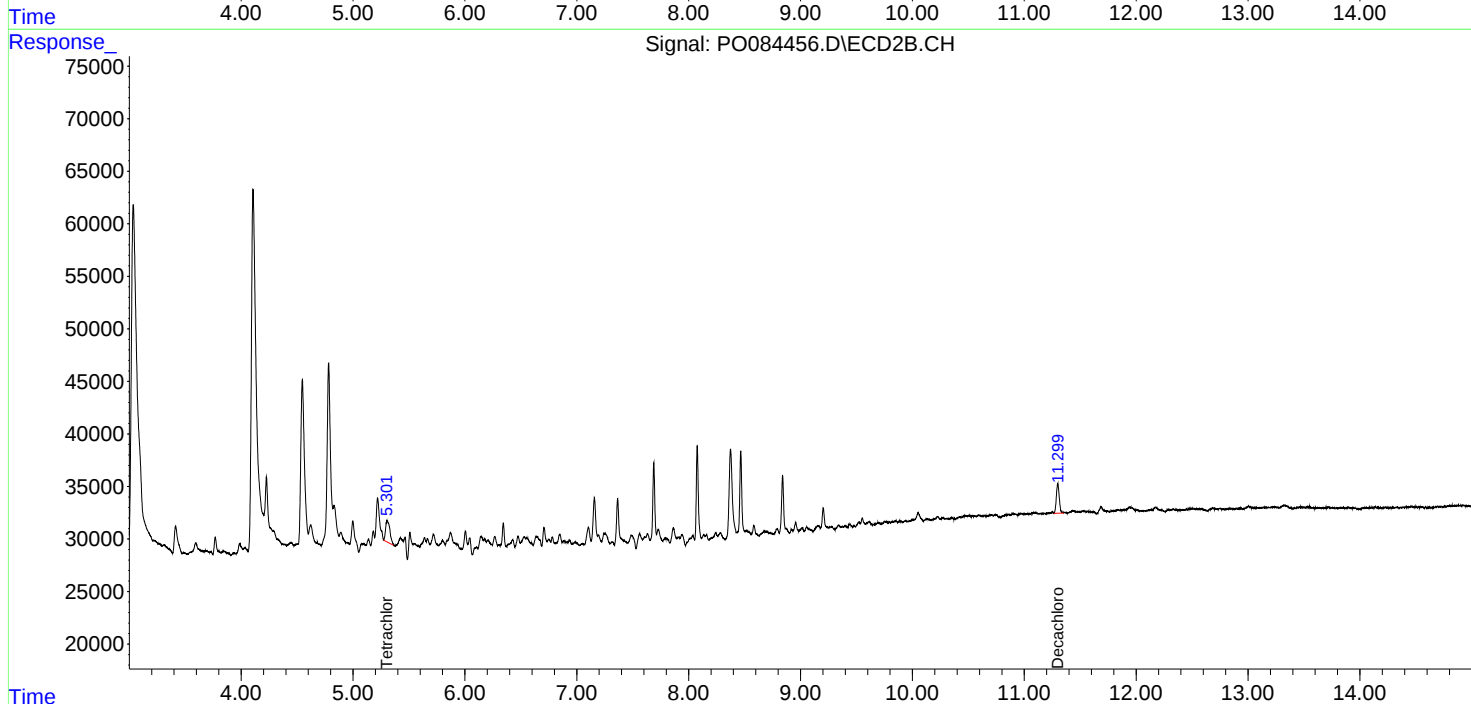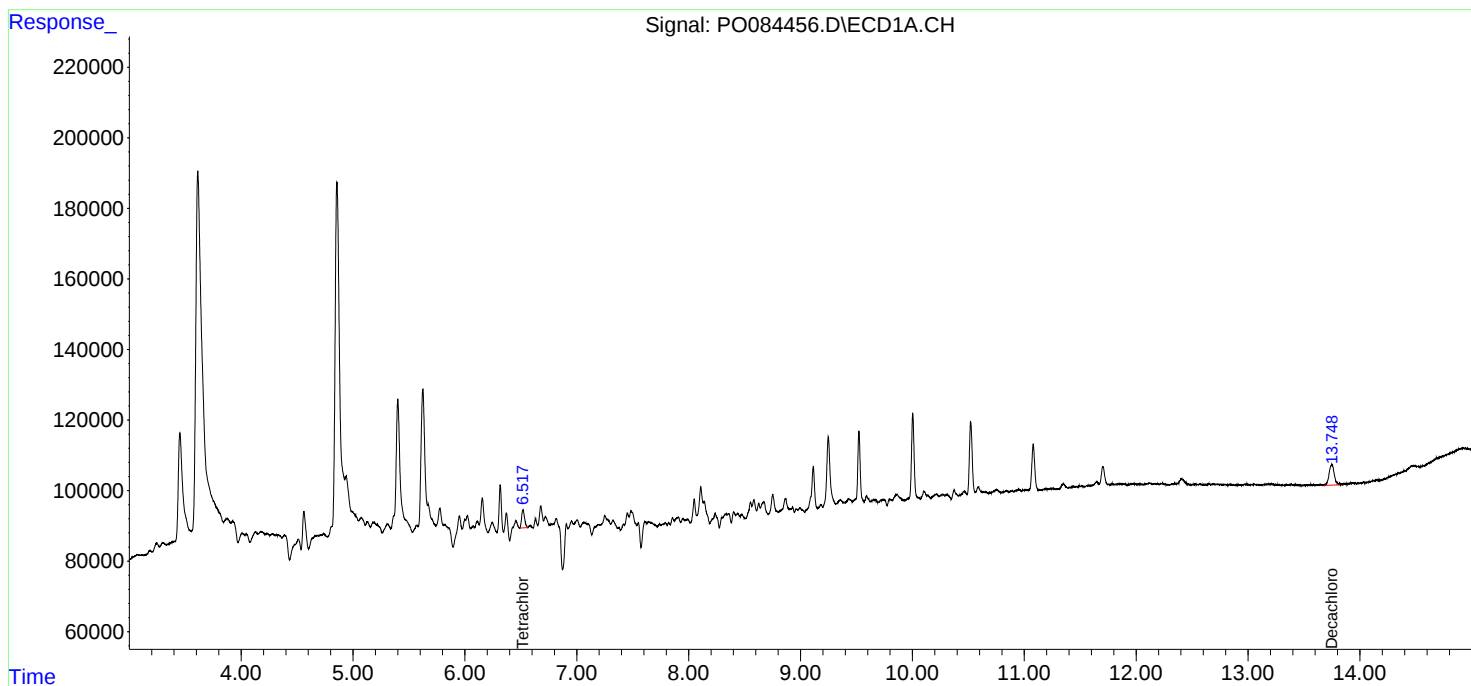


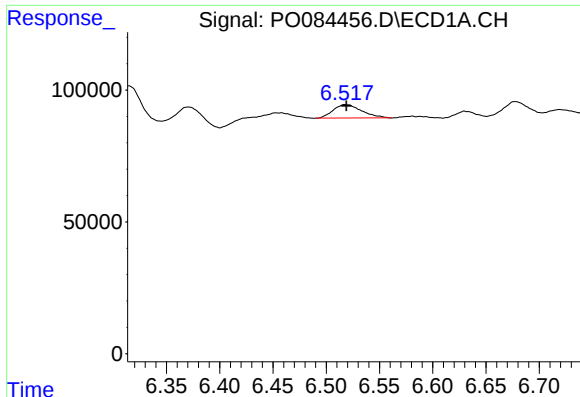

#1 Tetrachloro-m-xylene


R.T.: 6.517 min
Delta R.T.: -0.002 min
Response: 93844
Conc: 1.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260791102-END-1-1

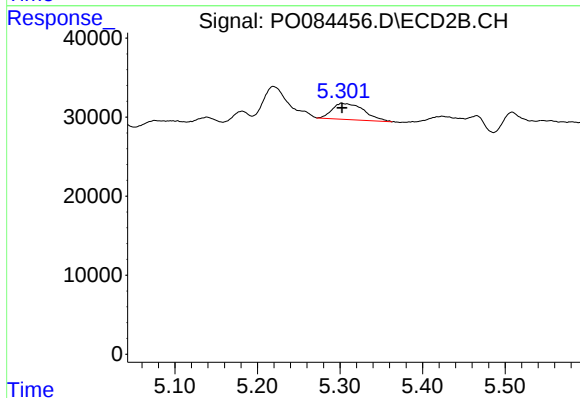


#1 Tetrachloro-m-xylene

R.T.: 5.301 min
Delta R.T.: -0.002 min
Response: 54908
Conc: 2.95 ng/ml m

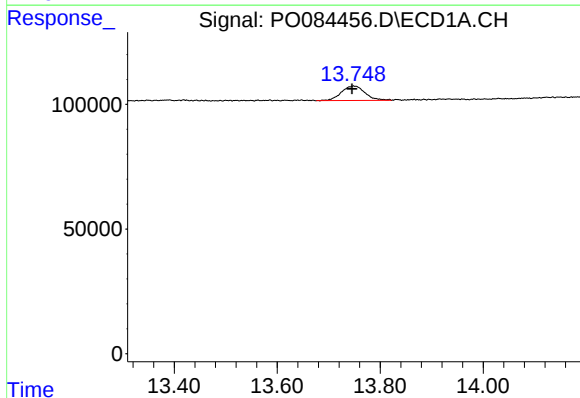

#2 Decachlorobiphenyl

R.T.: 13.748 min
Delta R.T.: 0.003 min
Response: 186886
Conc: 2.23 ng/ml

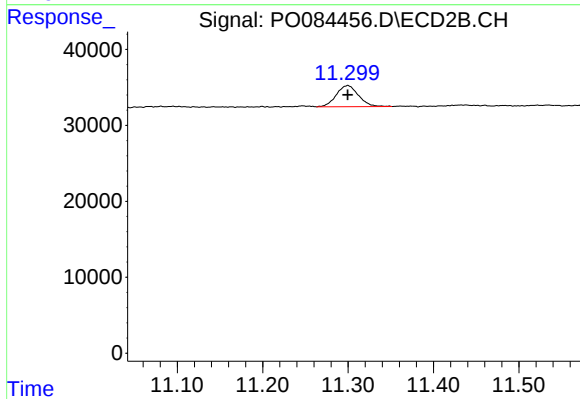

#2 Decachlorobiphenyl

R.T.: 11.299 min
Delta R.T.: 0.000 min
Response: 50487
Conc: 1.75 ng/ml m