

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012825\
 Data File : P0109171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2025 19:41
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 22:23:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 22 03:46:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.700	3.697	137.8E6	93330347	18.242	17.411
2) SA Decachlor...	8.764	8.714	125.8E6	61642520	18.157	17.926

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012825\
Data File : PO109171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2025 19:41
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 22:23:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 22 03:46:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

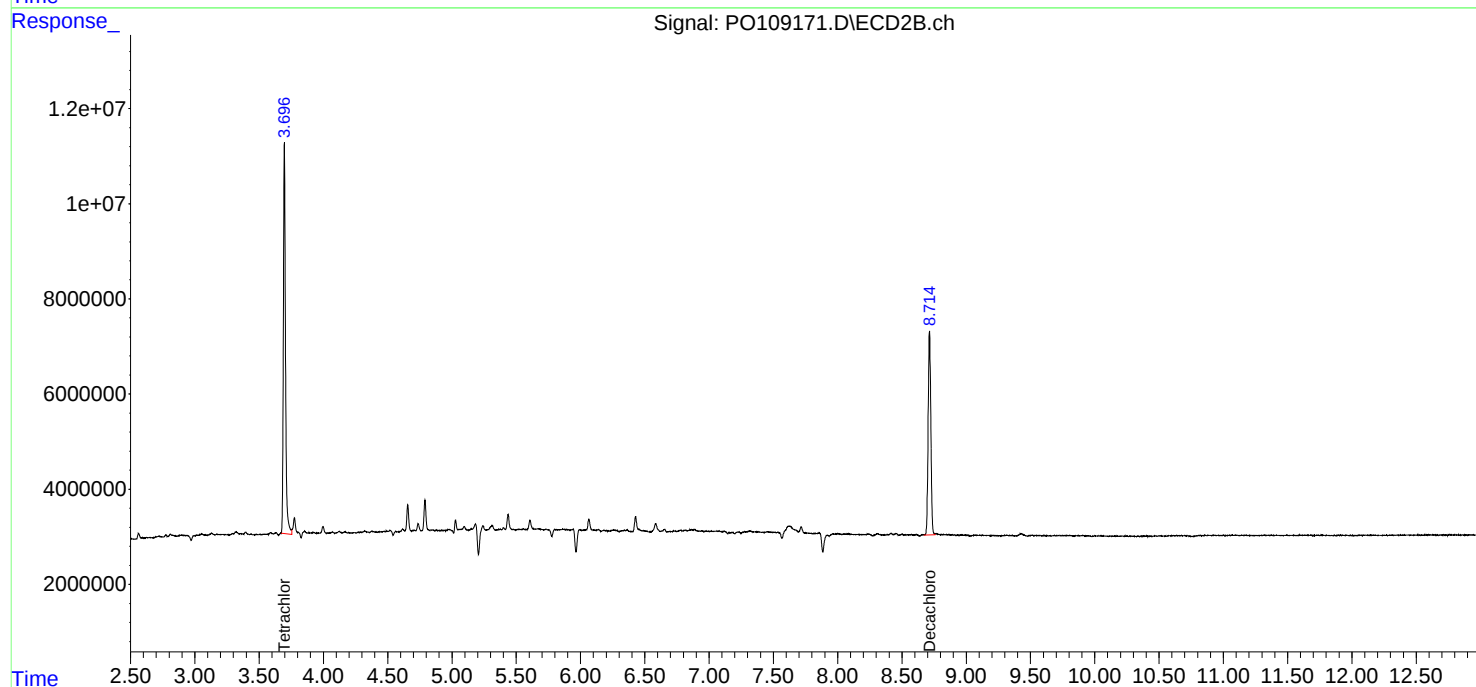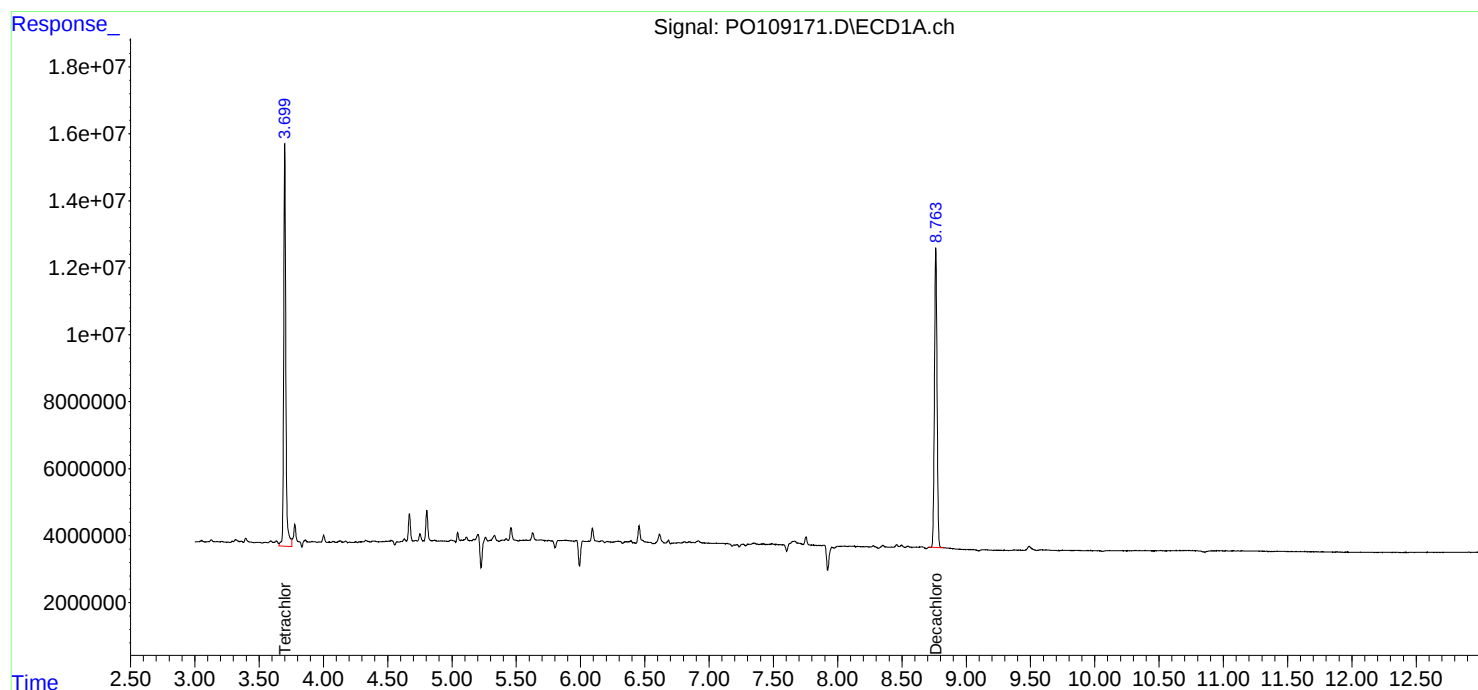


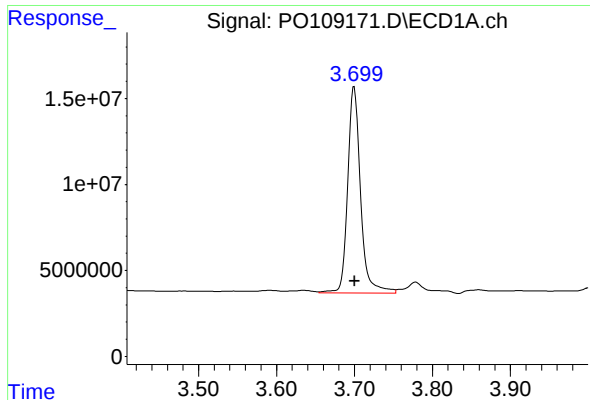

#1 Tetrachloro-m-xylene


R.T.: 3.700 min
Delta R.T.: 0.000 min
Response: 137845324
Conc: 18.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

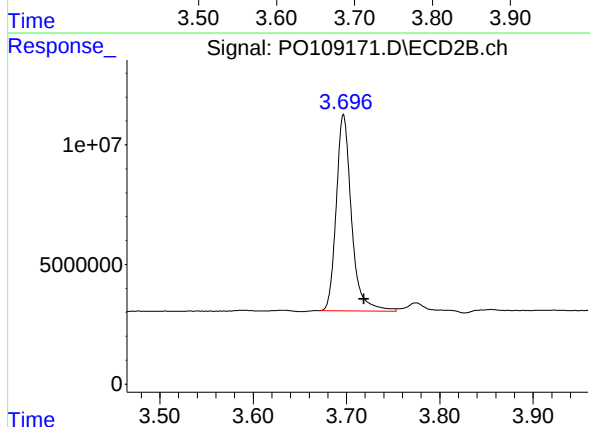


#1 Tetrachloro-m-xylene

R.T.: 3.697 min
Delta R.T.: -0.022 min
Response: 93330347
Conc: 17.41 ng/ml

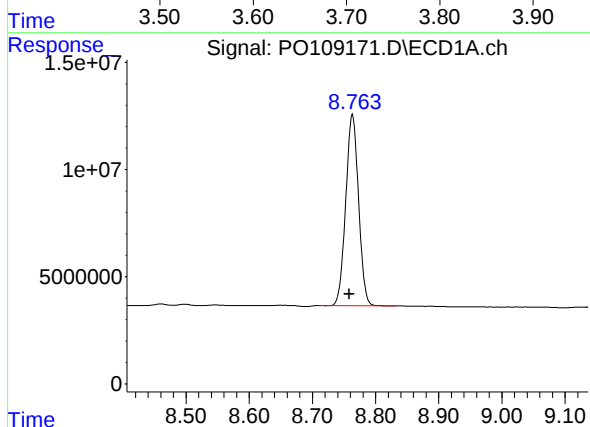

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: 0.005 min
Response: 125788135
Conc: 18.16 ng/ml

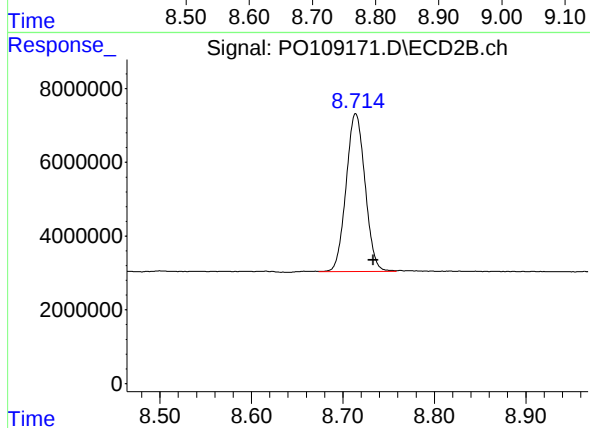

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: -0.019 min
Response: 61642520
Conc: 17.93 ng/ml