

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066124.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 3:50
 Operator : DD\AJ
 Sample : PB126460BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 04:49:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.155	3.433	851340	1135856	29.225	27.769
2)	SA Decachlor...	9.643	8.325	749395	1094678	19.016	18.677
Target Compounds							
5)	L1 AR-1016-3	0.000	4.719	0	15713	N.D.	11.287 #
6)	L1 AR-1016-4	0.000	4.719	0	15713	N.D.	13.601 #
13)	L3 AR-1232-3	0.000	4.719	0	15713	N.D.	28.185 #
14)	L3 AR-1232-4	0.000	4.750	0	5246	N.D.	10.870 #
18)	L4 AR-1242-3	0.000	4.719	0	15713	N.D.	14.783 #
19)	L4 AR-1242-4	0.000	4.750	0	5246	N.D.	5.104 #
22)	L5 AR-1248-2	0.000	4.719	0	15713	N.D.	10.576 #
23)	L5 AR-1248-3	0.000	4.750	0	5246	N.D.	3.509 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
Data File : P0066124.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 3:50
Operator : DD\AJ
Sample : PB126460BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 04:49:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

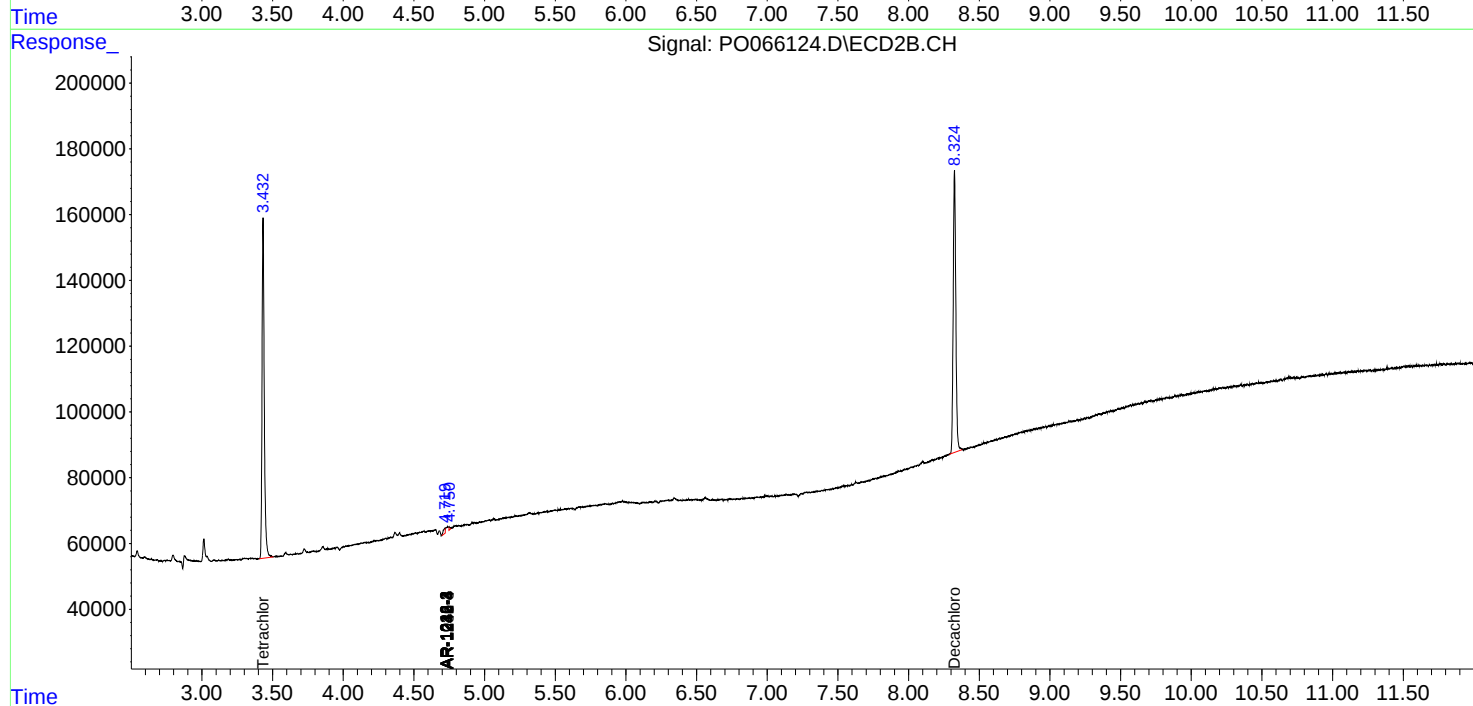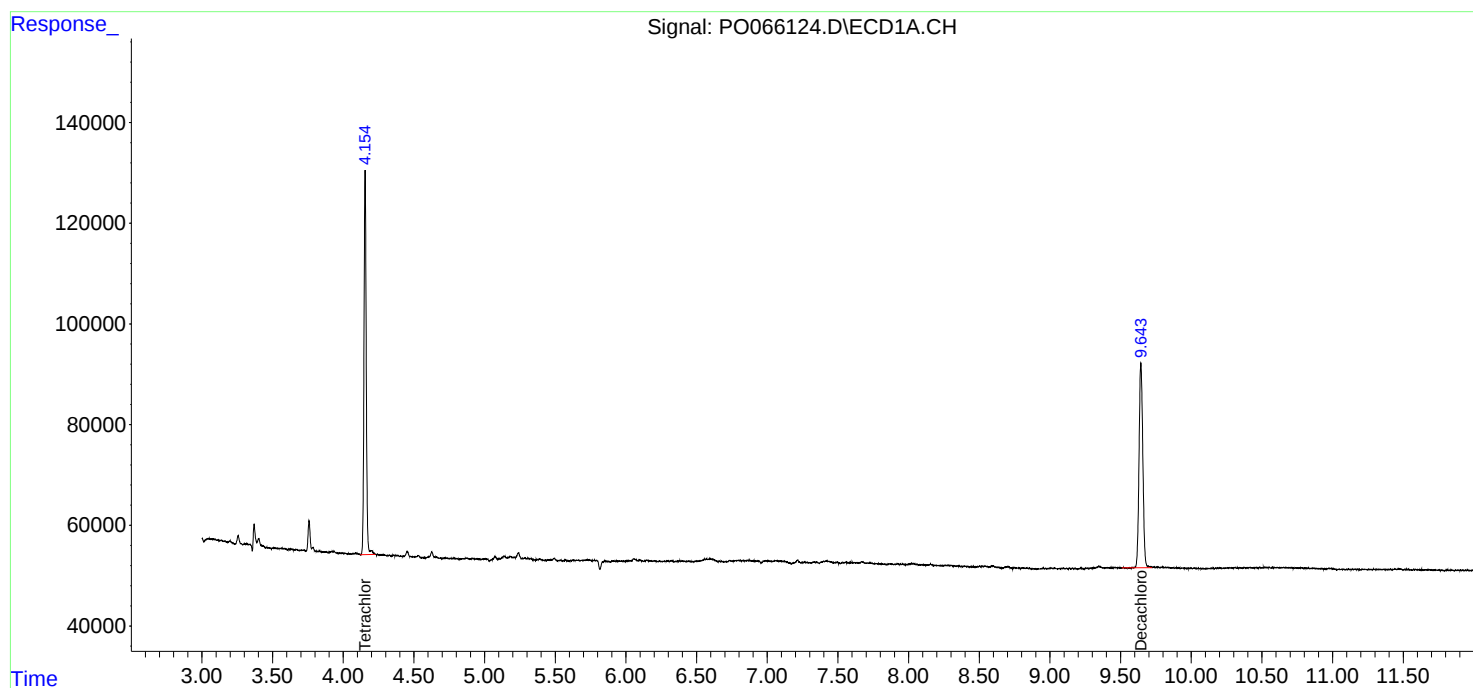


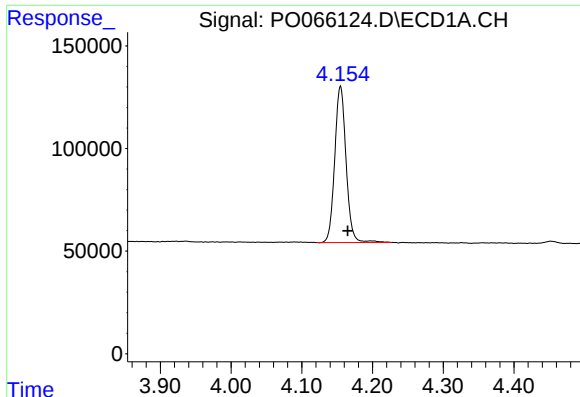

#1 Tetrachloro-m-xylene


R.T.: 4.155 min
Delta R.T.: -0.010 min
Response: 851340
Conc: 29.22 ng/ml

Instrument :
ECD_O
ClientSampleId :

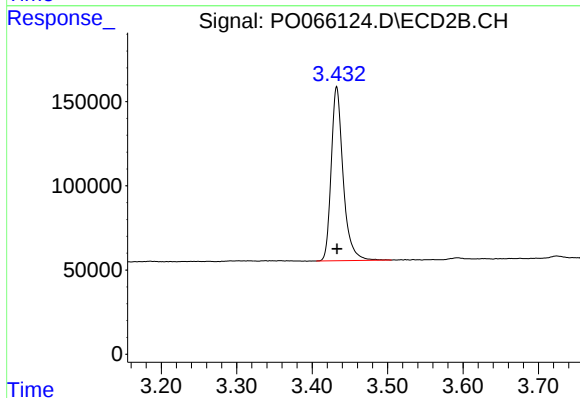


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 1135856
Conc: 27.77 ng/ml

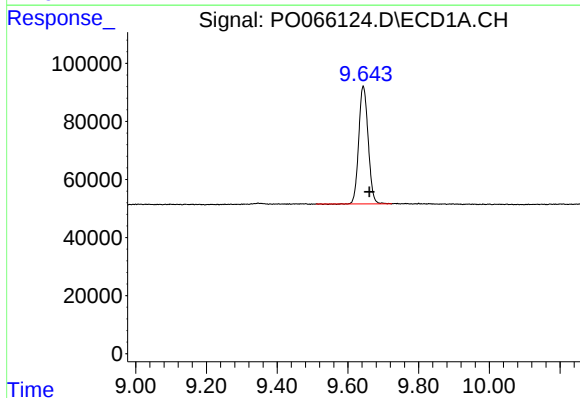


#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.018 min
Response: 749395
Conc: 19.02 ng/ml

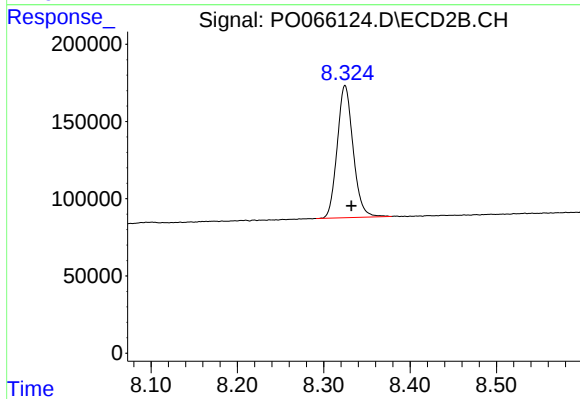

#2 Decachlorobiphenyl


R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 1094678
Conc: 18.68 ng/ml

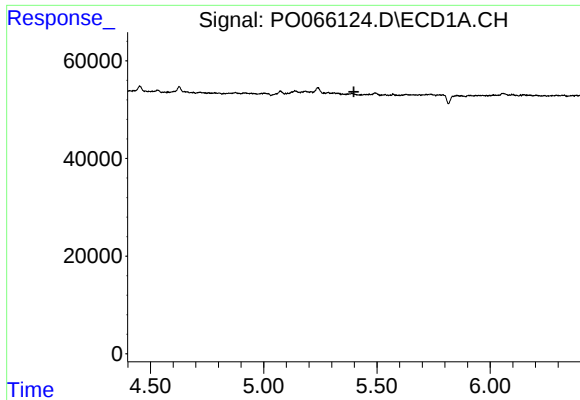

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

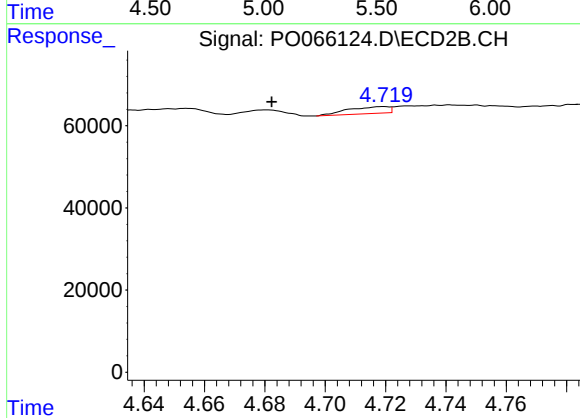


#5 AR-1016-3

R.T.: 4.719 min
Delta R.T.: 0.037 min
Response: 15713
Conc: 11.29 ng/ml

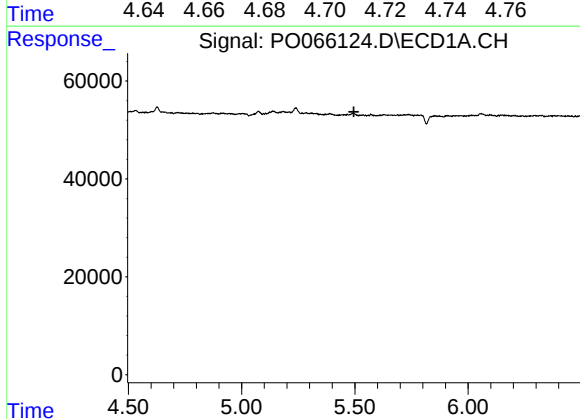


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.495 min
Response: 0
Conc: N.D.

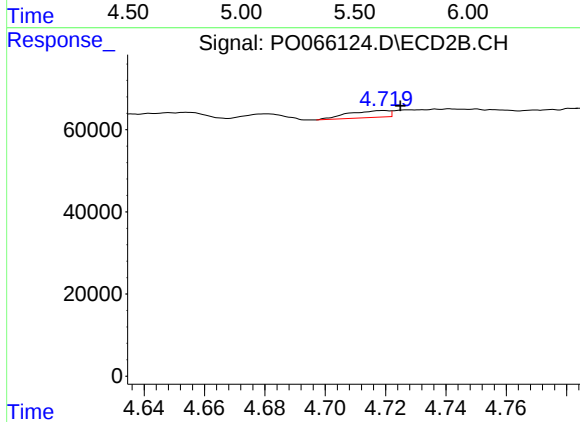

#6 AR-1016-4


R.T.: 4.719 min
Delta R.T.: -0.006 min
Response: 15713
Conc: 13.60 ng/ml

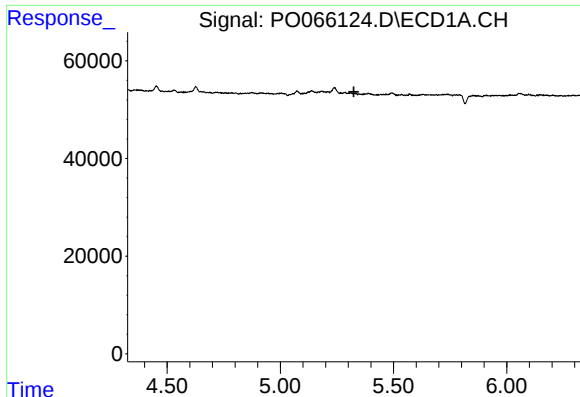

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 5.325 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

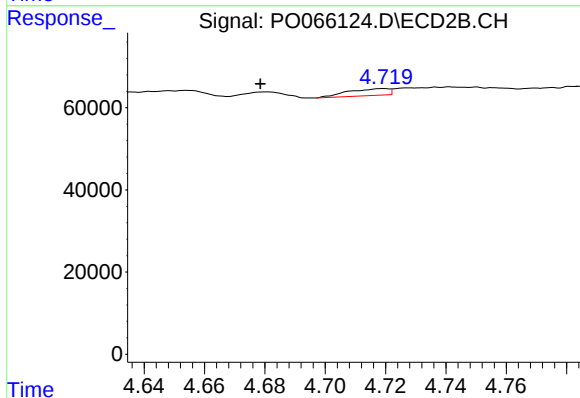


#13 AR-1232-3

R.T.: 4.719 min
Delta R.T.: 0.041 min
Response: 15713
Conc: 28.18 ng/ml

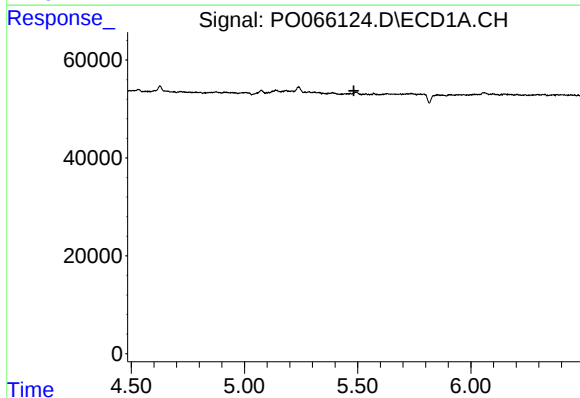


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.483 min
Response: 0
Conc: N.D.

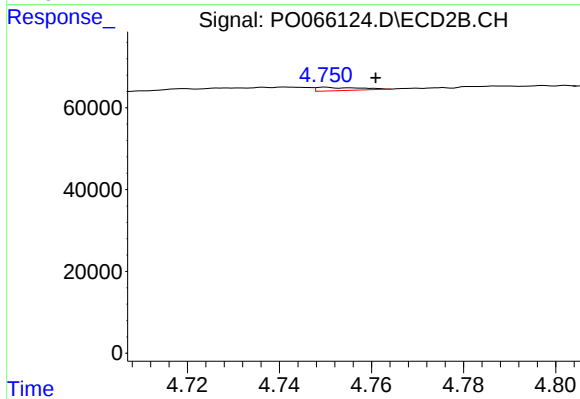

#14 AR-1232-4


R.T.: 4.750 min
Delta R.T.: -0.011 min
Response: 5246
Conc: 10.87 ng/ml

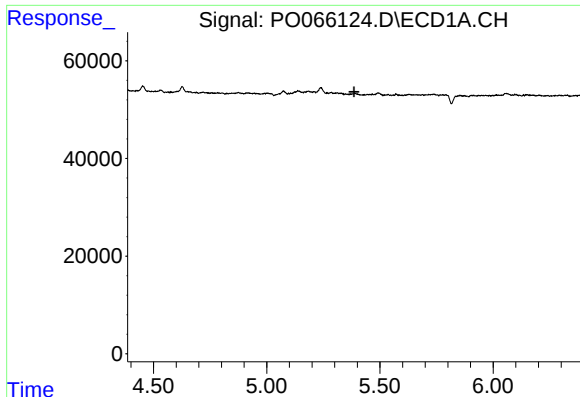

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

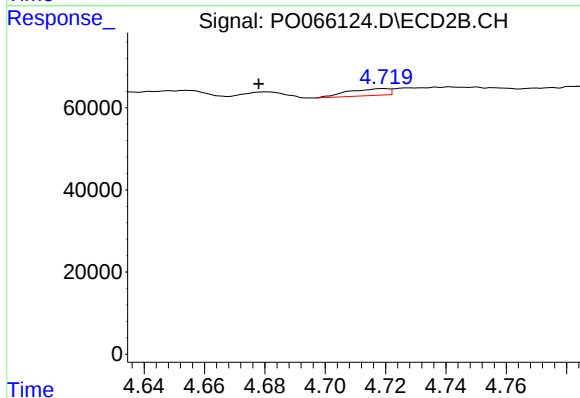


#18 AR-1242-3

R.T.: 4.719 min
Delta R.T.: 0.041 min
Response: 15713
Conc: 14.78 ng/ml

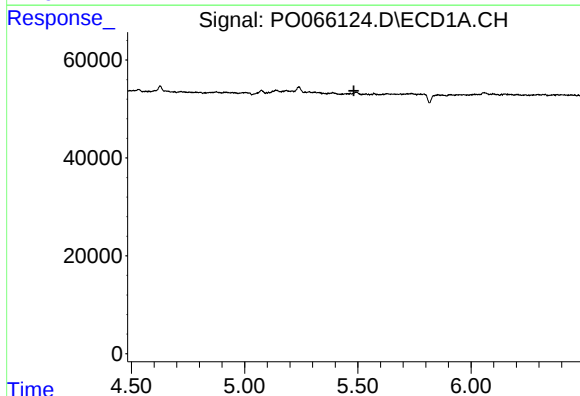


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.482 min
Response: 0
Conc: N.D.

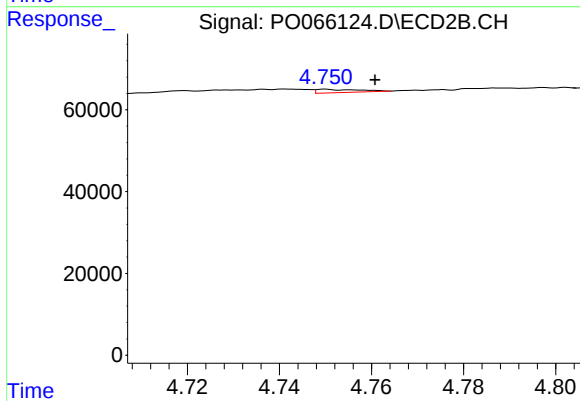

#19 AR-1242-4


R.T.: 4.750 min
Delta R.T.: -0.011 min
Response: 5246
Conc: 5.10 ng/ml

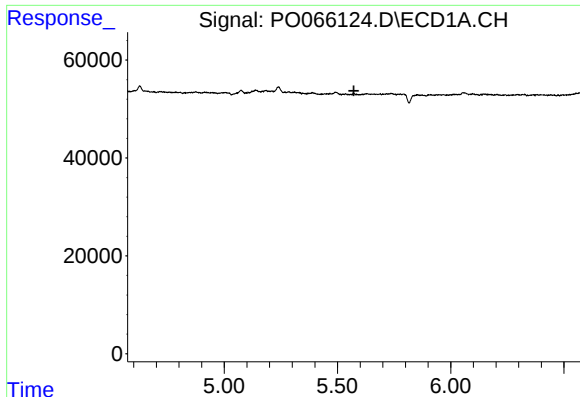

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T.: 5.572 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

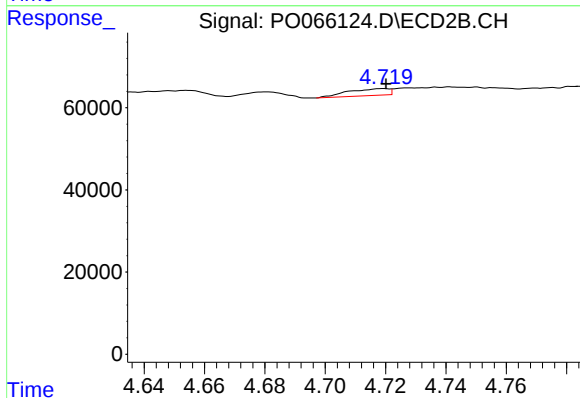


#22 AR-1248-2

R.T.: 4.719 min
Delta R.T.: 0.000 min
Response: 15713
Conc: 10.58 ng/ml

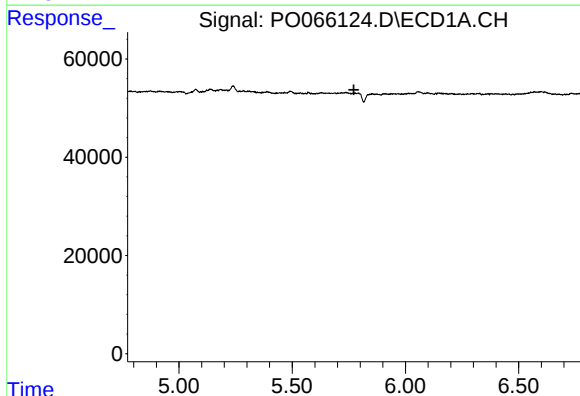

#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.772 min
Response: 0
Conc: N.D.

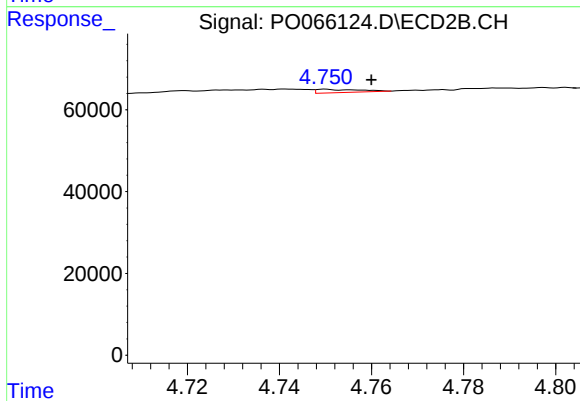

#23 AR-1248-3

R.T.: 4.750 min
Delta R.T.: -0.010 min
Response: 5246
Conc: 3.51 ng/ml