

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066091.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2020 16:22
 Operator : DD\AJ
 Sample : L1255-03RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0073-SITE-WATERRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 16:46:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 30 12:37:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.156	3.433	975347	1363178	33.482	33.326
2) SA Decachlor...	9.646	8.327	825278	1203258	20.942	20.530

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
Data File : P0066091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2020 16:22
Operator : DD\AJ
Sample : L1255-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0073-SITE-WATERRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 16:46:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 30 12:37:11 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

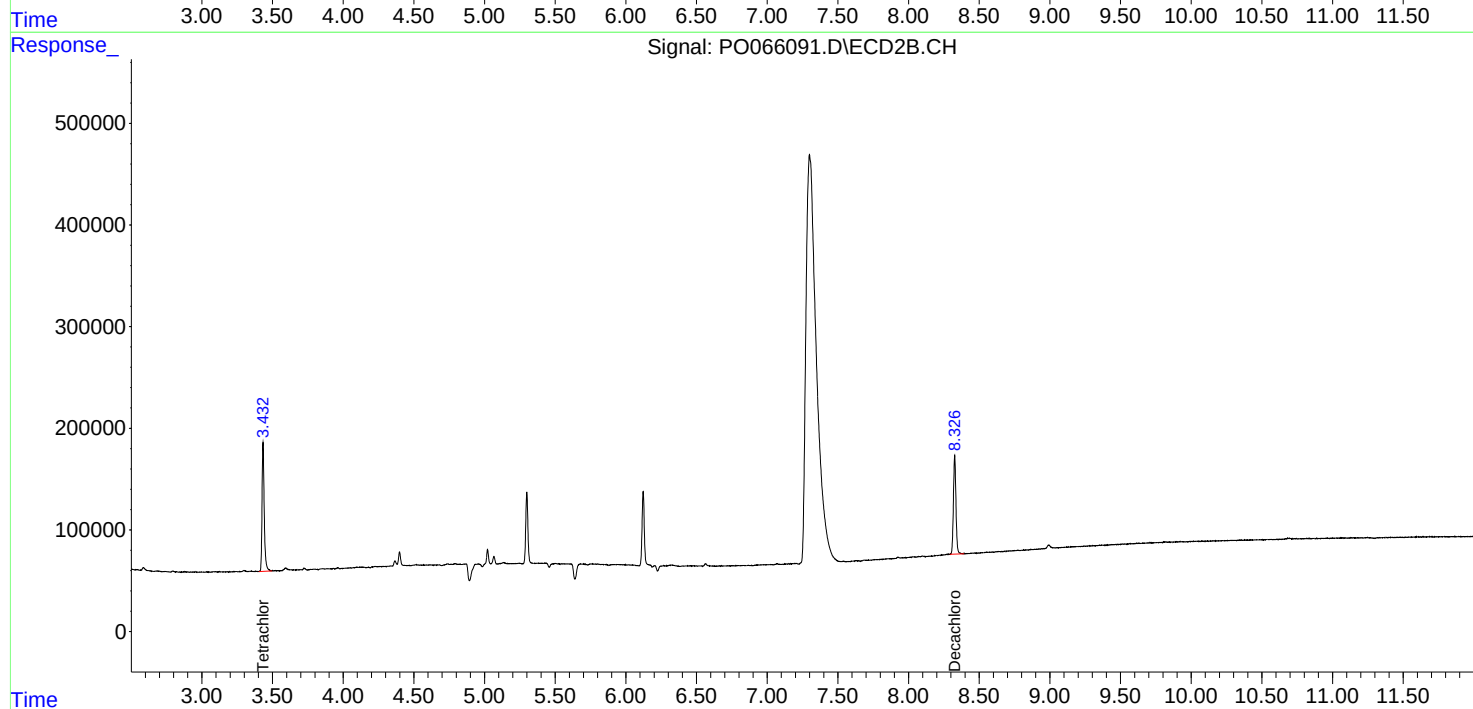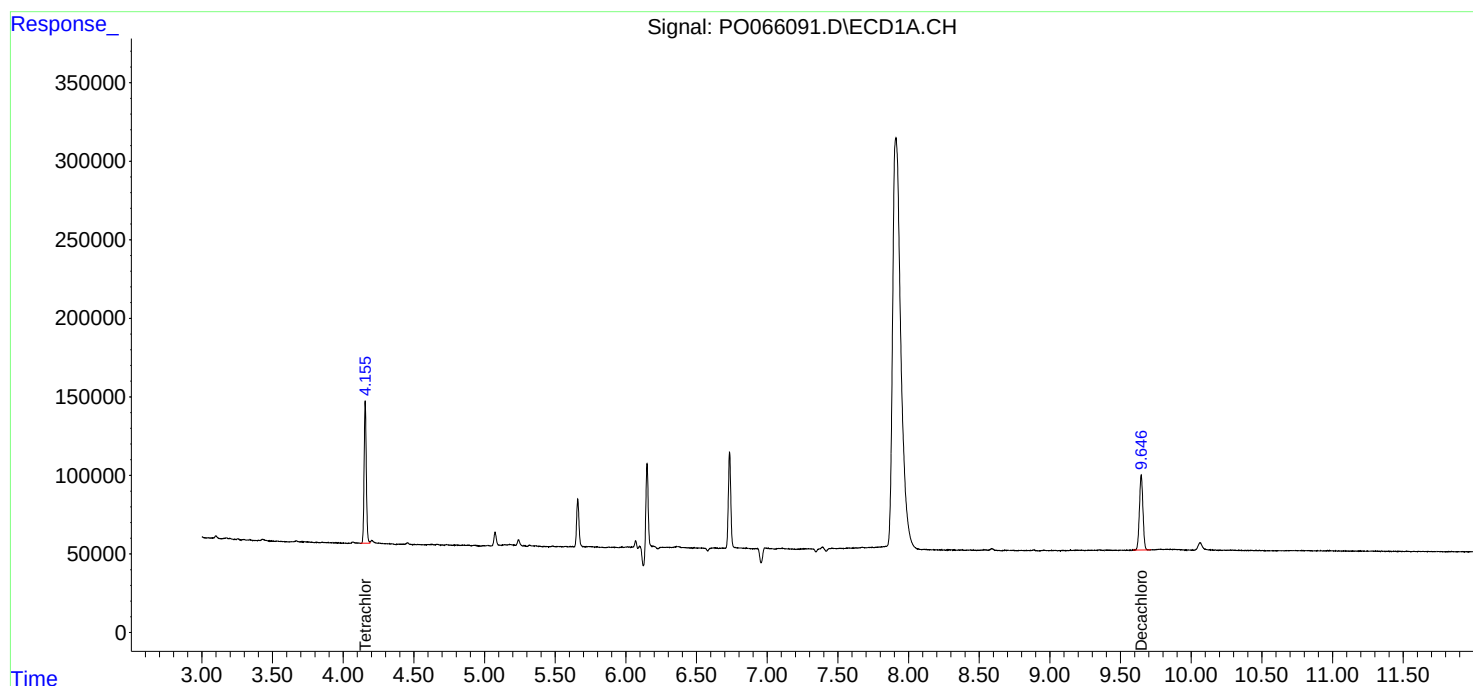


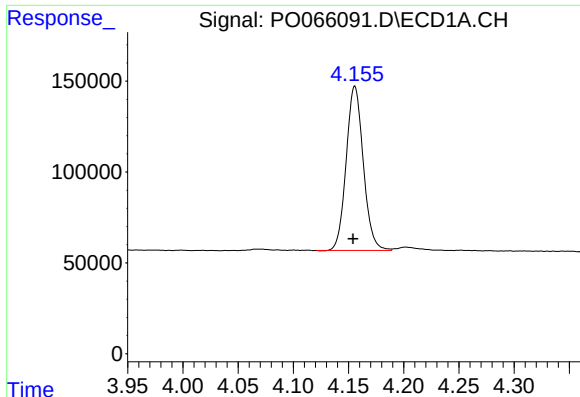

#1 Tetrachloro-m-xylene


R.T.: 4.156 min
Delta R.T.: 0.002 min
Response: 975347
Conc: 33.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
0073-SITE-WATERRE

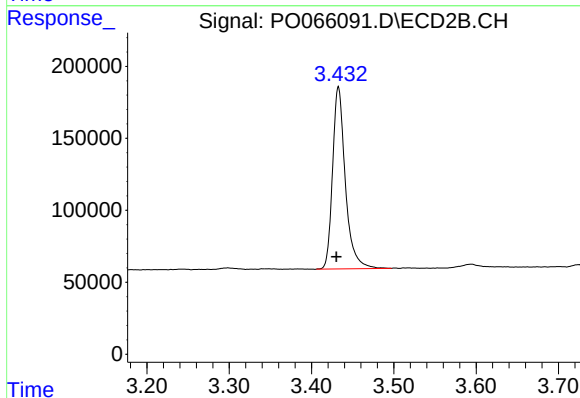


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.002 min
Response: 1363178
Conc: 33.33 ng/ml

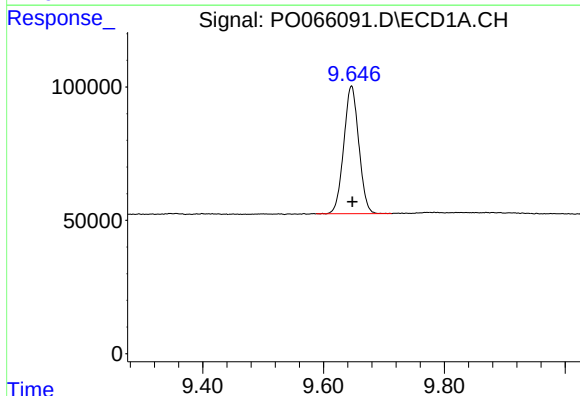

#2 Decachlorobiphenyl

R.T.: 9.646 min
Delta R.T.: -0.002 min
Response: 825278
Conc: 20.94 ng/ml

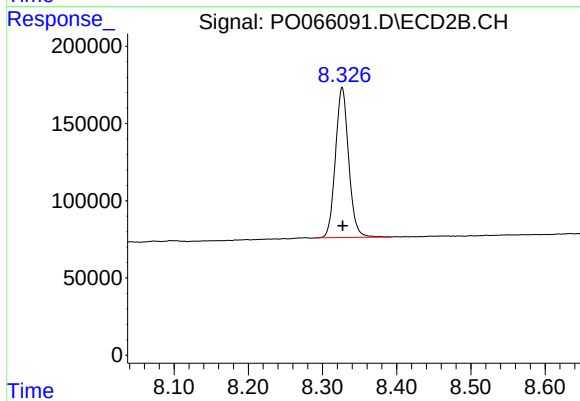

#2 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: 0.000 min
Response: 1203258
Conc: 20.53 ng/ml