

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066096.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2020 17:46
 Operator : DD\AJ
 Sample : L1266-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40652

Manual Integrations
 APPROVED

mohammad
 1/31/2020 2:05:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 02:58:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.434	683453	900785	23.461m	22.022
2) SA Decachlor...	9.647	8.328	969132	1447349	24.592	24.694

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
Data File : P0066096.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2020 17:46
Operator : DD\AJ
Sample : L1266-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
40652


Manual Integrations
APPROVED

mohammad
1/31/2020 2:05:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 02:58:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

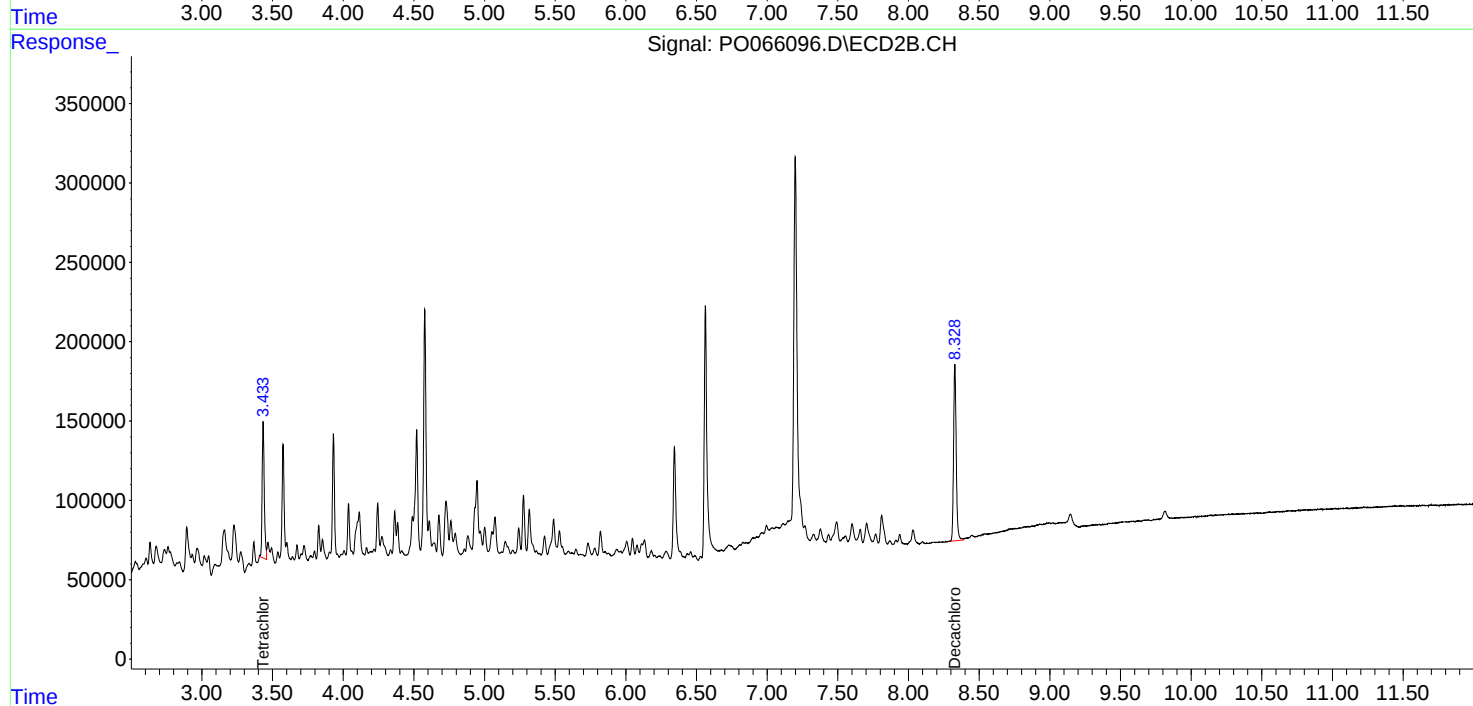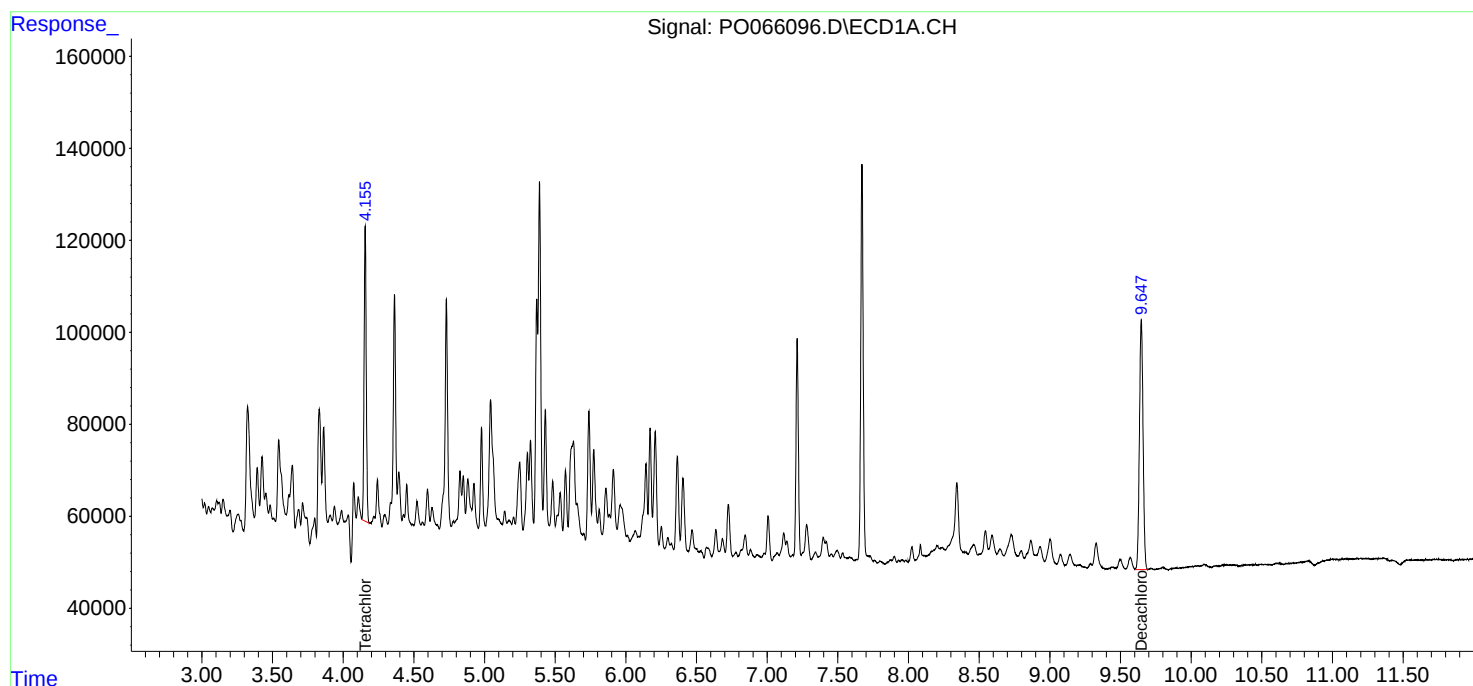

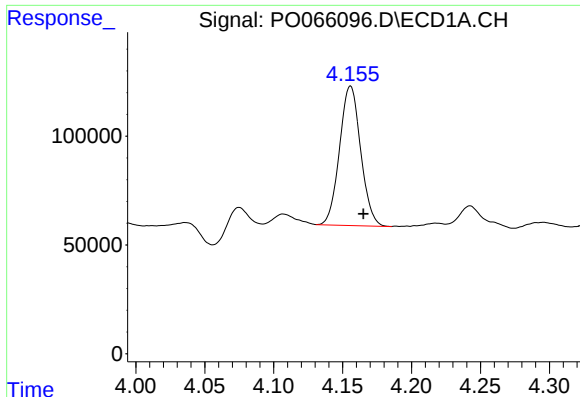


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: -0.010 min
Response: 683453
Conc: 23.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40652


Manual Integrations
APPROVED

mohammad
1/31/2020 2:05:37 PM

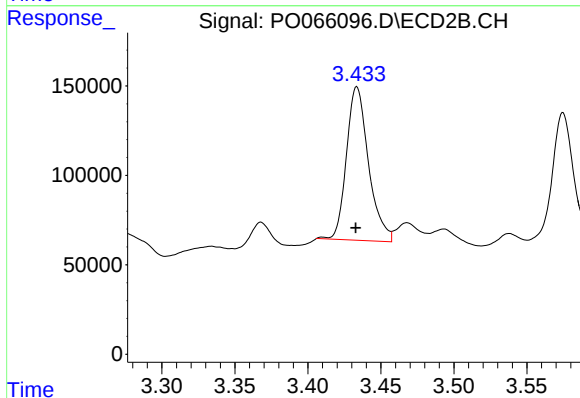


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 900785
Conc: 22.02 ng/ml

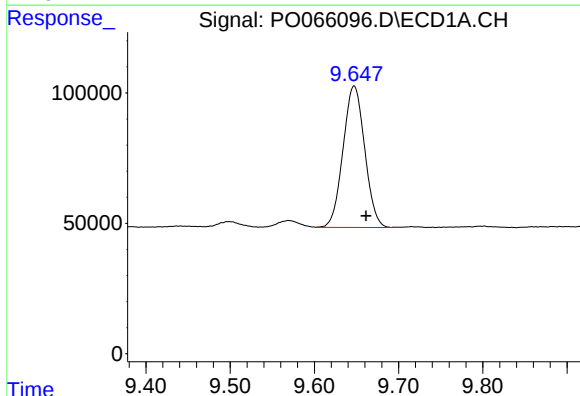

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.014 min
Response: 969132
Conc: 24.59 ng/ml

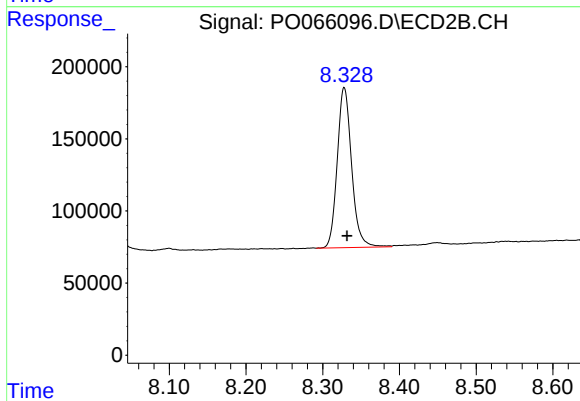

#2 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: -0.004 min
Response: 1447349
Conc: 24.69 ng/ml