

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066107.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2020 20:50
 Operator : DD\AJ
 Sample : L1297-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-0122220-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 03:01:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.431	471961	679374	16.201	16.609
2)	SA Decachlor...	9.645	8.325	561275	829211	14.243	14.148

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
Data File : P0066107.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2020 20:50
Operator : DD\AJ
Sample : L1297-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-0122220-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 03:01:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

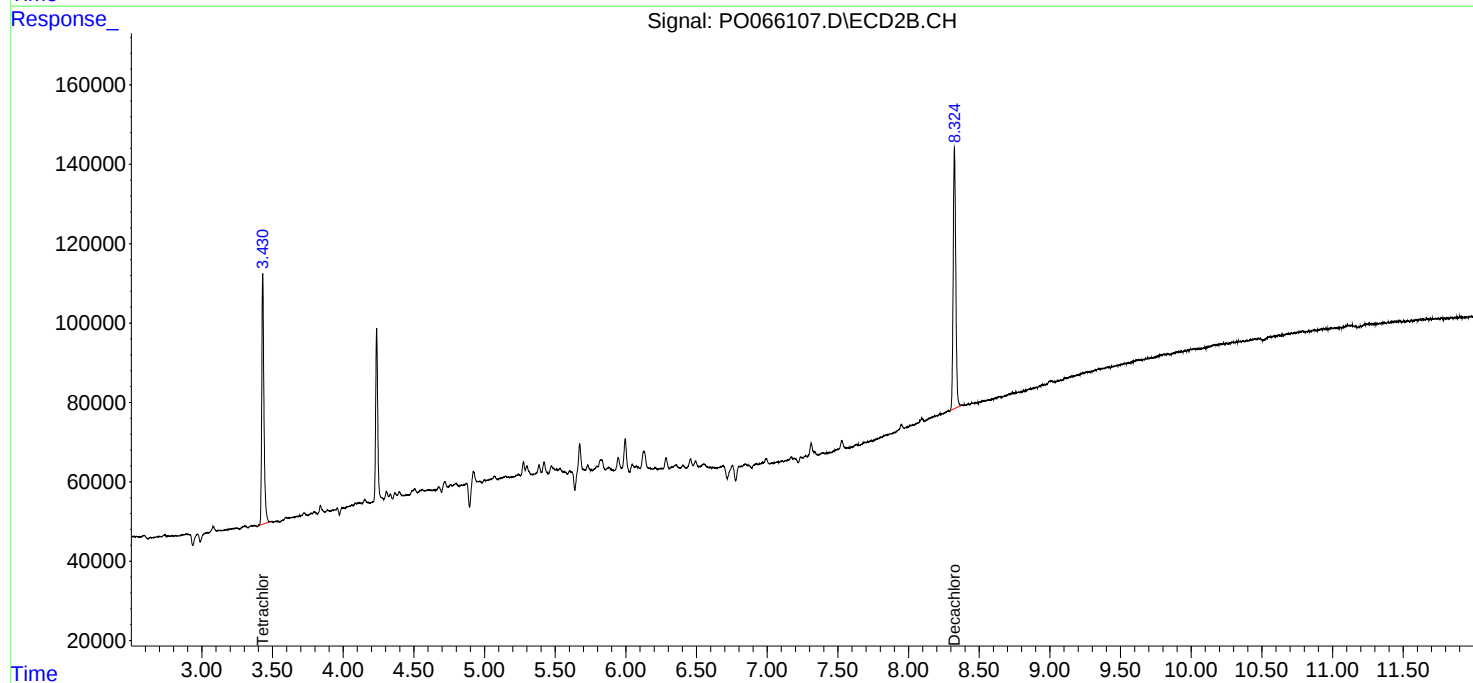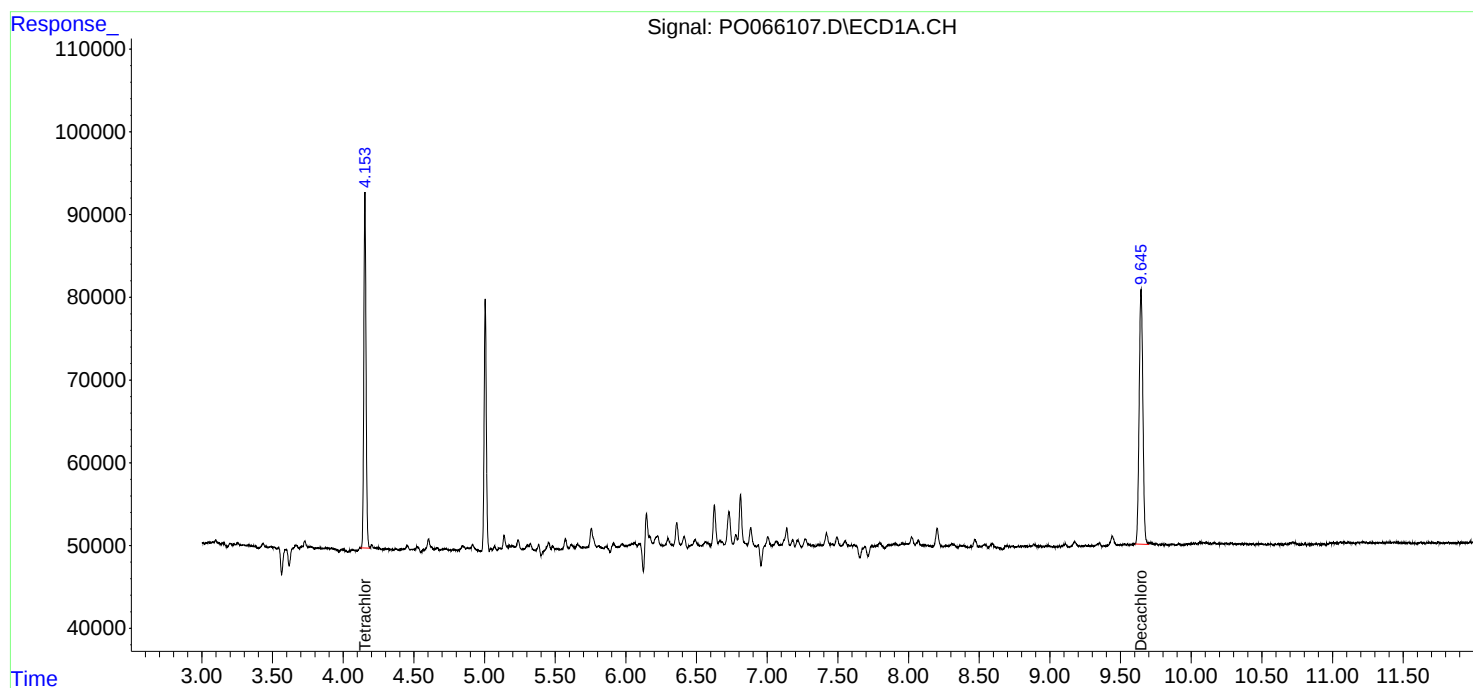


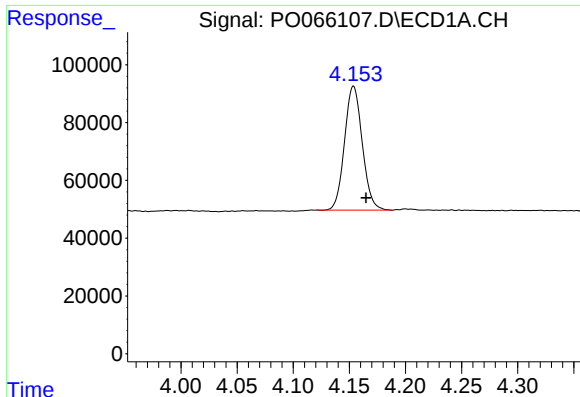

#1 Tetrachloro-m-xylene


R.T.: 4.154 min
Delta R.T.: -0.011 min
Response: 471961
Conc: 16.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-0122220-02

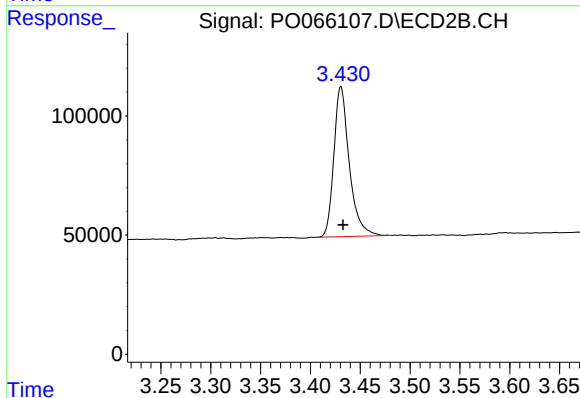


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.002 min
Response: 679374
Conc: 16.61 ng/ml

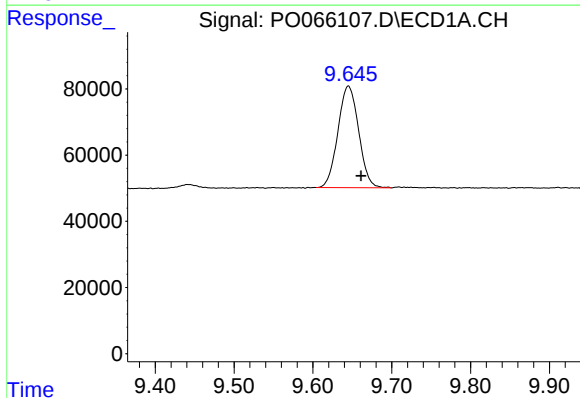

#2 Decachlorobiphenyl

R.T.: 9.645 min
Delta R.T.: -0.016 min
Response: 561275
Conc: 14.24 ng/ml

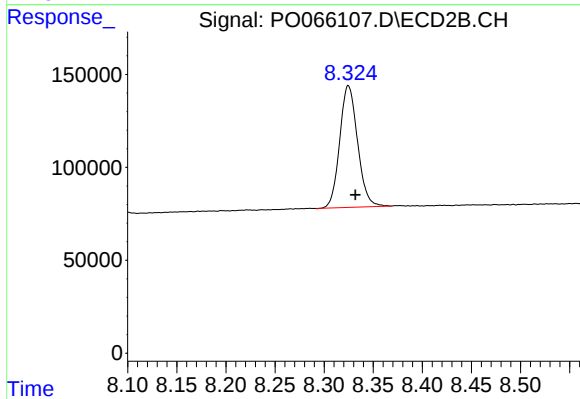

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 829211
Conc: 14.15 ng/ml