

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 1:52
 Operator : DD\AJ
 Sample : L1256-01 5X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TANK-1

Manual Integrations
 APPROVED

mohammad
 1/31/2020 2:06:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 03:07:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.152	3.435	97816	365993	3.358m	8.948m#
2) SA Decachlor...	9.650	8.324	229183	160800	5.816m	2.744m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO013020\
Data File : PO066120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 1:52
Operator : DD\AJ
Sample : L1256-01 5X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TANK-1


Manual Integrations
APPROVED

mohammad
1/31/2020 2:06:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 03:07:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

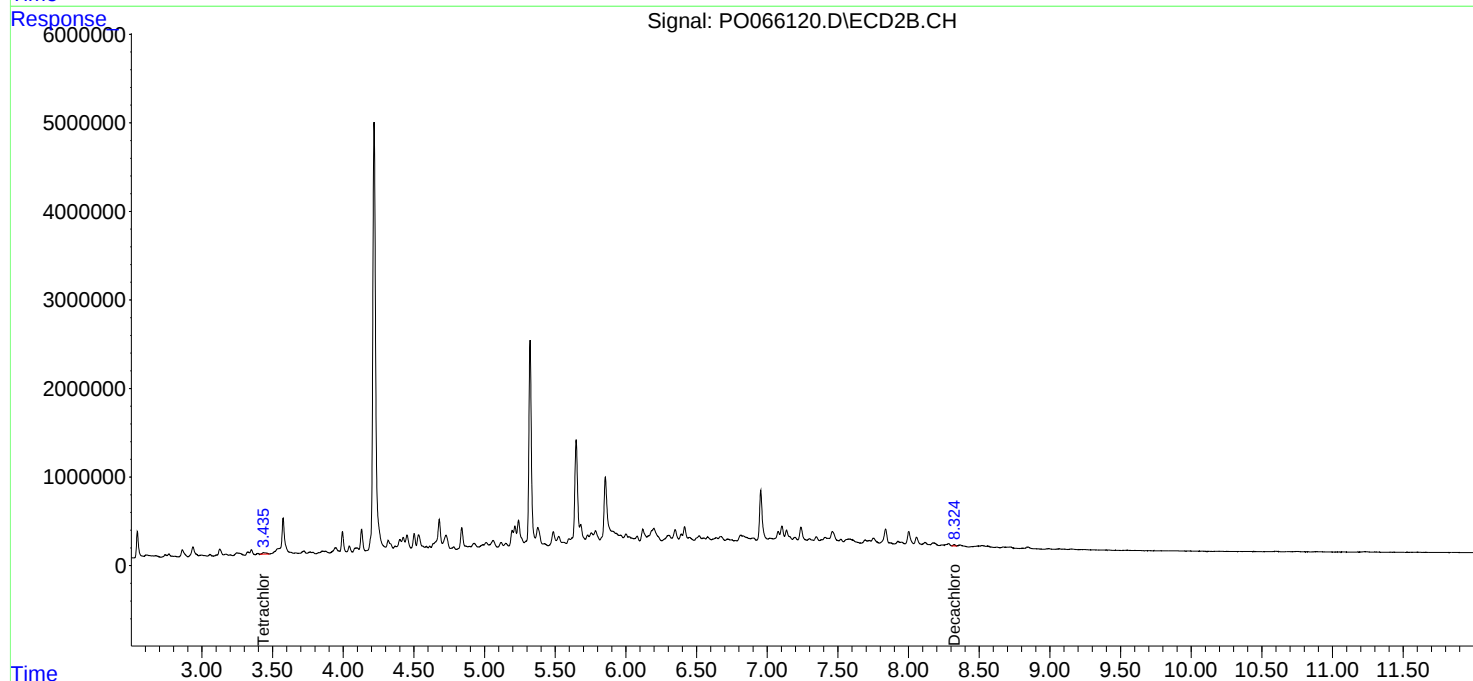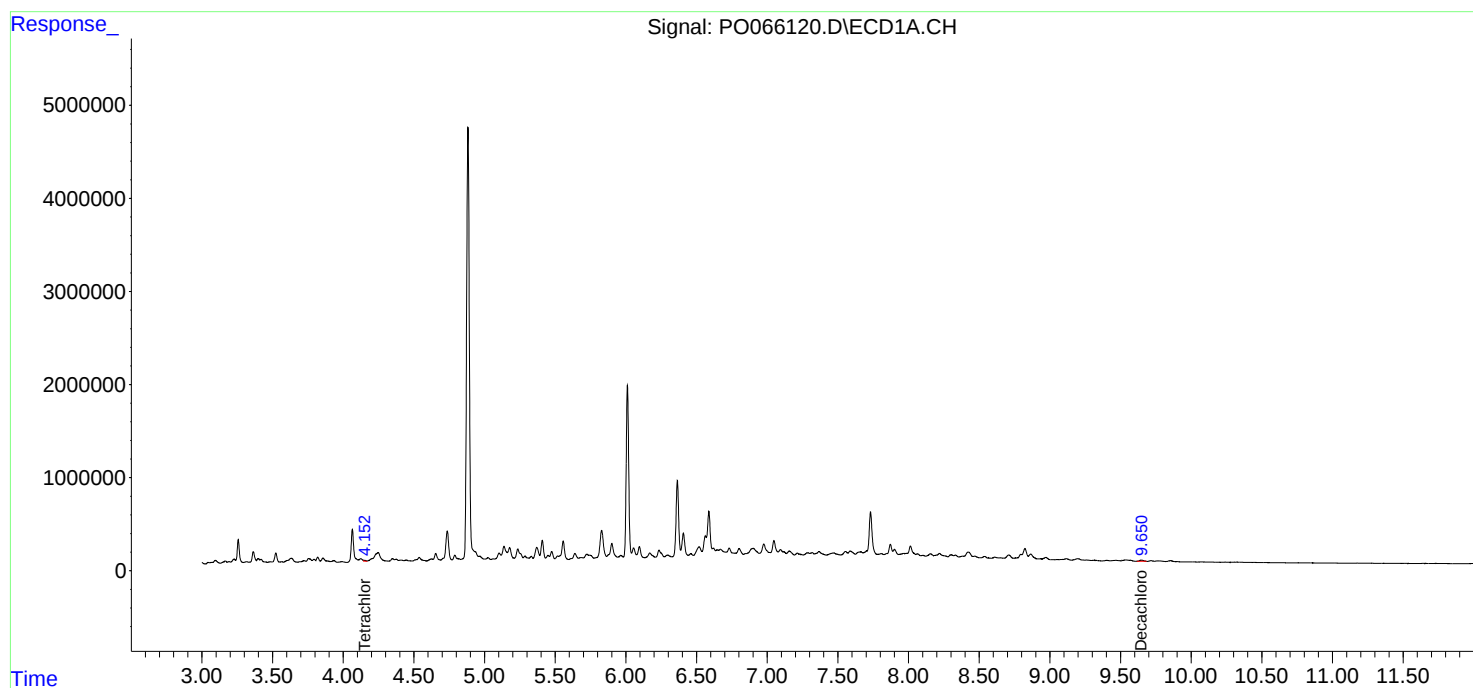

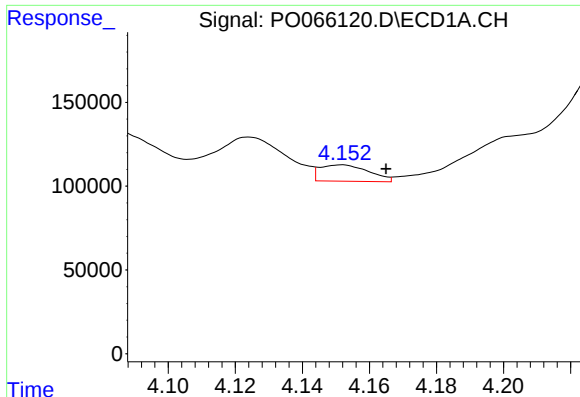


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.013 min
Response: 97816
Conc: 3.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TANK-1


Manual Integrations
APPROVED

mohammad
1/31/2020 2:06:11 PM

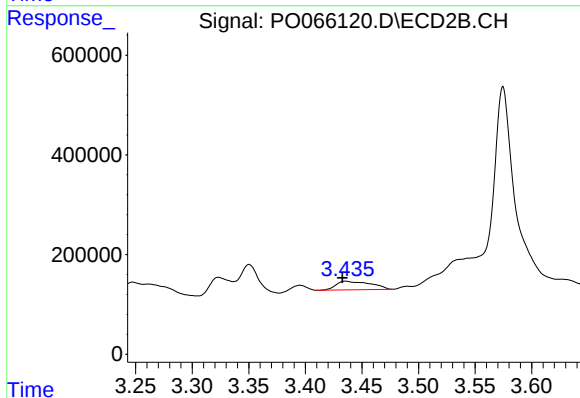


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.002 min
Response: 365993
Conc: 8.95 ng/ml m

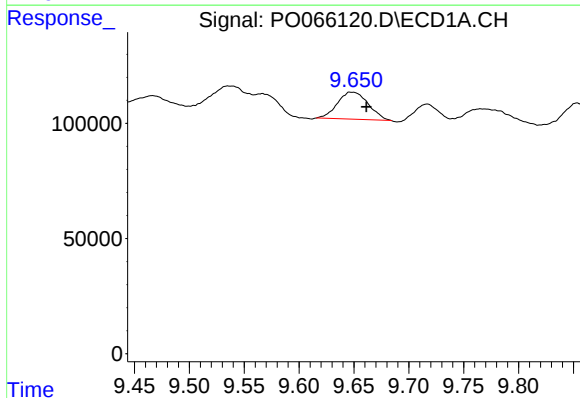

#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: -0.012 min
Response: 229183
Conc: 5.82 ng/ml m

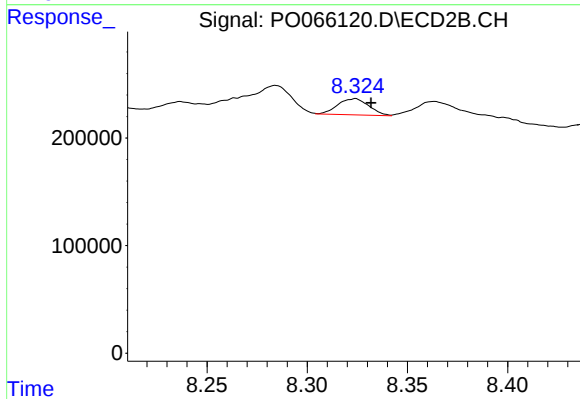

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.008 min
Response: 160800
Conc: 2.74 ng/ml m