

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066131.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 5:47
 Operator : DD\AJ
 Sample : L1004-16
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BU-01-012920

Manual Integrations
 APPROVED

mohammad
 1/31/2020 2:06:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 07:15:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.152	3.430	918777	1379278	31.540m	33.720
2) SA Decachlor...	9.643	8.325	761730	1009491	19.329	17.224

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
Data File : P0066131.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 5:47
Operator : DD\AJ
Sample : L1004-16
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BU-01-012920


Manual Integrations
APPROVED

mohammad
1/31/2020 2:06:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 07:15:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

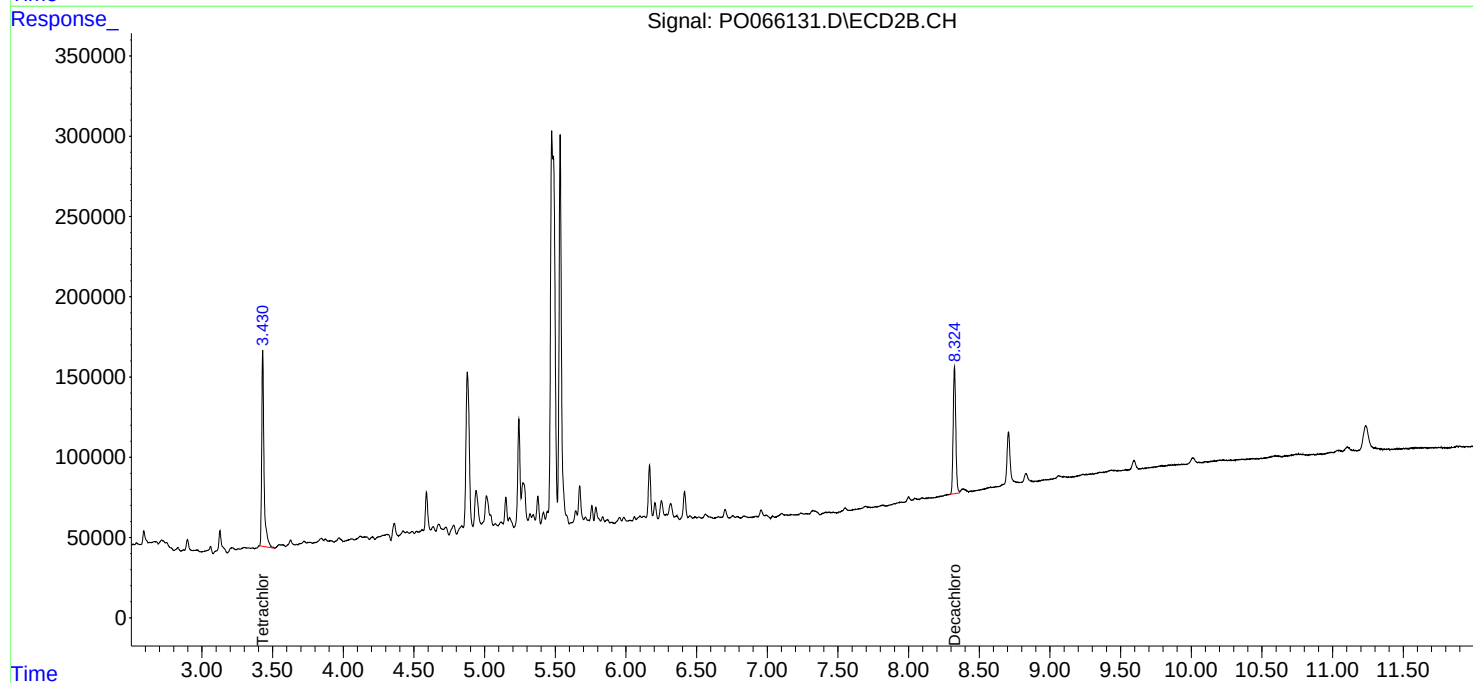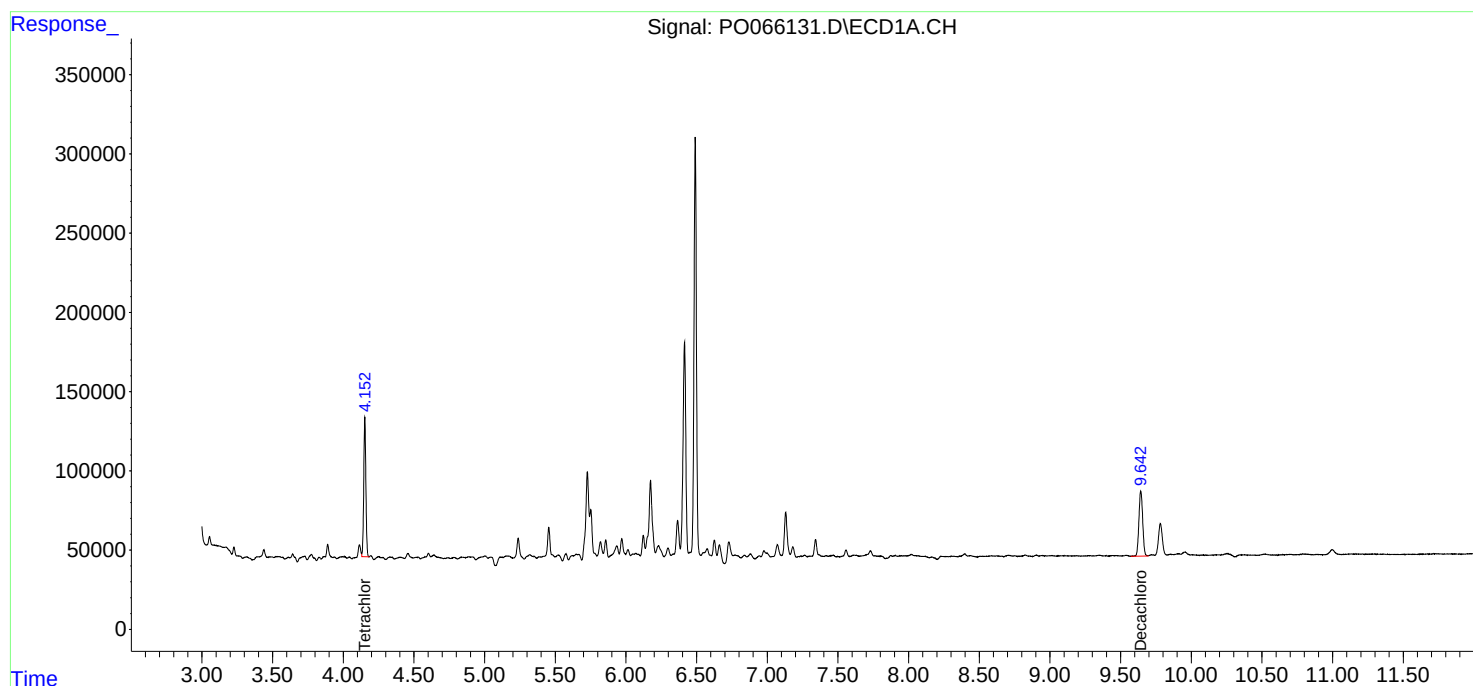

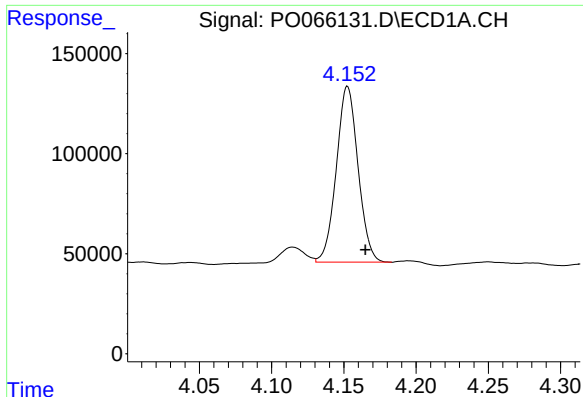


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.013 min
Response: 918777
Conc: 31.54 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BU-01-012920


Manual Integrations
APPROVED

mohammad
1/31/2020 2:06:24 PM

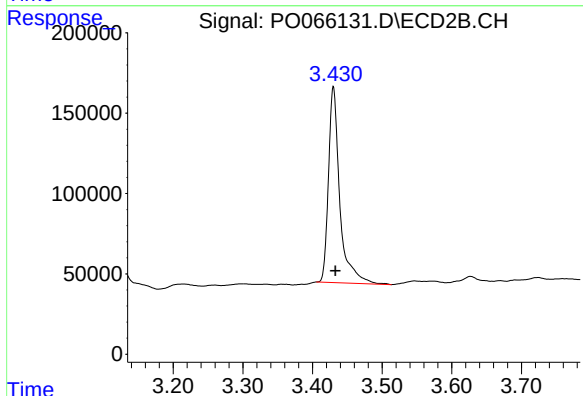


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 1379278
Conc: 33.72 ng/ml

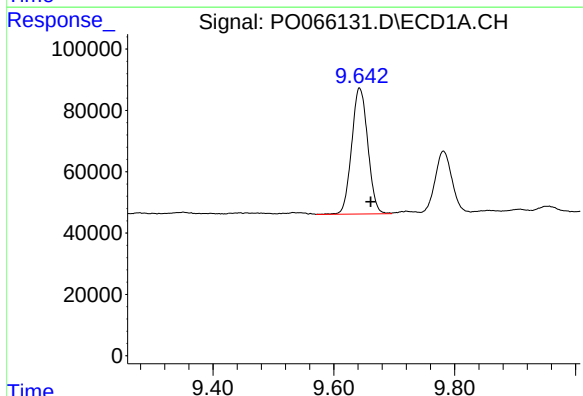

#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.019 min
Response: 761730
Conc: 19.33 ng/ml

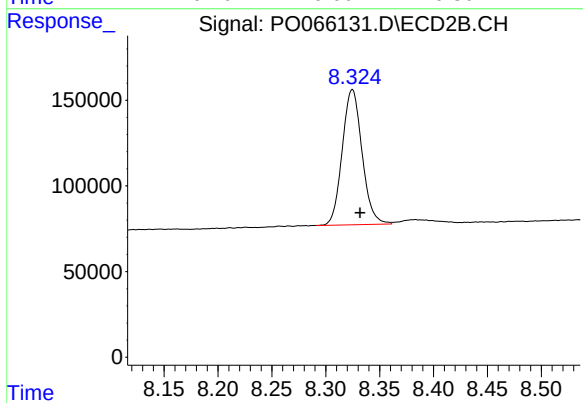

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 1009491
Conc: 17.22 ng/ml