

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
 Data File : P0066142.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 8:51
 Operator : DD\AJ
 Sample : L1274-01RE
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BORING-B1-SAMPLE-S1RE

Manual Integrations
 APPROVED

mohammad
 1/31/2020 2:22:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 12:30:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.430	1087940	1613319	37.347m	39.441
2) SA Decachlor...	9.644	8.324	768853	1036415	19.510	17.683

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013020\
Data File : P0066142.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 8:51
Operator : DD\AJ
Sample : L1274-01RE
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BORING-B1-SAMPLE-S1RE


Manual Integrations
APPROVED

mohammad
1/31/2020 2:22:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 12:30:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

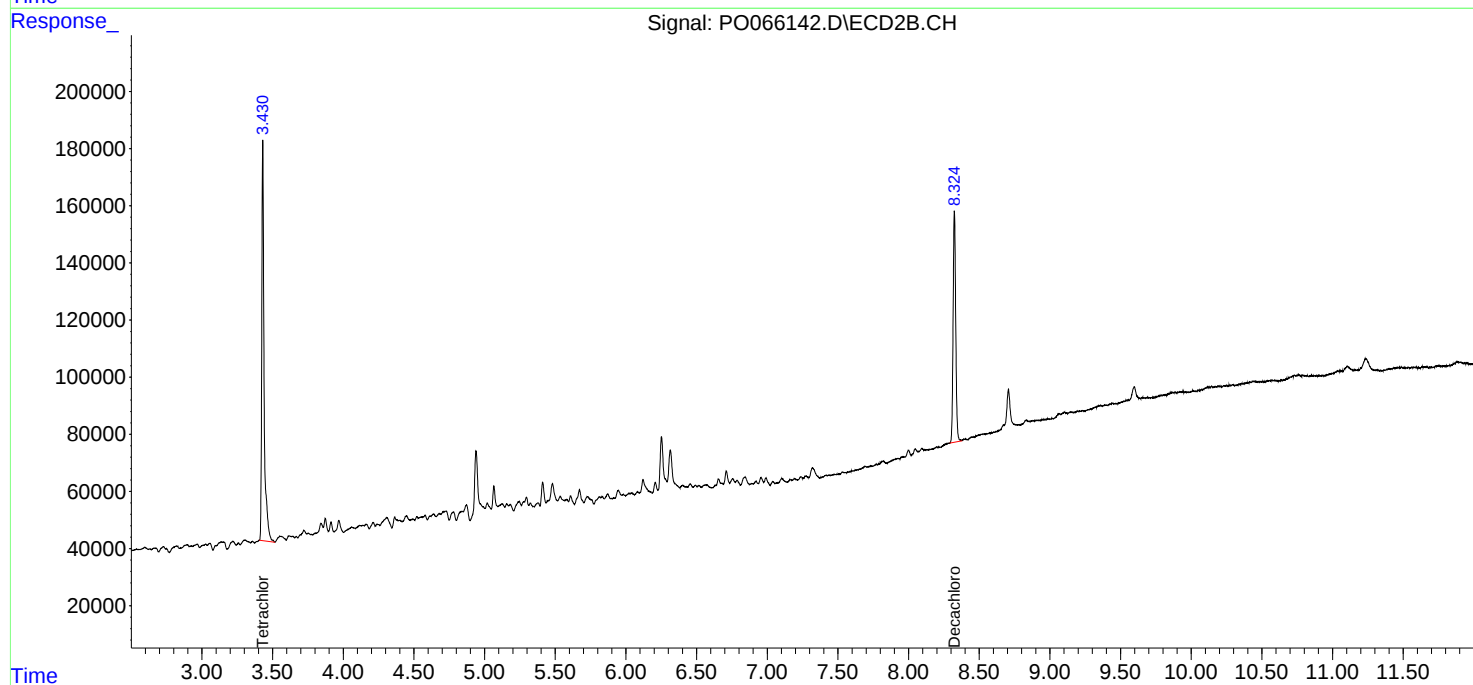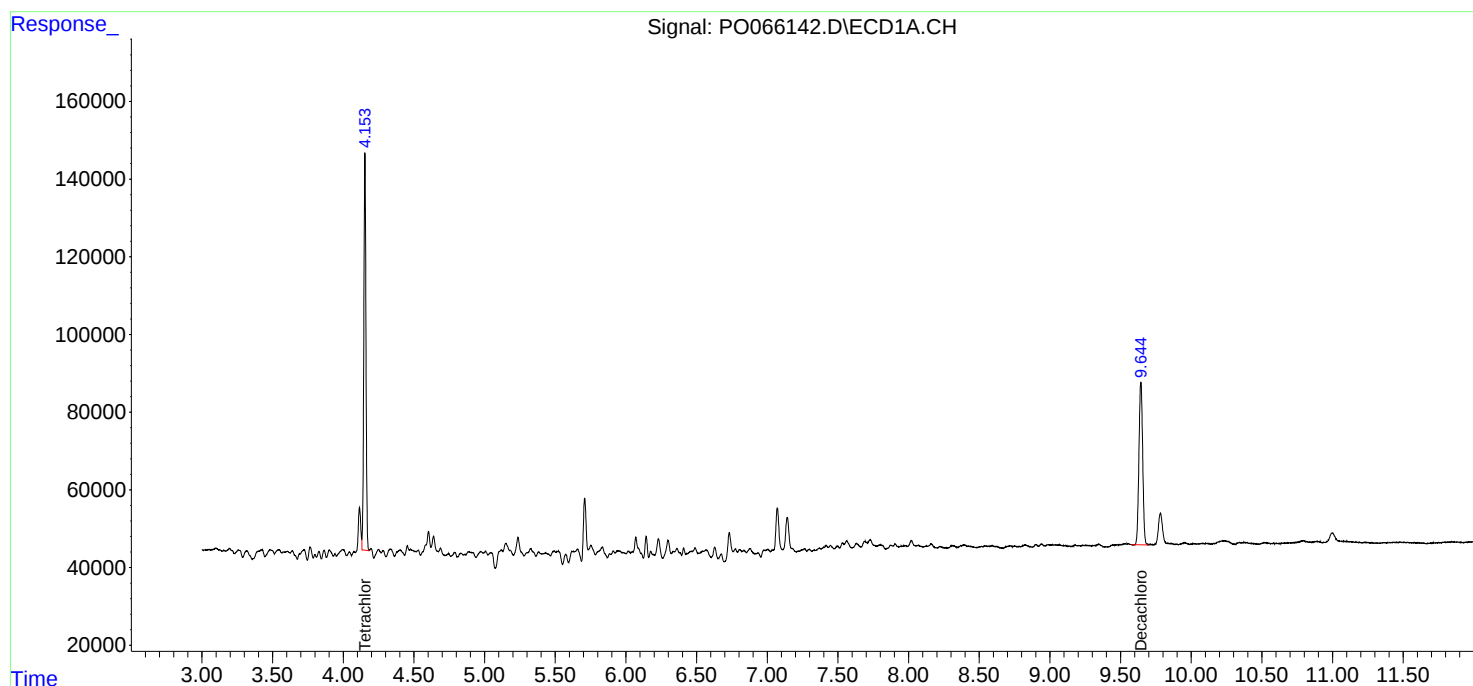

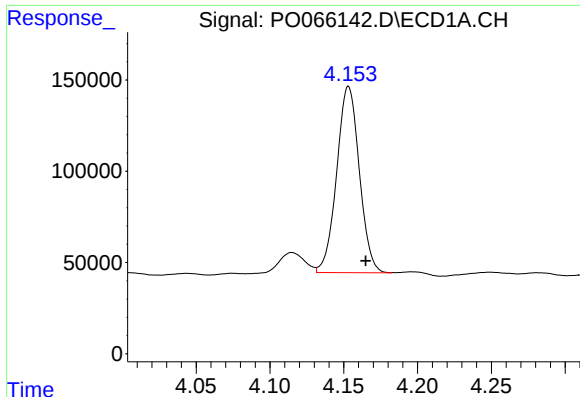

#1 Tetrachloro-m-xylene

R.T.: 4.153 min

Delta R.T.: -0.012 min


Response: 1087940

Conc: 37.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BORING-B1-SAMPLE-S1RE

Manual Integrations
APPROVED

mohammad
1/31/2020 2:22:15 PM

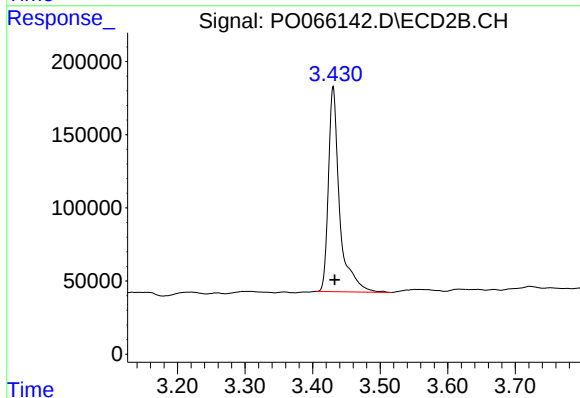


#1 Tetrachloro-m-xylene

R.T.: 3.430 min

Delta R.T.: -0.002 min

Response: 1613319

Conc: 39.44 ng/ml

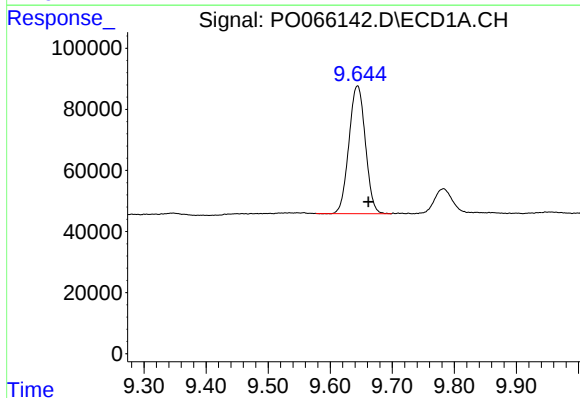


#2 Decachlorobiphenyl

R.T.: 9.644 min

Delta R.T.: -0.017 min

Response: 768853

Conc: 19.51 ng/ml

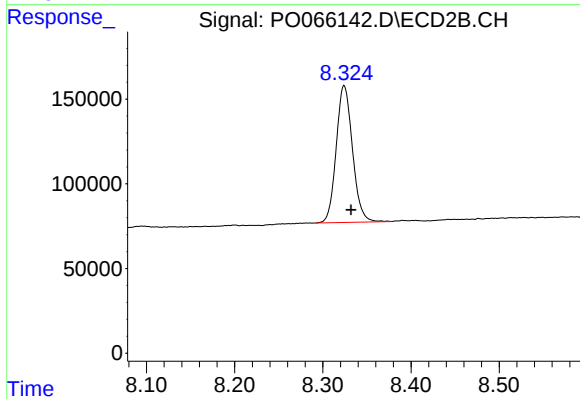

#2 Decachlorobiphenyl

R.T.: 8.324 min

Delta R.T.: -0.008 min

Response: 1036415

Conc: 17.68 ng/ml