

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013125\
 Data File : P0109330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2025 13:43
 Operator : YP/AJ
 Sample : Q1244-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-02-01302025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/03/2025
 Supervised By :Ankita Jodhani 02/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 16:38:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 22 03:46:11 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.698	3.695	122.0E6	90632796	16.141m	16.908m
2) SA Decachlor...	8.759	8.710	104.9E6	54896604	15.141	15.964

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO013125\
Data File : PO109330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2025 13:43
Operator : YP/AJ
Sample : Q1244-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-02-01302025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2025
Supervised By :Ankita Jodhani 02/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 16:38:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012125.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 22 03:46:11 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

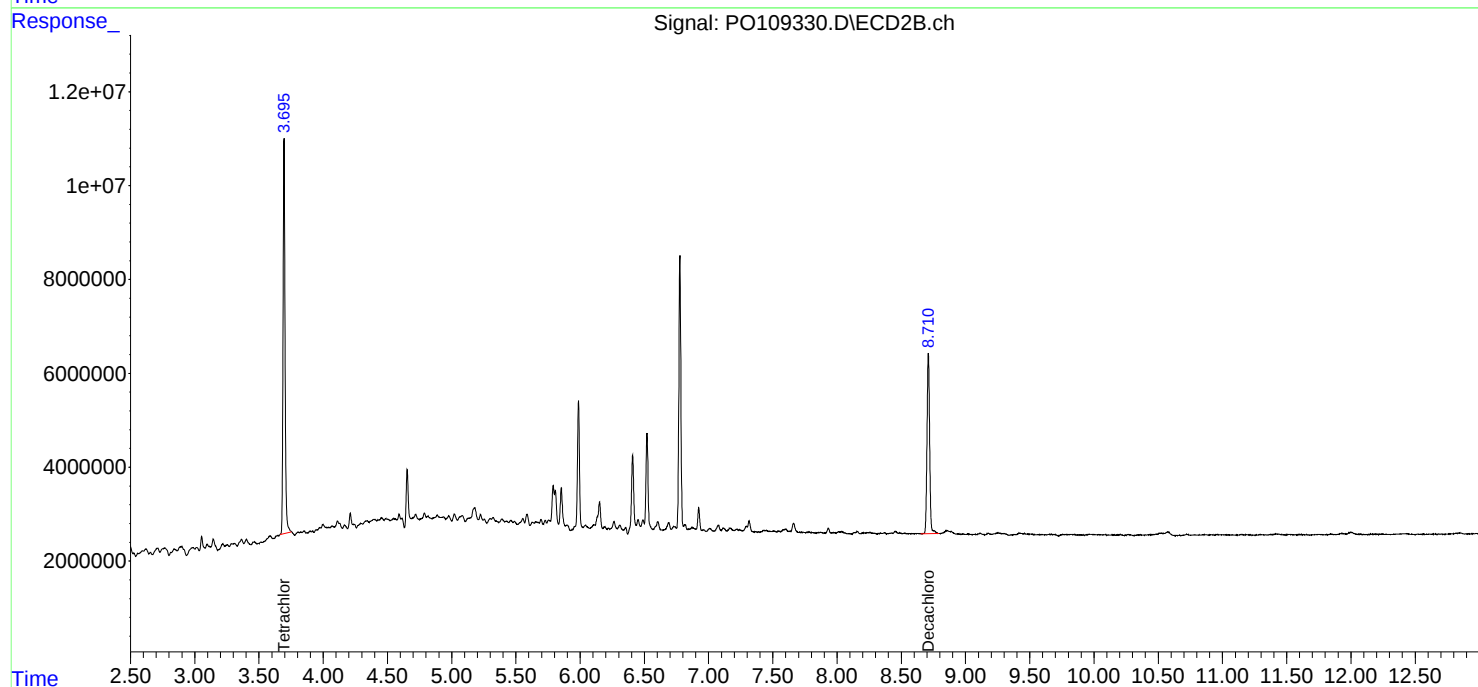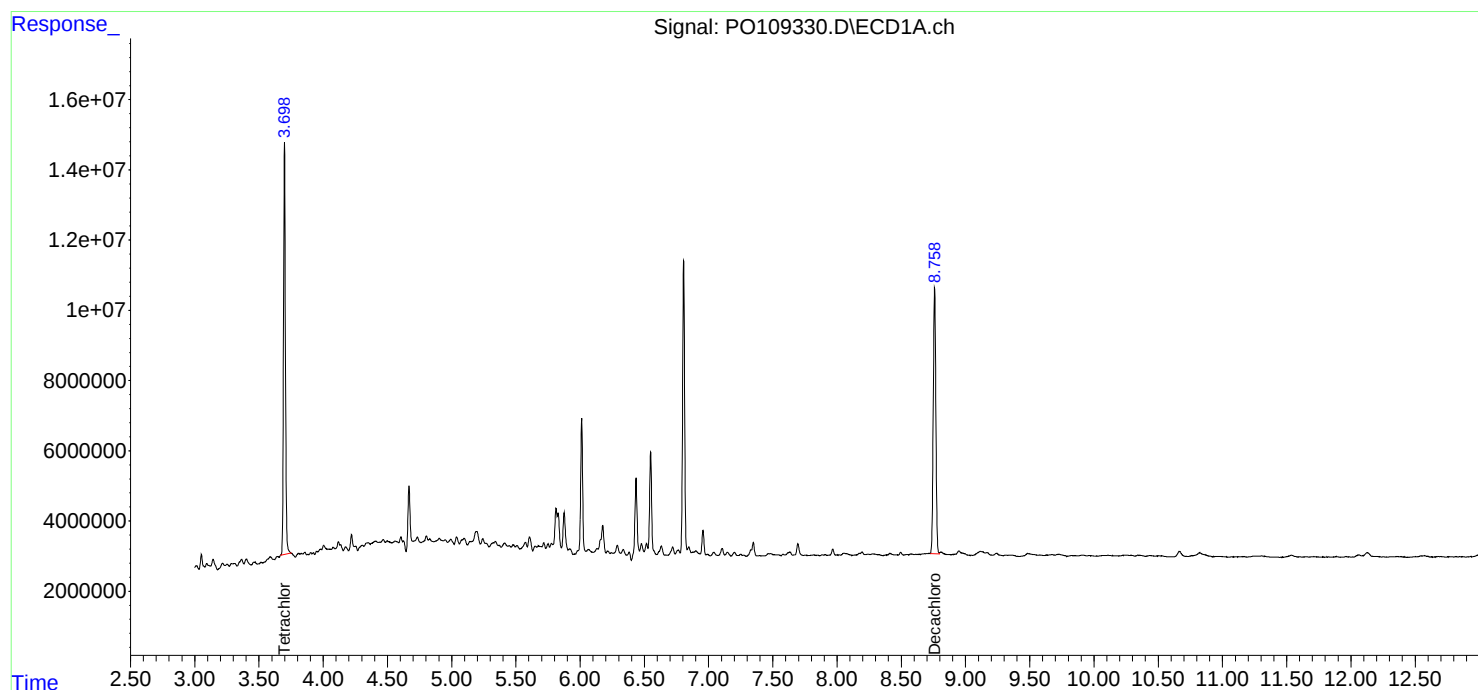

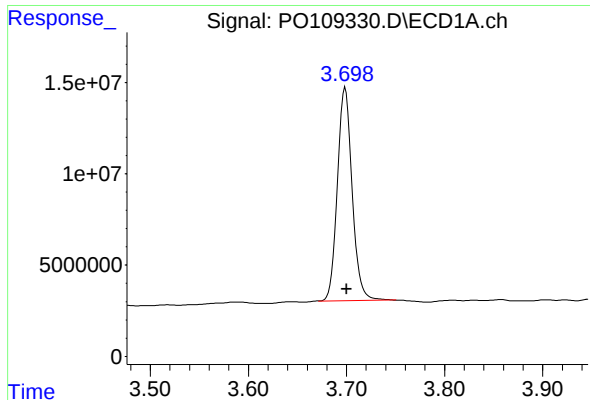


#1 Tetrachloro-m-xylene

R.T.: 3.698 min
Delta R.T.: -0.002 min
Response: 121967425
Conc: 16.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-02-01302025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2025
Supervised By :Ankita Jodhani 02/03/2025

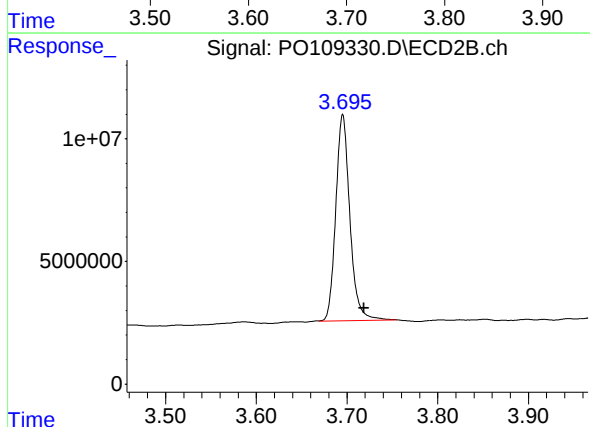


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: -0.024 min
Response: 90632796
Conc: 16.91 ng/ml

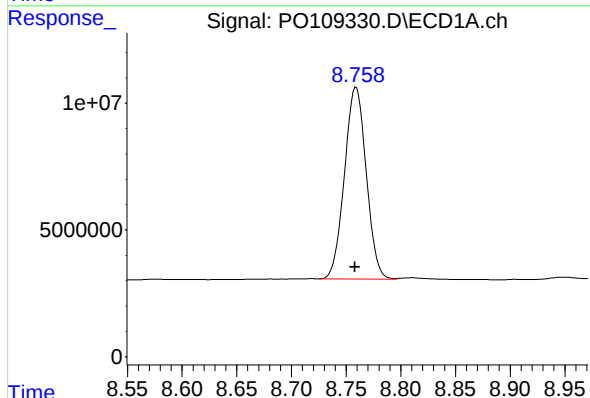

#2 Decachlorobiphenyl

R.T.: 8.759 min
Delta R.T.: 0.000 min
Response: 104895626
Conc: 15.14 ng/ml

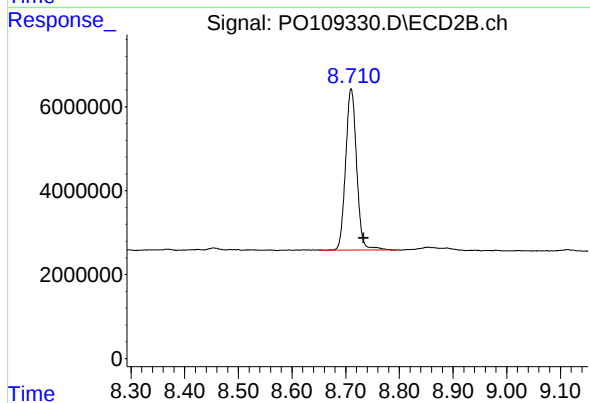

#2 Decachlorobiphenyl

R.T.: 8.710 min
Delta R.T.: -0.023 min
Response: 54896604
Conc: 15.96 ng/ml