

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020123\
 Data File : P0092335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2023 21:35
 Operator : YP/AJ
 Sample : 01335-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 338

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/02/2023
 Supervised By :Ankita Jodhani 02/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:52:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.646	23497722	11286598	8.117	8.038
2) SA Decachlor...	10.367	8.686	14669442	7466664	7.108	6.614
Target Compounds						
31) L7 AR-1260-1	7.270	6.222	11875789	5551750	90.135	73.495
32) L7 AR-1260-2	7.534	6.411	23444224	7889383	158.101m	90.047 #
33) L7 AR-1260-3	7.902	6.560	11693762	10947540	103.244	126.285
34) L7 AR-1260-4	8.128	7.040	13485748	3722782	108.787m	55.591 #
35) L7 AR-1260-5	8.465	7.283	16864873	10496079	75.948	73.760

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020123\
Data File : PO092335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2023 21:35
Operator : YP/AJ
Sample : 01335-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
338


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:52:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

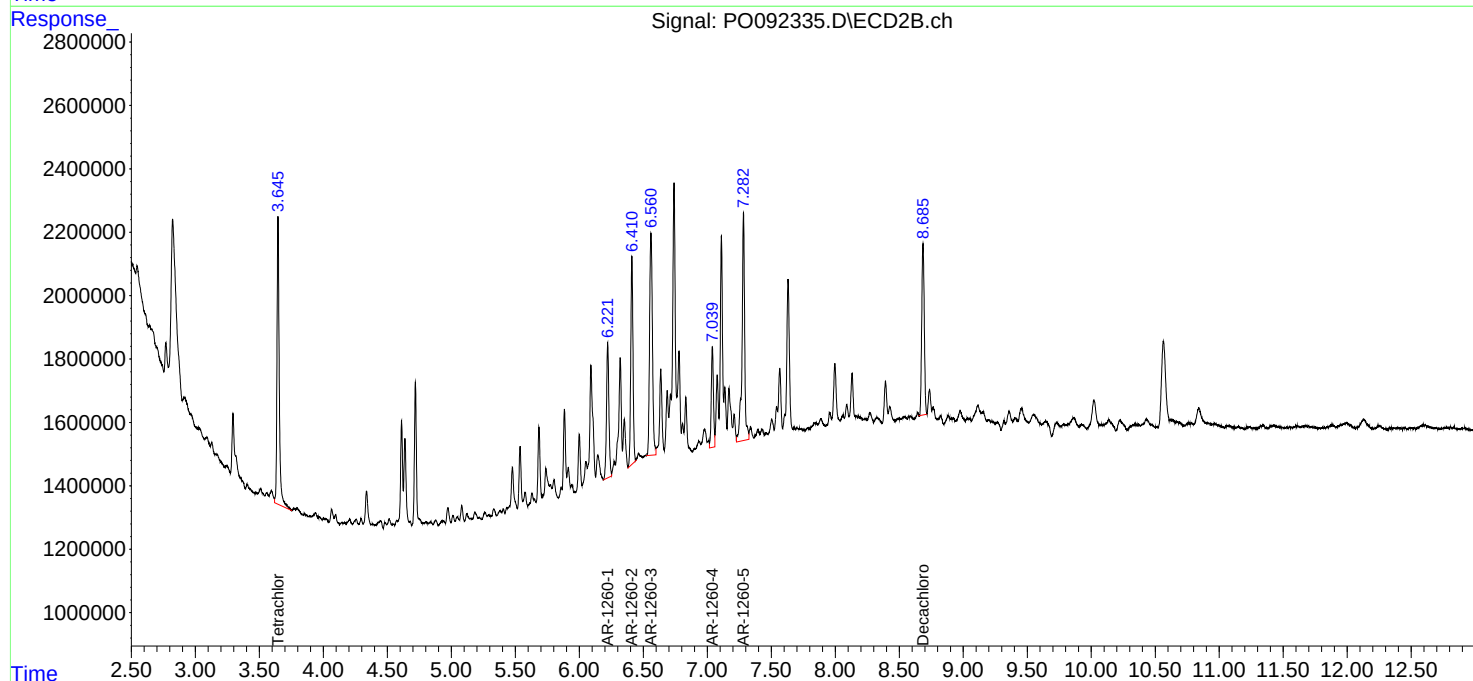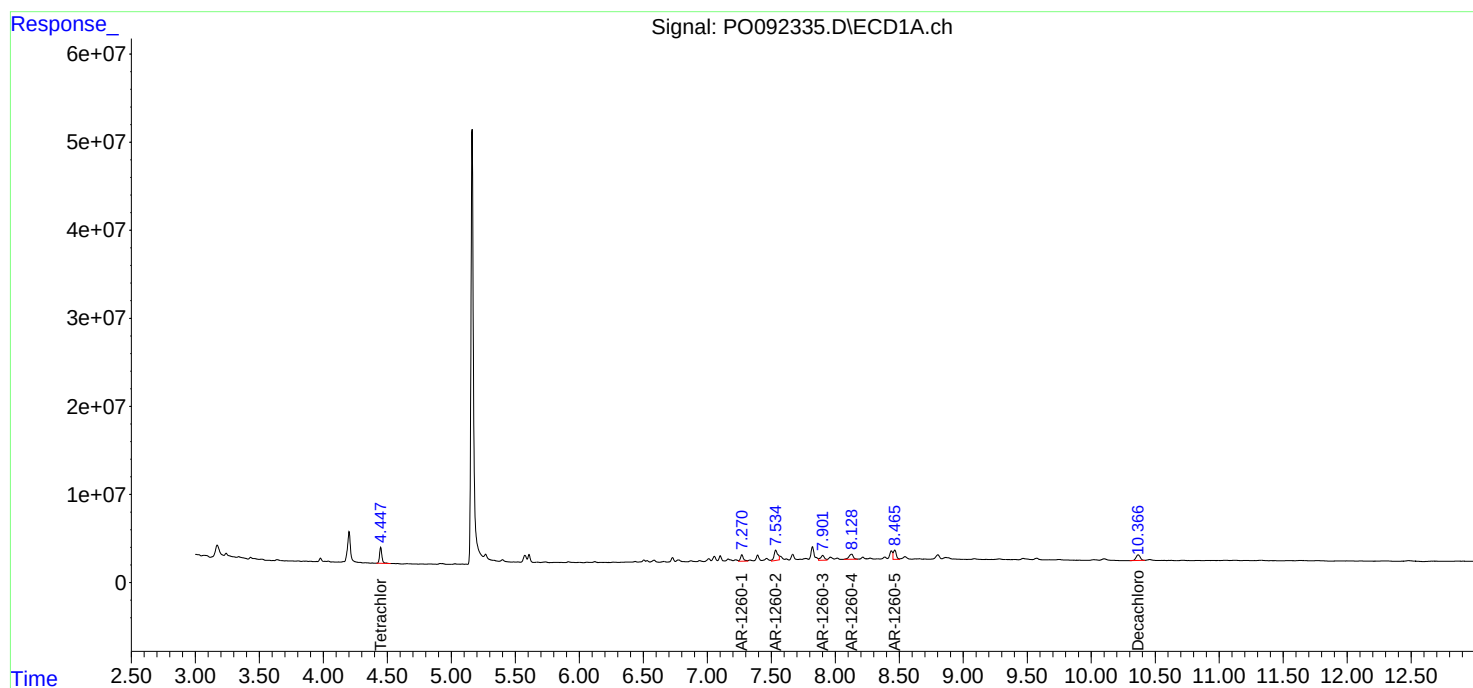

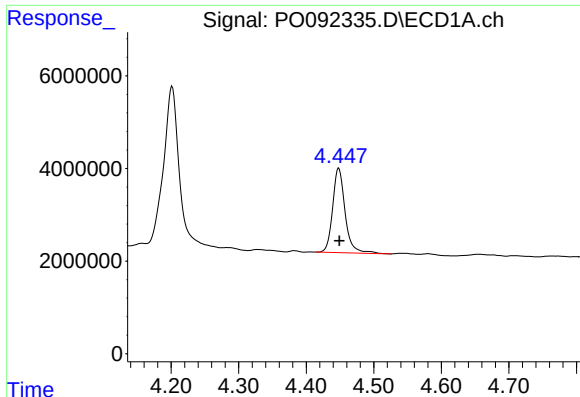


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 23497722
Conc: 8.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
338


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

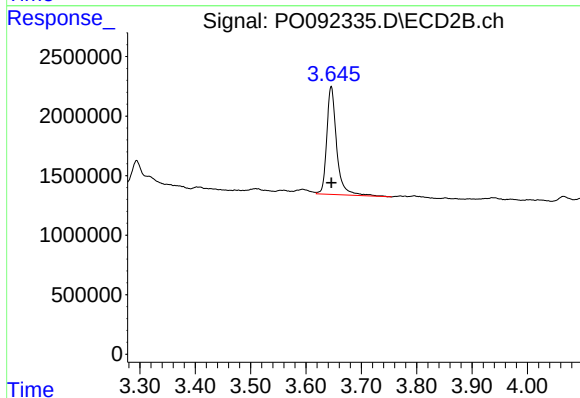


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 11286598
Conc: 8.04 ng/ml

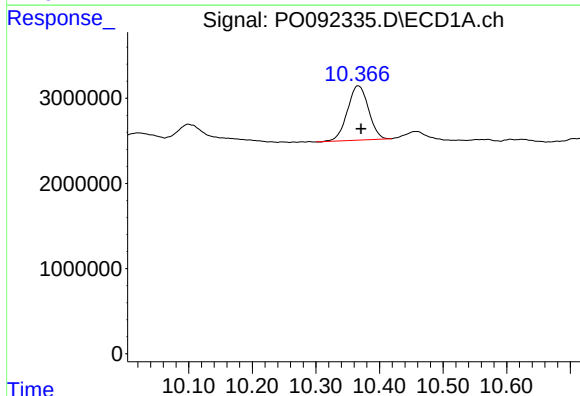


#2 Decachlorobiphenyl

R.T.: 10.367 min
Delta R.T.: -0.005 min
Response: 14669442
Conc: 7.11 ng/ml

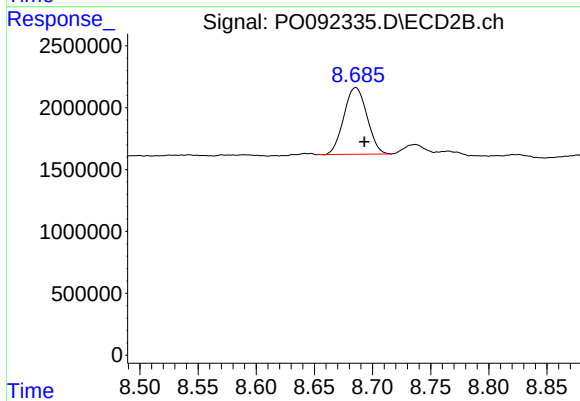

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.008 min
Response: 7466664
Conc: 6.61 ng/ml

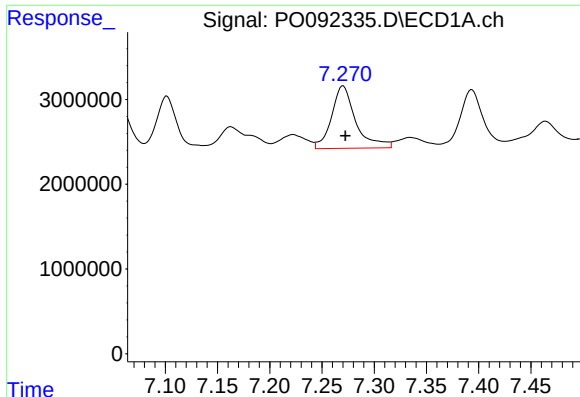


#31 AR-1260-1

R.T.: 7.270 min
Delta R.T.: -0.002 min
Response: 11875789
Conc: 90.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
338


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

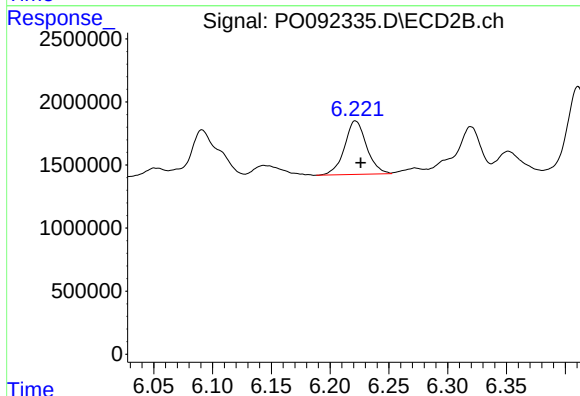


#31 AR-1260-1

R.T.: 6.222 min
Delta R.T.: -0.004 min
Response: 5551750
Conc: 73.49 ng/ml

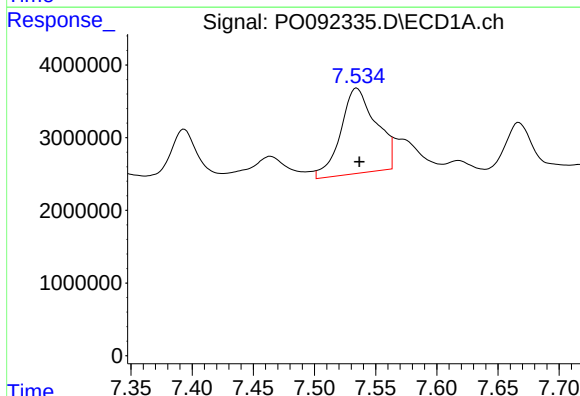


#32 AR-1260-2

R.T.: 7.534 min
Delta R.T.: -0.003 min
Response: 23444224
Conc: 158.10 ng/ml m

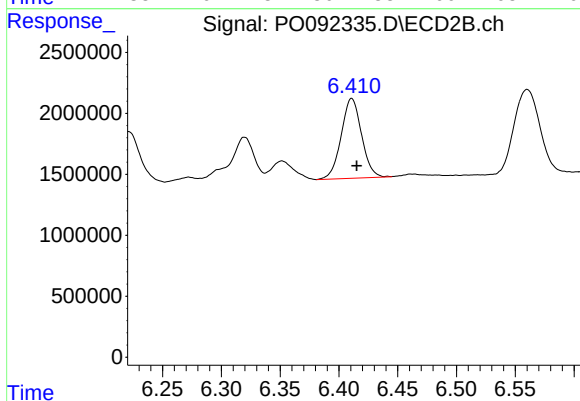

#32 AR-1260-2

R.T.: 6.411 min
Delta R.T.: -0.004 min
Response: 7889383
Conc: 90.05 ng/ml

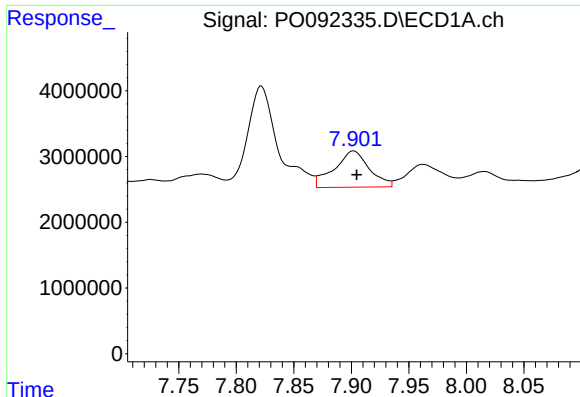


#33 AR-1260-3

R.T.: 7.902 min
Delta R.T.: -0.003 min
Response: 11693762
Conc: 103.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
338


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

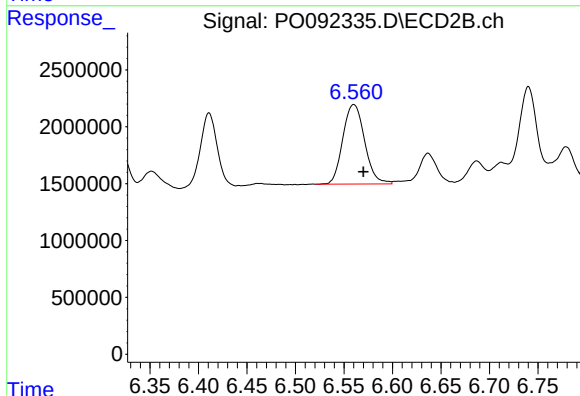


#33 AR-1260-3

R.T.: 6.560 min
Delta R.T.: -0.010 min
Response: 10947540
Conc: 126.28 ng/ml

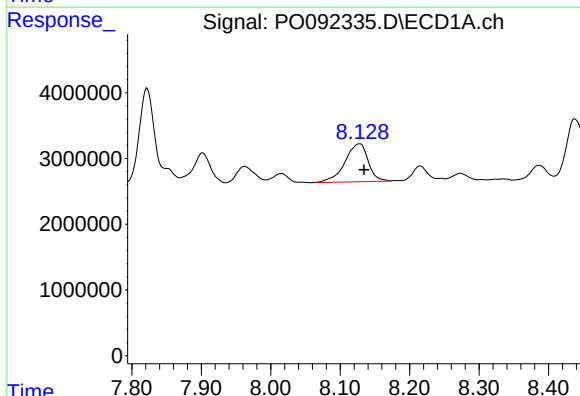


#34 AR-1260-4

R.T.: 8.128 min
Delta R.T.: -0.006 min
Response: 13485748
Conc: 108.79 ng/ml m

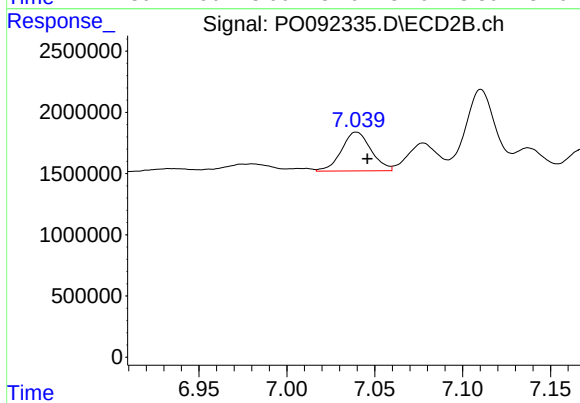

#34 AR-1260-4

R.T.: 7.040 min
Delta R.T.: -0.006 min
Response: 3722782
Conc: 55.59 ng/ml

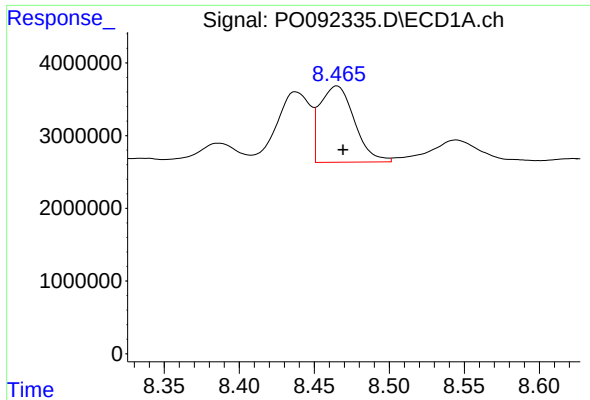


#35 AR-1260-5

R.T.: 8.465 min
Delta R.T.: -0.004 min
Response: 16864873
Conc: 75.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
338

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

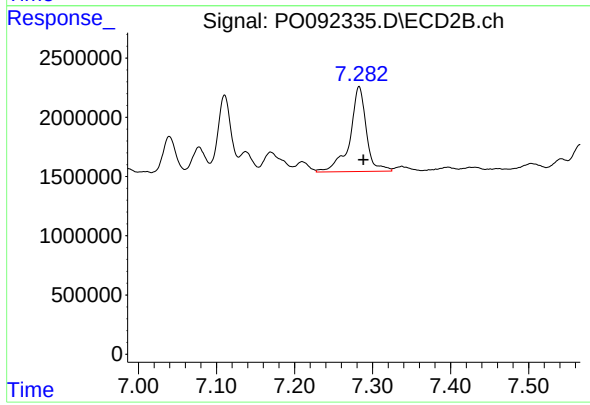

#35 AR-1260-5

R.T.: 7.283 min
Delta R.T.: -0.006 min
Response: 10496079
Conc: 73.76 ng/ml