

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020123\
 Data File : P0092342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2023 00:32
 Operator : YP/AJ
 Sample : 01369-07 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP1-0131

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/02/2023
 Supervised By :Ankita Jodhani 02/02/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:42:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.647	2479604	1258688	0.857	0.896
2) SA Decachlor...	10.368	8.685	2223463	1277076	1.077m	1.131

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020123\
Data File : PO092342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2023 00:32
Operator : YP/AJ
Sample : 01369-07 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP1-0131


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:42:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

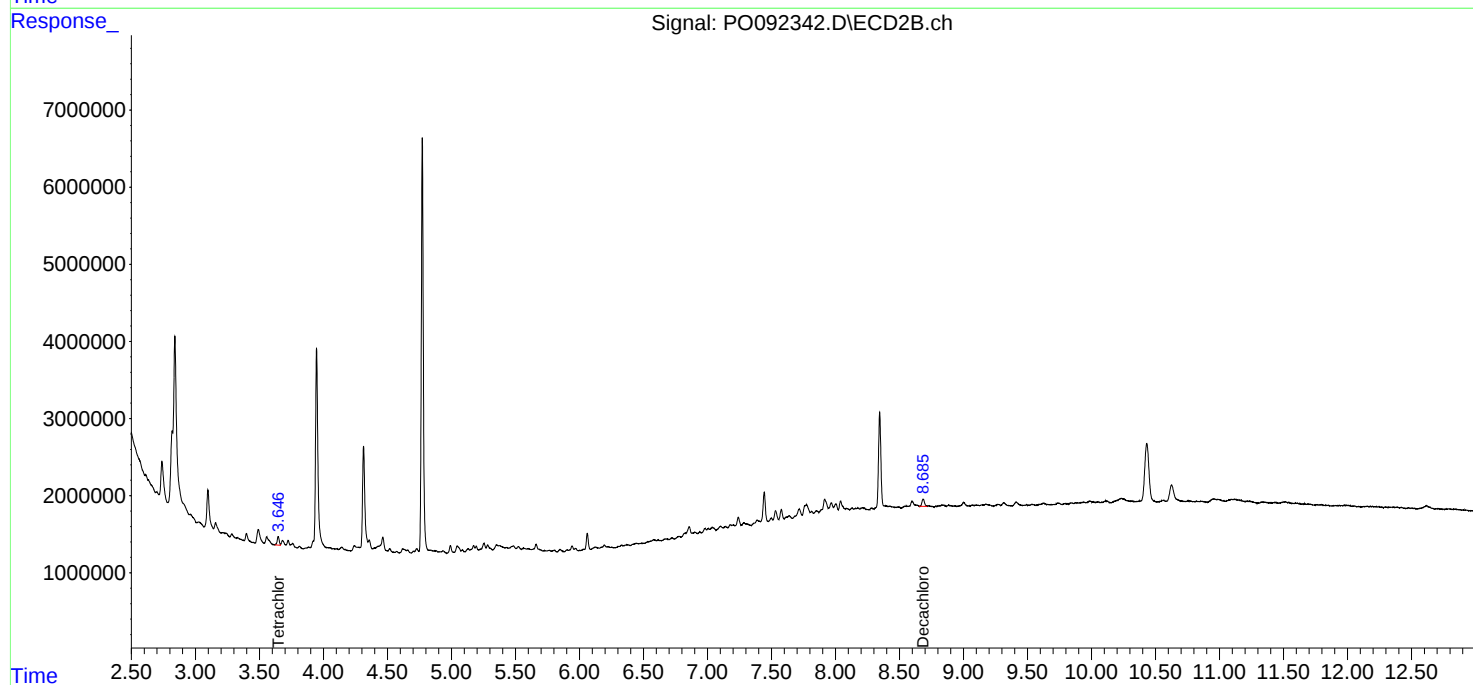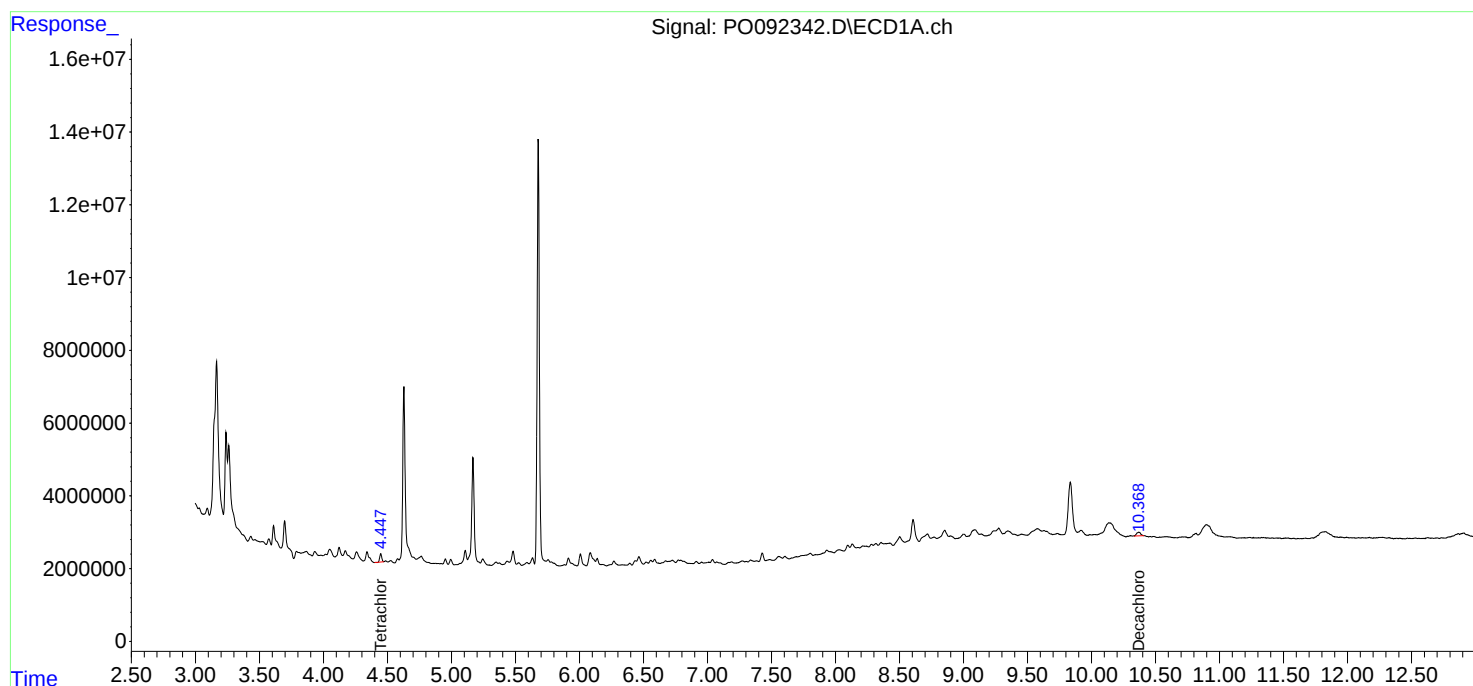

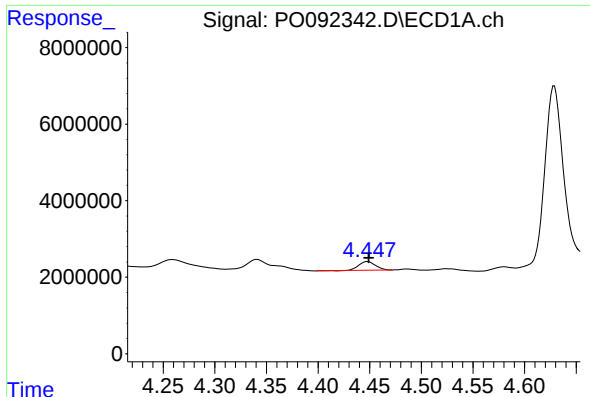


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.001 min
Response: 2479604
Conc: 0.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP1-0131


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/02/2023
Supervised By :Ankita Jodhani 02/02/2023

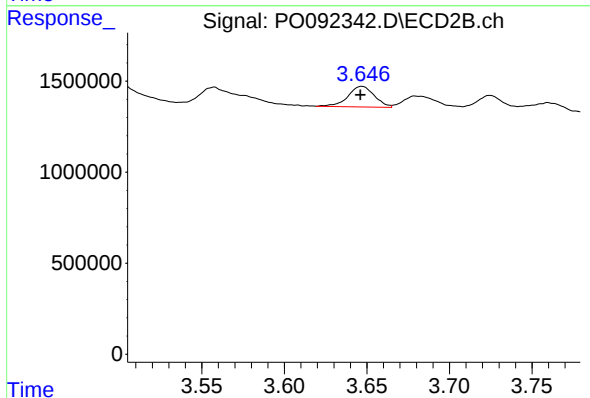


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 1258688
Conc: 0.90 ng/ml

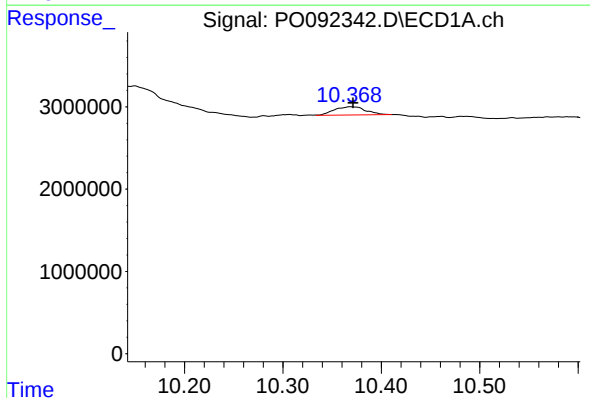

#2 Decachlorobiphenyl

R.T.: 10.368 min
Delta R.T.: -0.003 min
Response: 2223463
Conc: 1.08 ng/ml m

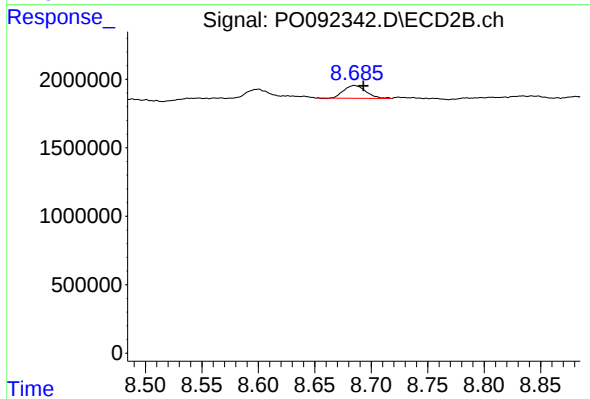

#2 Decachlorobiphenyl

R.T.: 8.685 min
Delta R.T.: -0.008 min
Response: 1277076
Conc: 1.13 ng/ml