

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020124\
 Data File : P0101529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2024 17:56
 Operator : YP/AJ
 Sample : P1312-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 19690

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:22:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.333	3.634	57448084	29779264	14.966m	11.523m
2) SA Decachlor...	10.063	8.680	60469211	33500164	25.951	17.678 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020124\
Data File : PO101529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2024 17:56
Operator : YP/AJ
Sample : P1312-03
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
19690


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:22:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 24 04:51:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

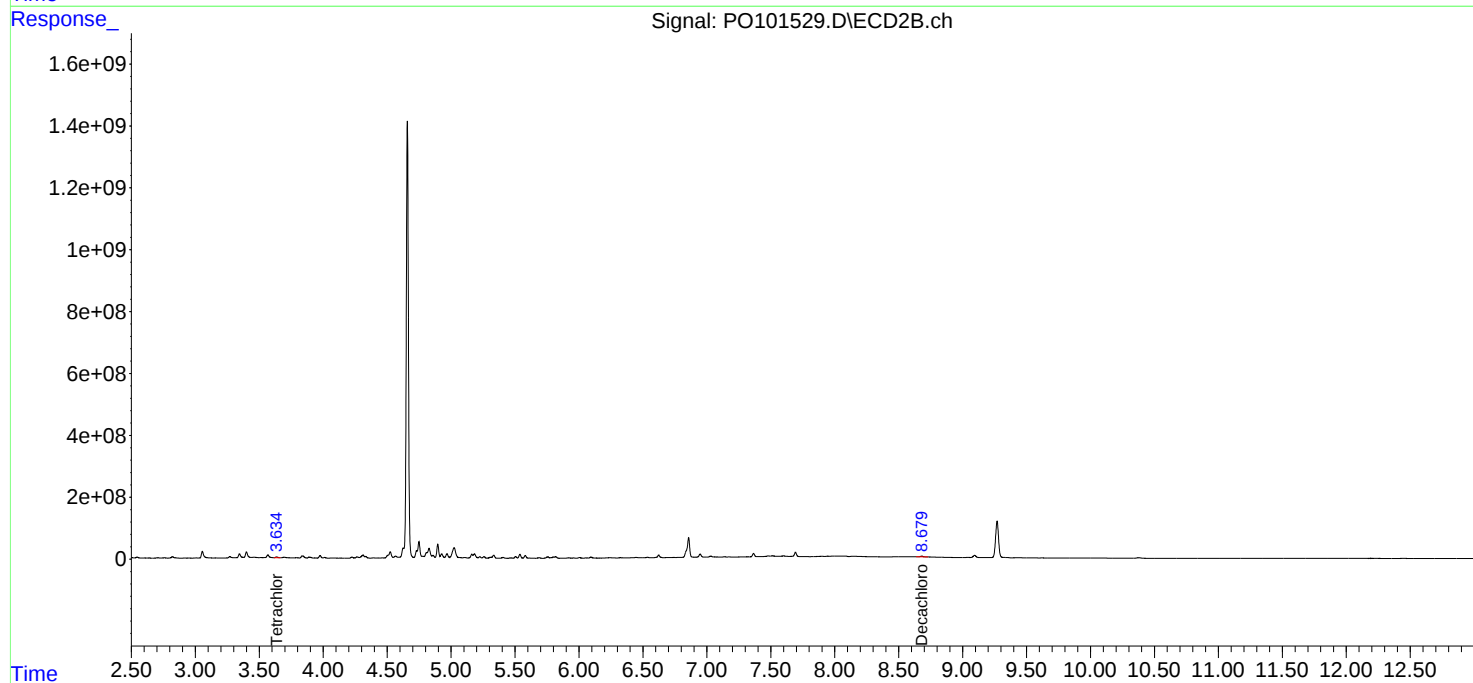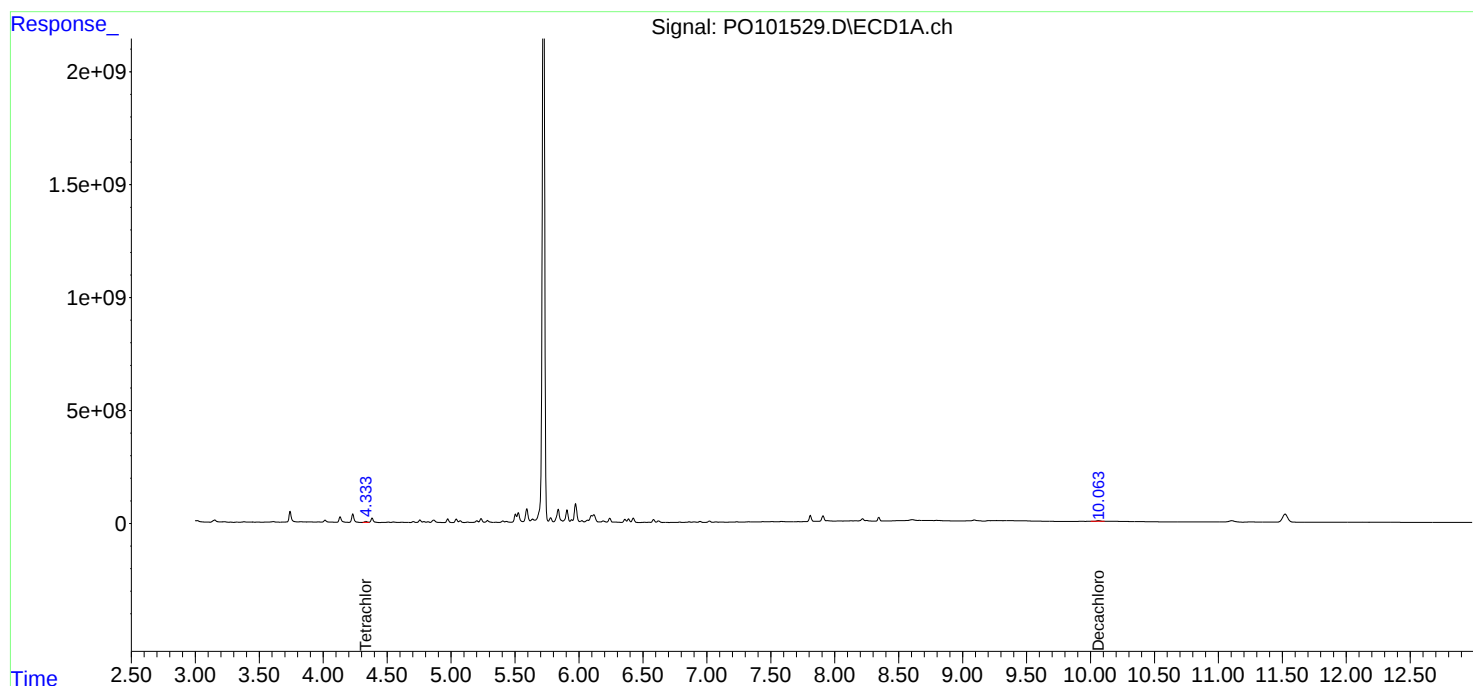

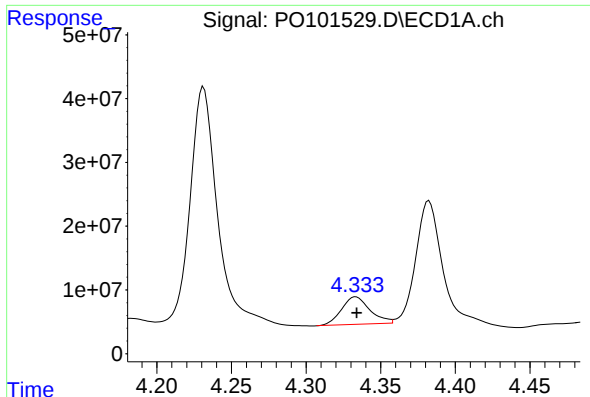


#1 Tetrachloro-m-xylene

R.T.: 4.333 min
Delta R.T.: -0.001 min
Response: 57448084
Conc: 14.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
19690


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

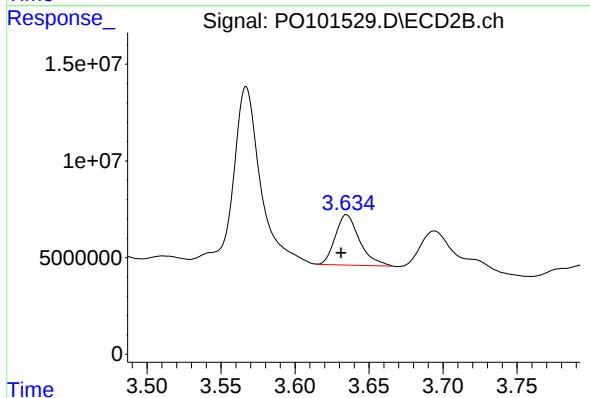


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.003 min
Response: 29779264
Conc: 11.52 ng/ml m

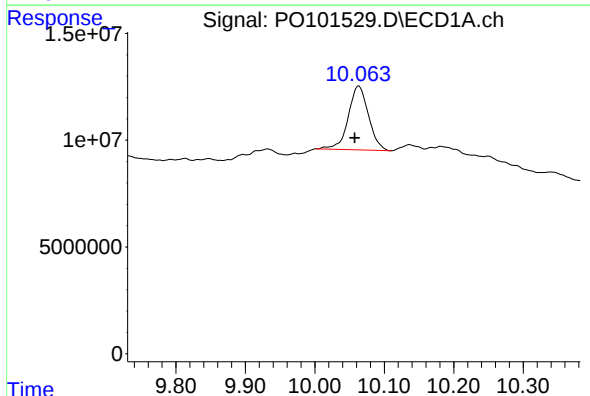

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: 0.006 min
Response: 60469211
Conc: 25.95 ng/ml

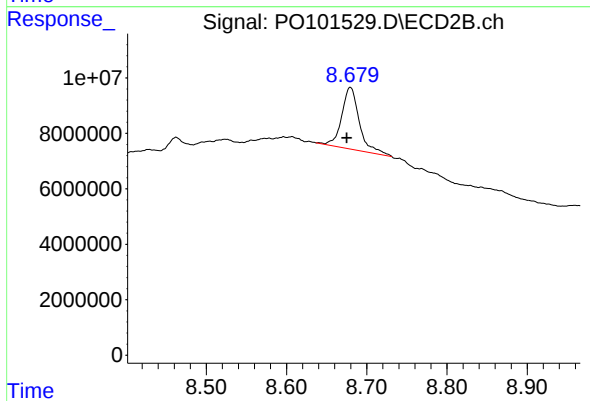

#2 Decachlorobiphenyl

R.T.: 8.680 min
Delta R.T.: 0.004 min
Response: 33500164
Conc: 17.68 ng/ml