

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020124\
 Data File : P0101563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 03:58
 Operator : YP/AJ
 Sample : P1315-03 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC278948LOK-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 06:29:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.627	7338621	4268116	1.912	1.652
2) SA Decachlor...	10.057	8.674	19009045	12118897	8.158	6.395m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020124\
Data File : PO101563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 03:58
Operator : YP/AJ
Sample : P1315-03 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC278948LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 06:29:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 24 04:51:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

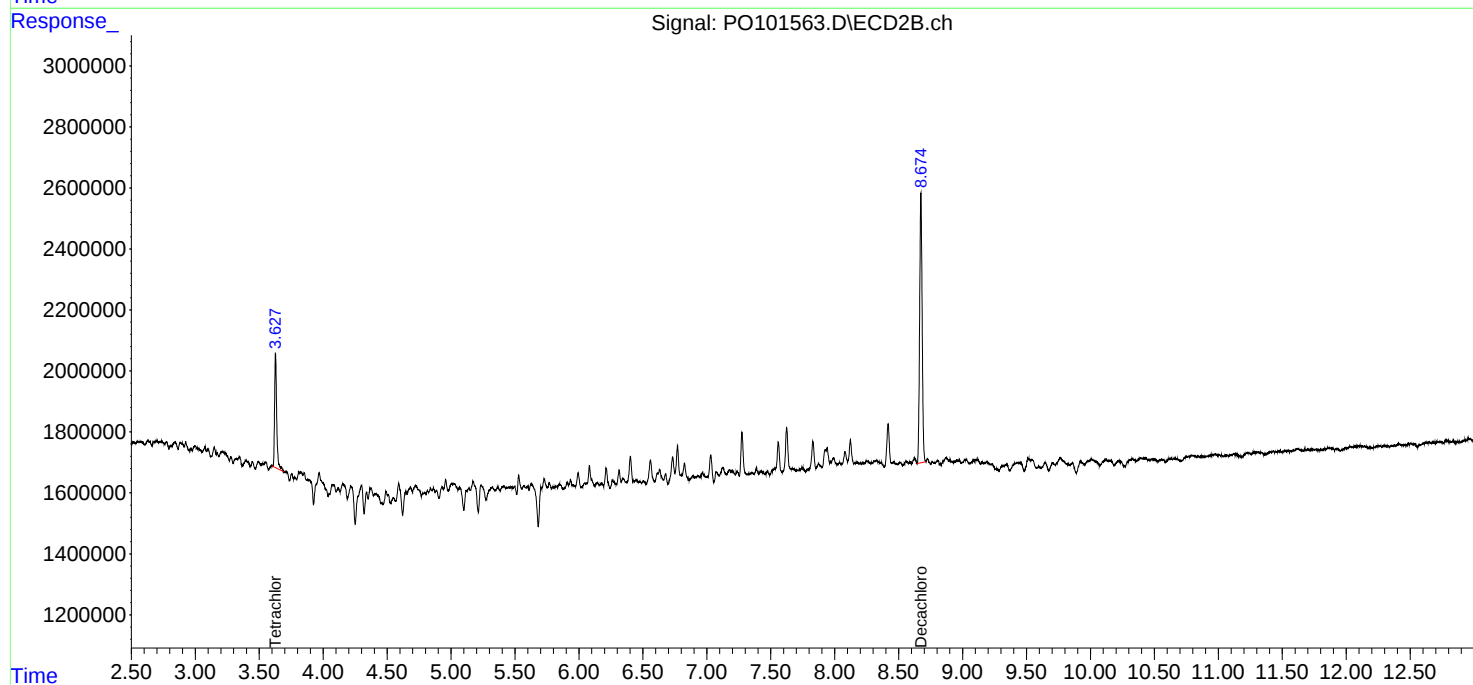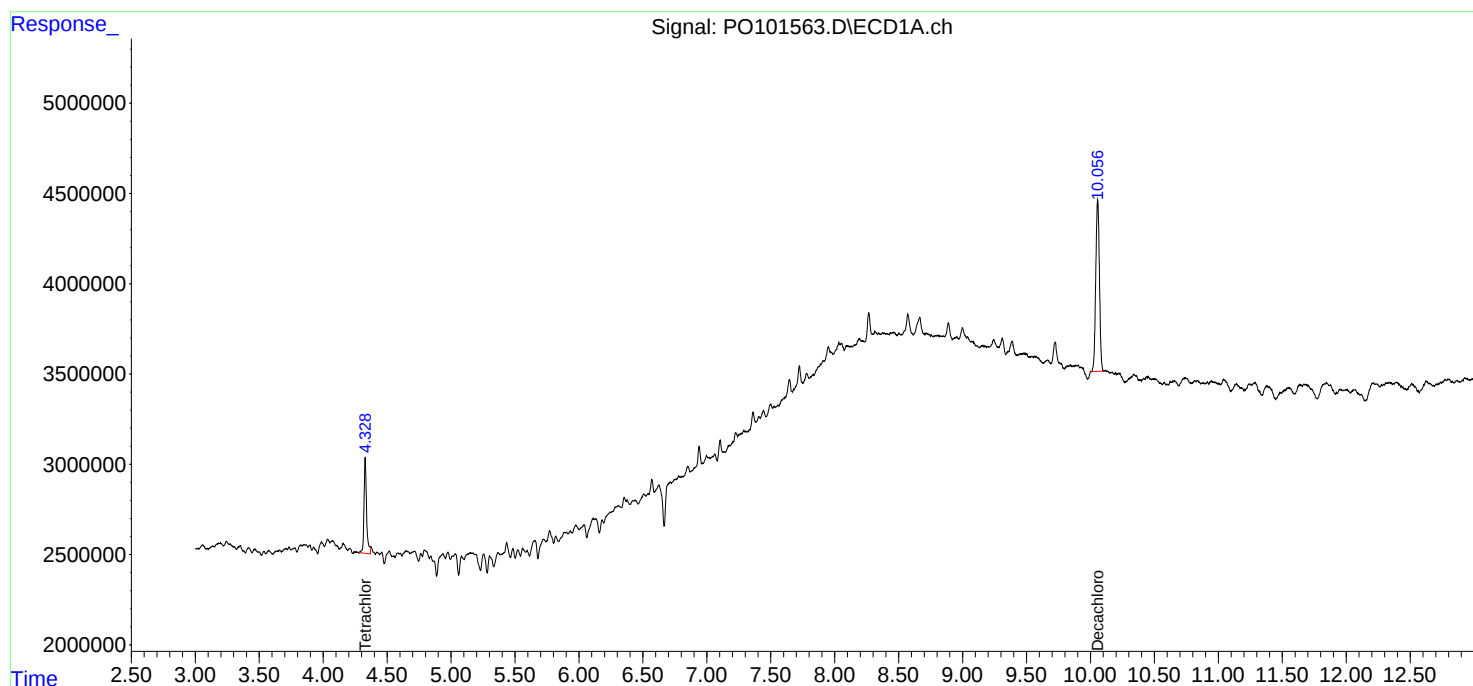

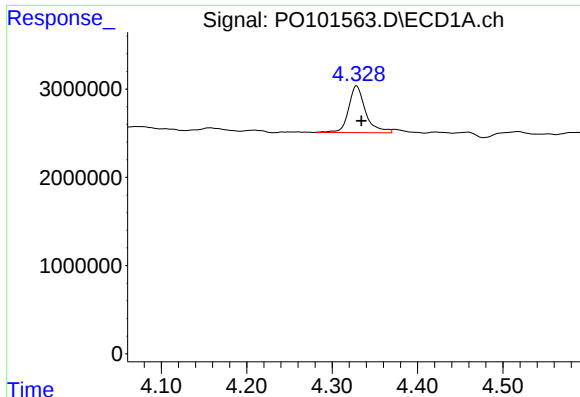


#1 Tetrachloro-m-xylene

R.T.: 4.329 min
Delta R.T.: -0.005 min
Response: 7338621
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC278948LOK-END-1-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

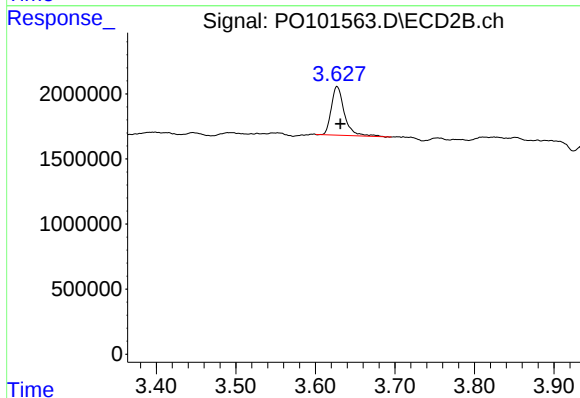


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: -0.004 min
Response: 4268116
Conc: 1.65 ng/ml

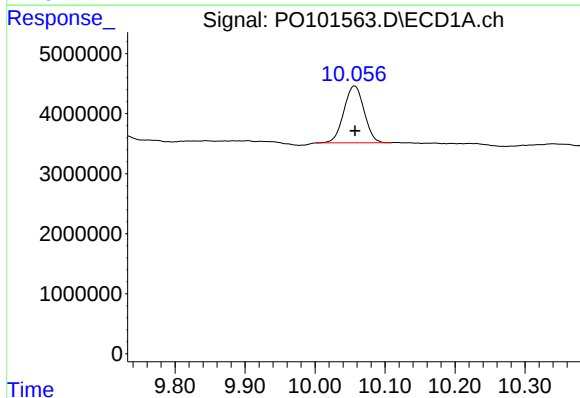

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: 0.000 min
Response: 19009045
Conc: 8.16 ng/ml

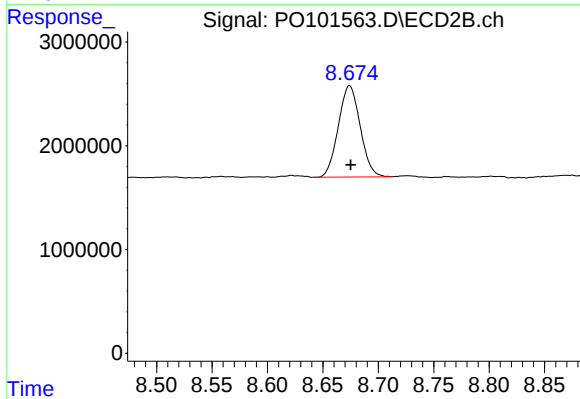

#2 Decachlorobiphenyl

R.T.: 8.674 min
Delta R.T.: -0.001 min
Response: 12118897
Conc: 6.40 ng/ml m