

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020124\
 Data File : P0101564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2024 04:14
 Operator : YP/AJ
 Sample : P1315-04 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC278948LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
 Supervised By :Sohil Jodhani 02/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 06:30:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.628	5508633	3481514	1.435	1.347
2) SA Decachlor...	10.055	8.673	4796457	3770659	2.058m	1.990m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020124\
Data File : PO101564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2024 04:14
Operator : YP/AJ
Sample : P1315-04 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC278948LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 06:30:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 24 04:51:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

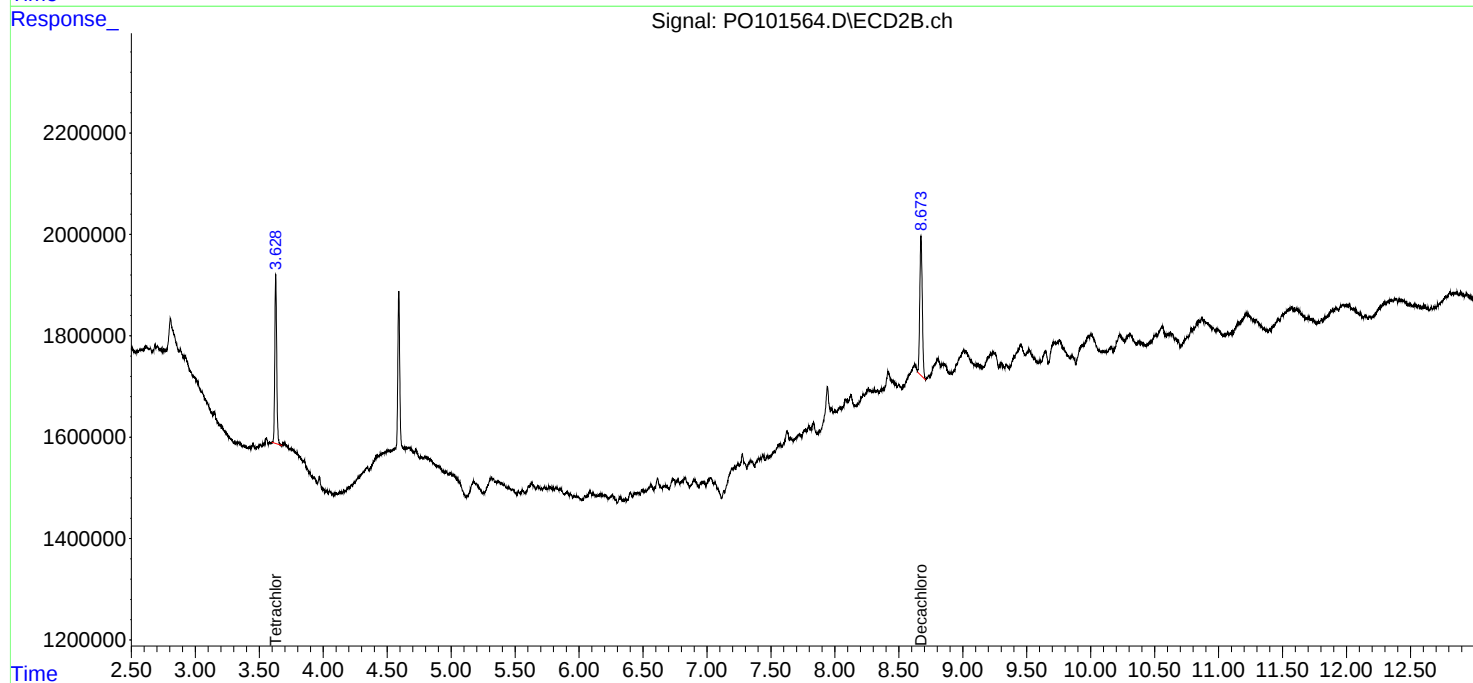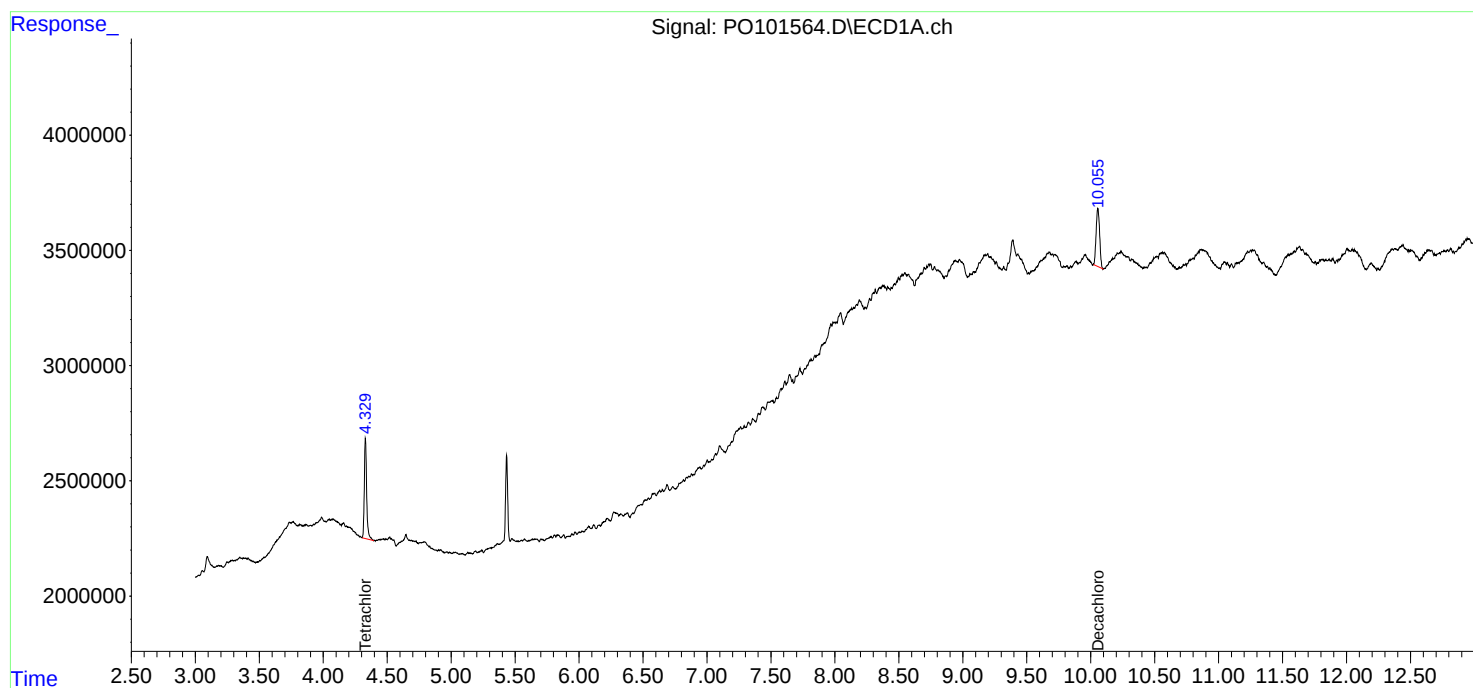

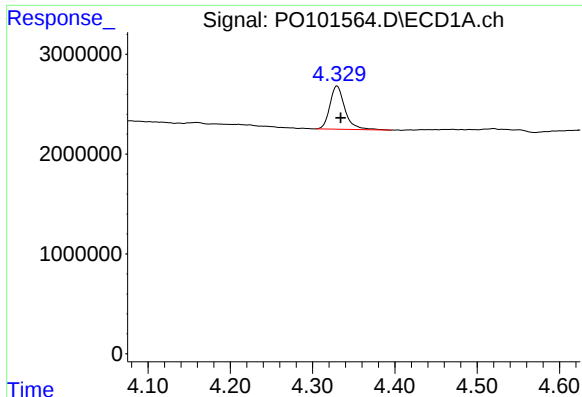


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: -0.004 min
Response: 5508633
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC278948LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/02/2024
Supervised By :Sohil Jodhani 02/02/2024

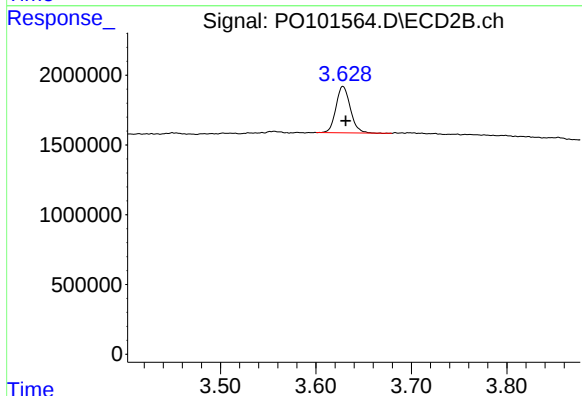


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.003 min
Response: 3481514
Conc: 1.35 ng/ml

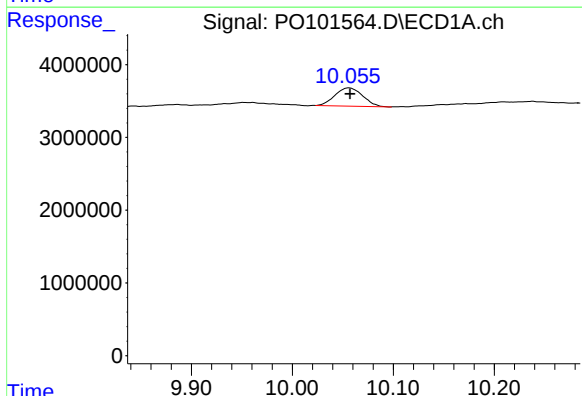

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: -0.002 min
Response: 4796457
Conc: 2.06 ng/ml m

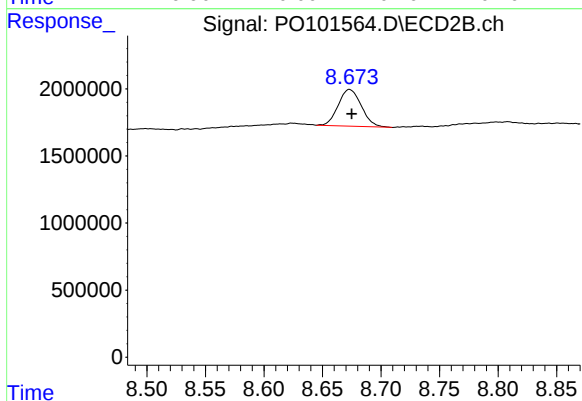

#2 Decachlorobiphenyl

R.T.: 8.673 min
Delta R.T.: -0.002 min
Response: 3770659
Conc: 1.99 ng/ml m