

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020223\
 Data File : P0092365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2023 13:39
 Operator : YP/AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/03/2023
 Supervised By :Ankita Jodhani 02/03/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 17:12:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.645	140.8E6	64577419	48.646	45.991
2) SA Decachlor...	10.369	8.686	104.6E6	54425372	50.660	48.211
Target Compounds						
26) L6 AR-1254-1	6.506	5.537	49928346	35720253	450.961	455.675
27) L6 AR-1254-2	6.729	5.684	78279878	31784946	481.561	459.381
28) L6 AR-1254-3	7.102	6.090	80311007	48401240	486.942	453.471
29) L6 AR-1254-4	7.395	6.320	53075325	26404223	485.214	448.332
30) L6 AR-1254-5	7.823	6.740	61901690	41770918	439.958m	458.943

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020223\
Data File : PO092365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2023 13:39
Operator : YP/AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2023
Supervised By :Ankita Jodhani 02/03/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 17:12:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

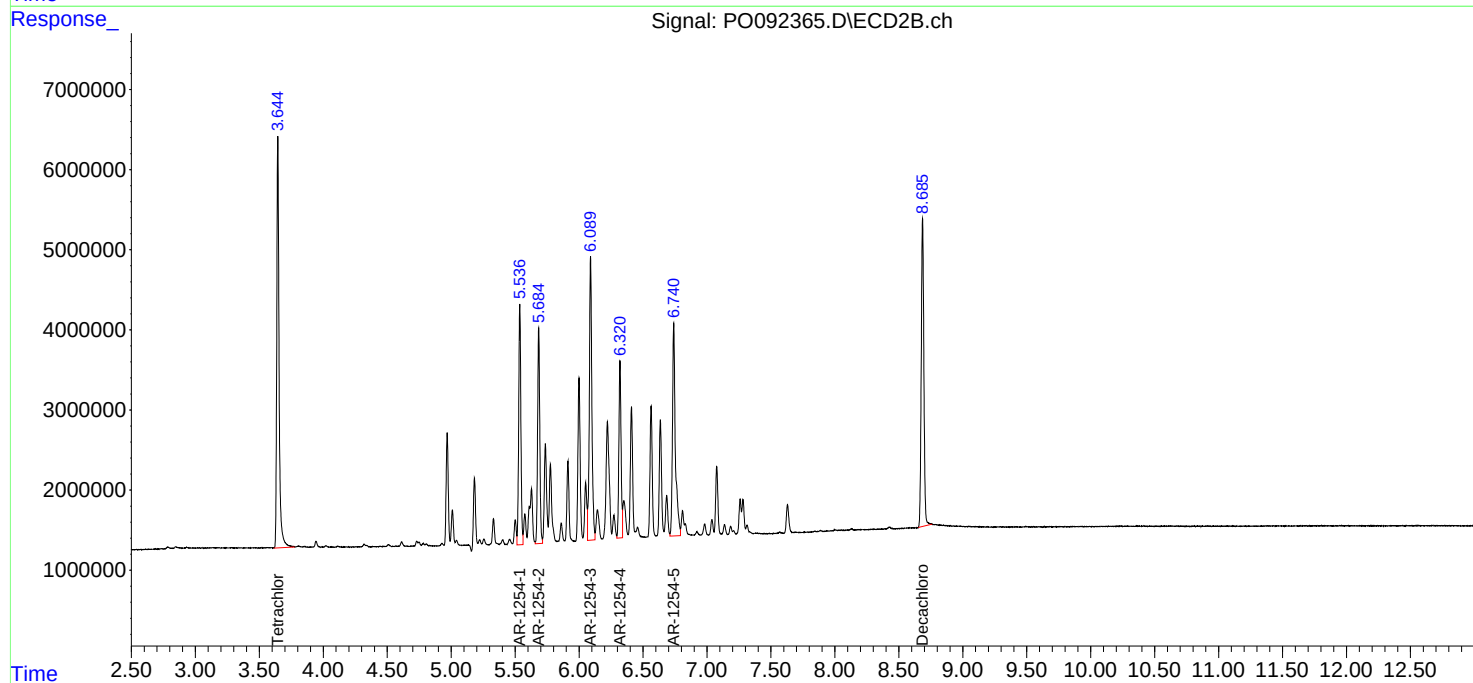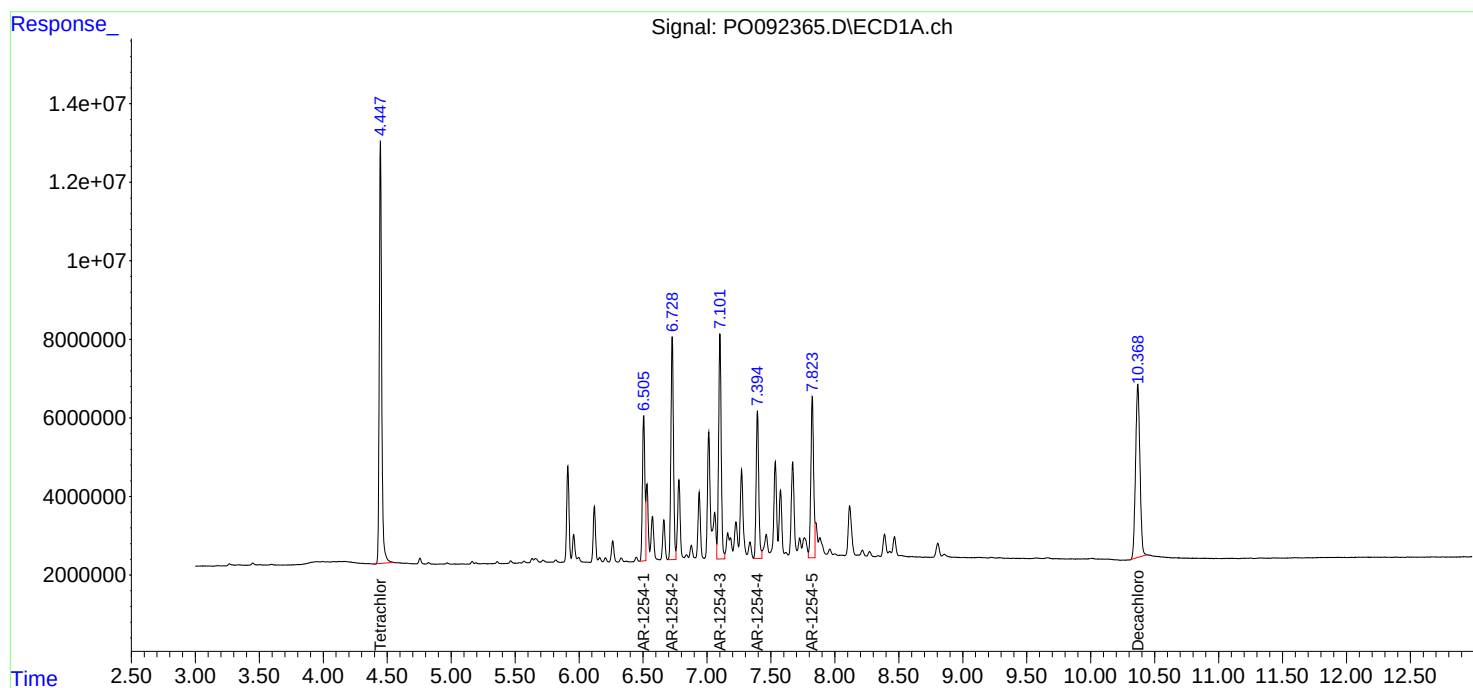

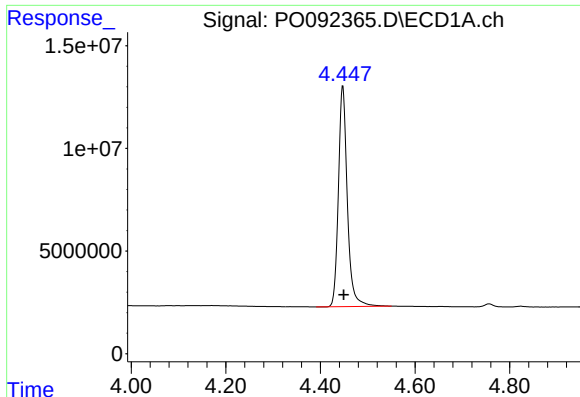


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: -0.002 min
Response: 140824998
Conc: 48.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2023
Supervised By :Ankita Jodhani 02/03/2023

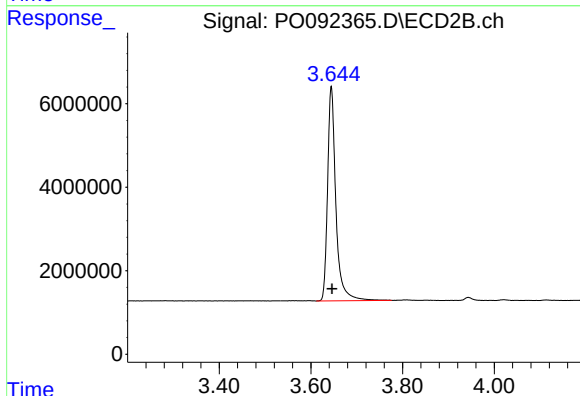


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.001 min
Response: 64577419
Conc: 45.99 ng/ml

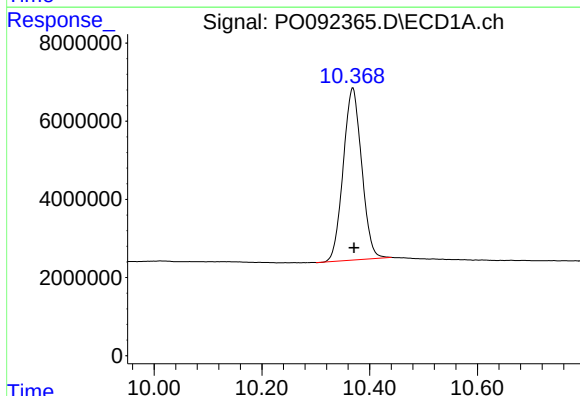


#2 Decachlorobiphenyl

R.T.: 10.369 min
Delta R.T.: -0.003 min
Response: 104559850
Conc: 50.66 ng/ml

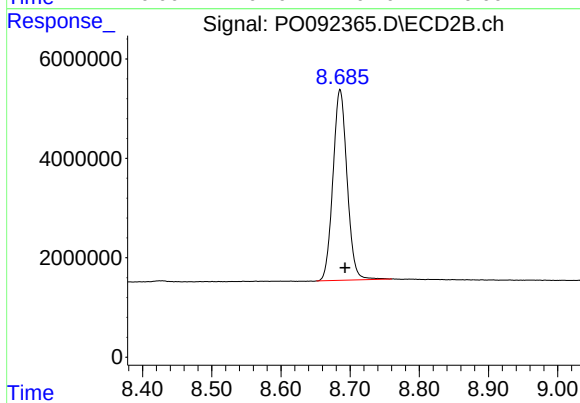

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.008 min
Response: 54425372
Conc: 48.21 ng/ml

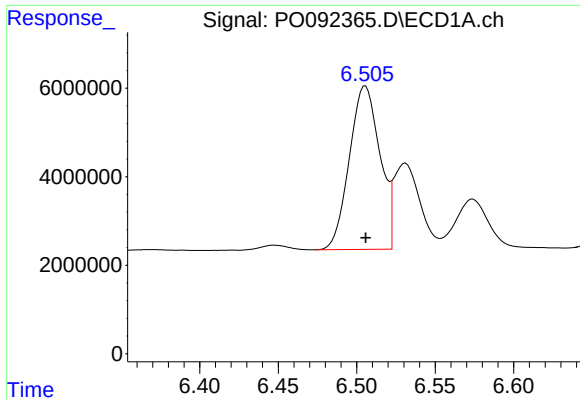


#26 AR-1254-1

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 49928346
Conc: 450.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2023
Supervised By :Ankita Jodhani 02/03/2023

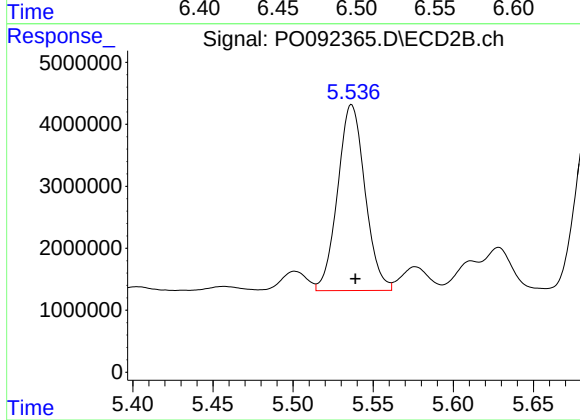


#26 AR-1254-1

R.T.: 5.537 min
Delta R.T.: -0.002 min
Response: 35720253
Conc: 455.68 ng/ml

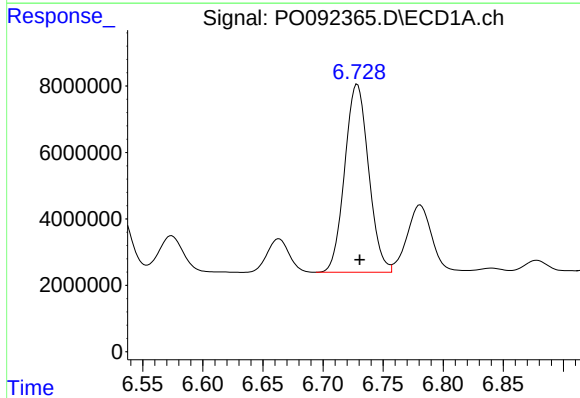


#27 AR-1254-2

R.T.: 6.729 min
Delta R.T.: -0.002 min
Response: 78279878
Conc: 481.56 ng/ml

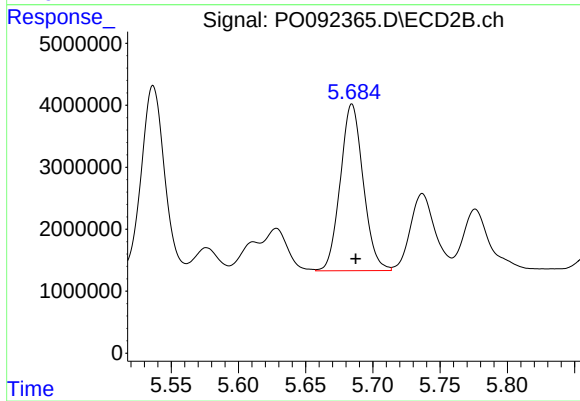

#27 AR-1254-2

R.T.: 5.684 min
Delta R.T.: -0.003 min
Response: 31784946
Conc: 459.38 ng/ml

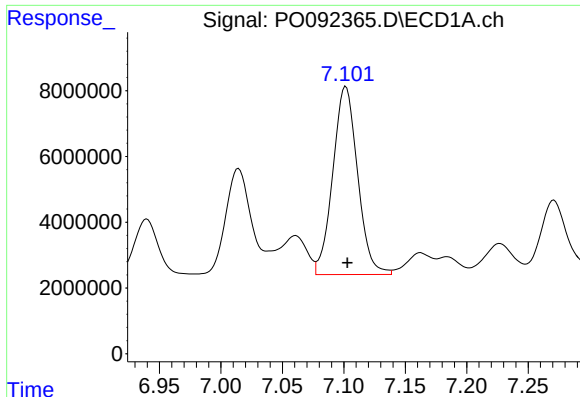


#28 AR-1254-3

R.T.: 7.102 min
Delta R.T.: -0.001 min
Response: 80311007
Conc: 486.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2023
Supervised By :Ankita Jodhani 02/03/2023

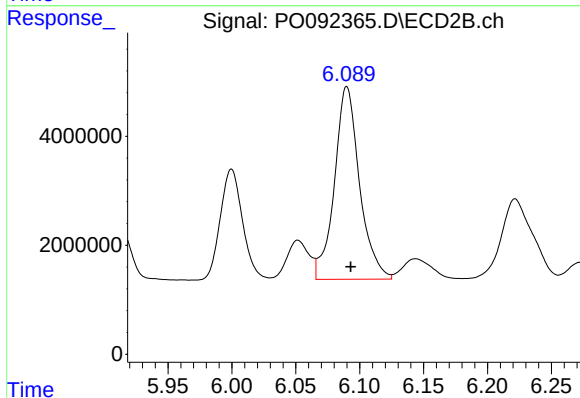


#28 AR-1254-3

R.T.: 6.090 min
Delta R.T.: -0.003 min
Response: 48401240
Conc: 453.47 ng/ml

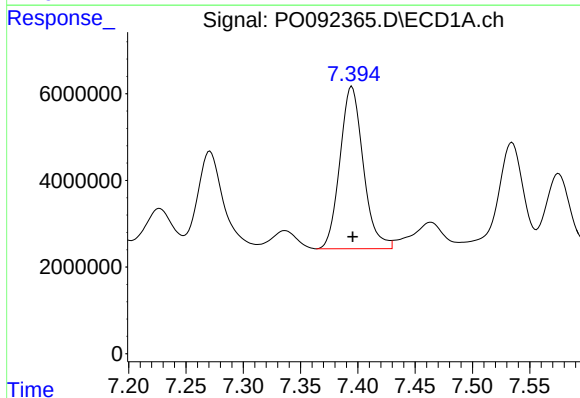


#29 AR-1254-4

R.T.: 7.395 min
Delta R.T.: 0.000 min
Response: 53075325
Conc: 485.21 ng/ml

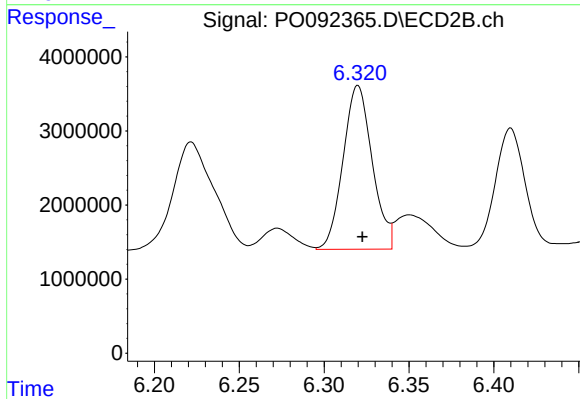

#29 AR-1254-4

R.T.: 6.320 min
Delta R.T.: -0.003 min
Response: 26404223
Conc: 448.33 ng/ml

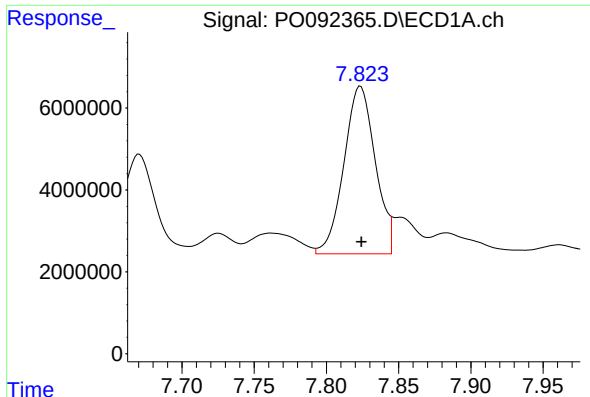


#30 AR-1254-5

R.T.: 7.823 min
Delta R.T.: -0.001 min
Response: 61901690
Conc: 439.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2023
Supervised By :Ankita Jodhani 02/03/2023

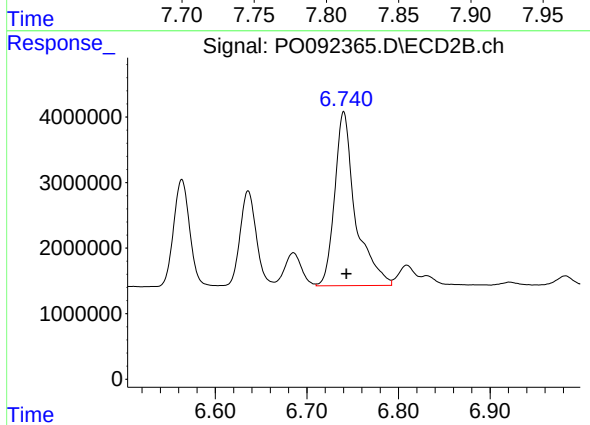

#30 AR-1254-5

R.T.: 6.740 min
Delta R.T.: -0.003 min
Response: 41770918
Conc: 458.94 ng/ml