

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020320\
 Data File : P0066195.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2020 10:17
 Operator : DD\AJ
 Sample : L1329-18RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-11RE

Manual Integrations
 APPROVED

mohammad
 2/5/2020 3:27:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 16:41:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.150	3.426	382444	470672	13.128m	11.507m
2) SA Decachlor...	9.646	8.323	133871	223324	3.397	3.810

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020320\
Data File : P0066195.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2020 10:17
Operator : DD\AJ
Sample : L1329-18RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-11RE


Manual Integrations
APPROVED

mohammad
2/5/2020 3:27:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 16:41:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

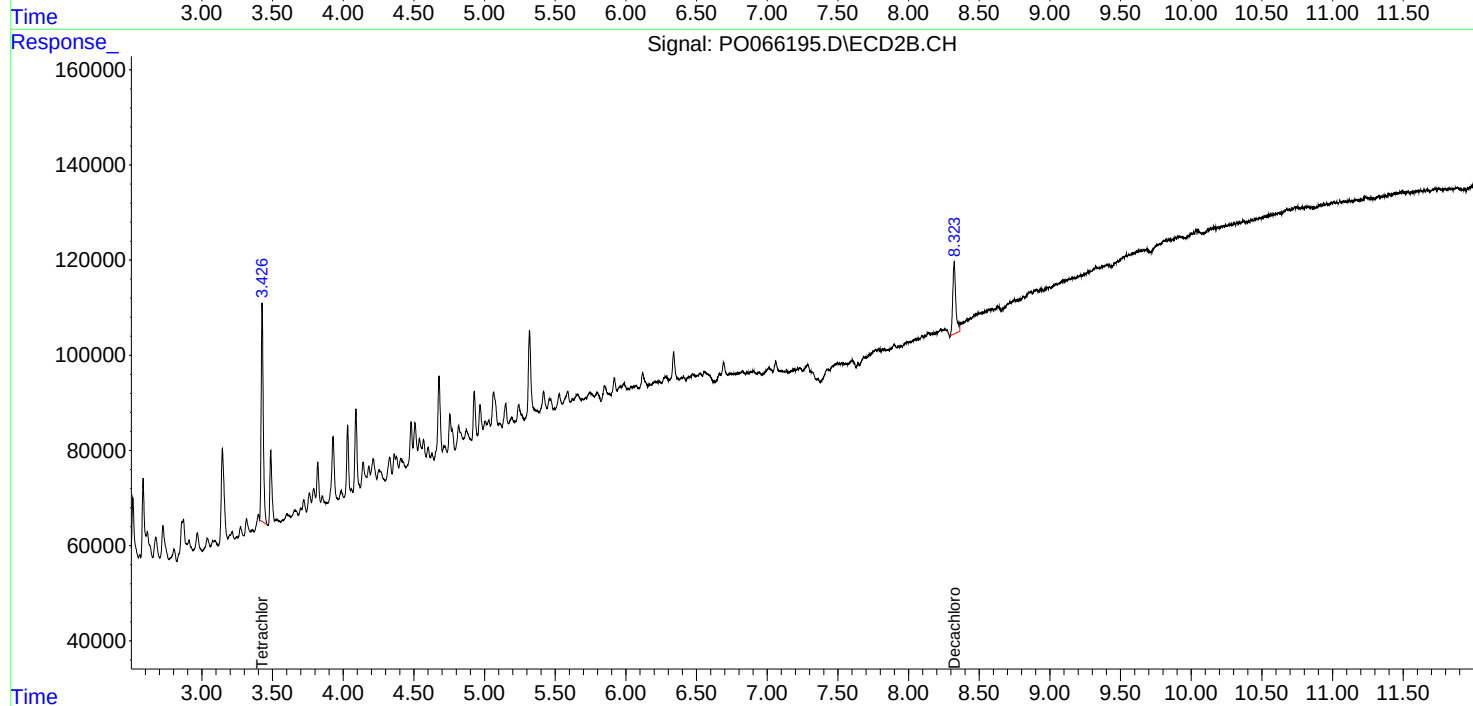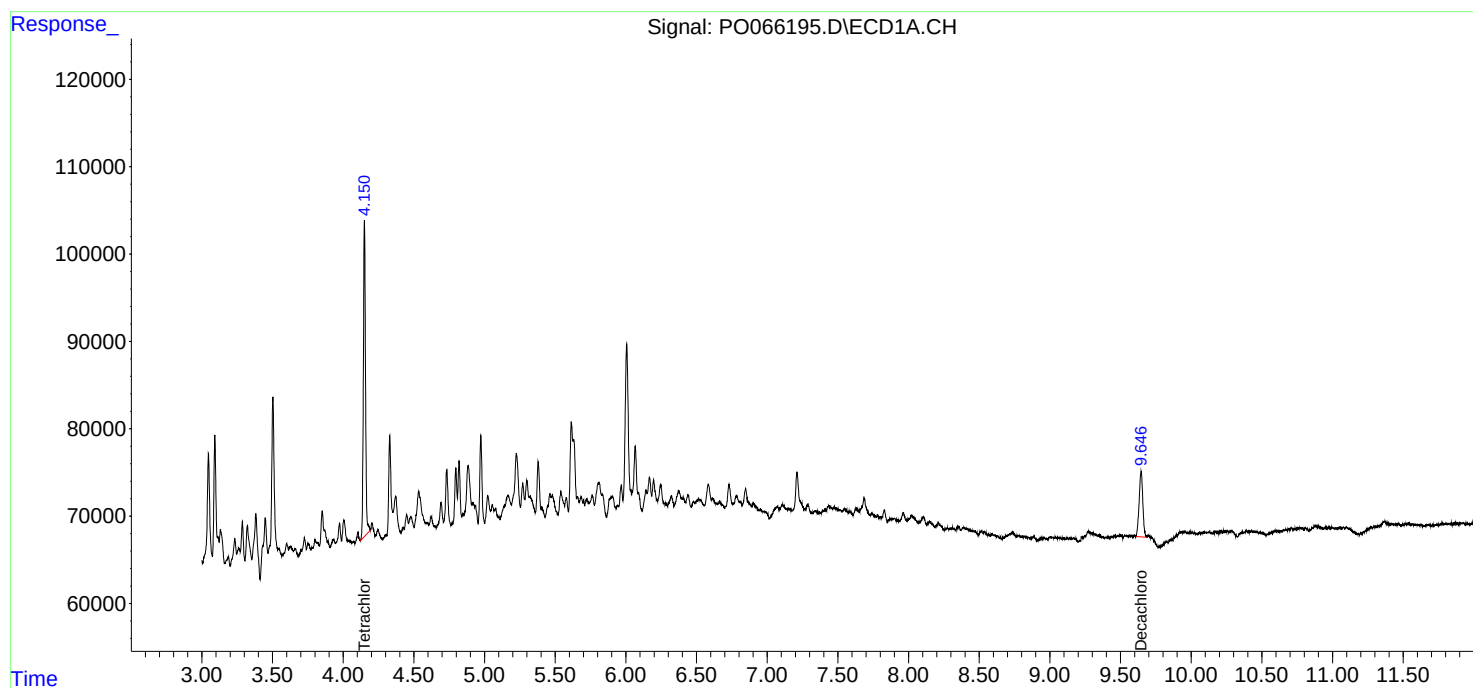

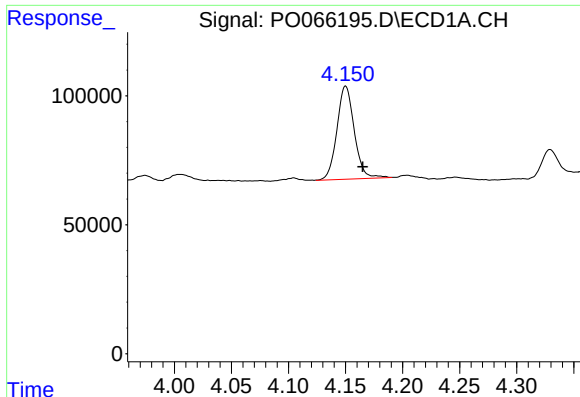


#1 Tetrachloro-m-xylene

R.T.: 4.150 min
Delta R.T.: -0.015 min
Response: 382444
Conc: 13.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-11RE


Manual Integrations
APPROVED

mohammad
2/5/2020 3:27:49 PM

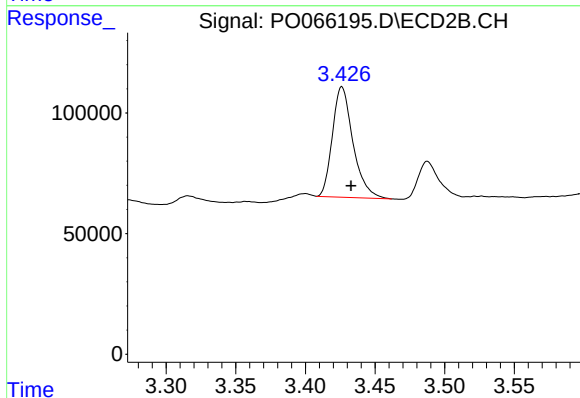


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: -0.007 min
Response: 470672
Conc: 11.51 ng/ml m

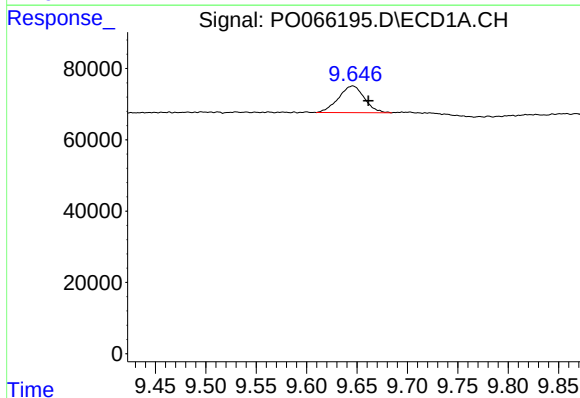

#2 Decachlorobiphenyl

R.T.: 9.646 min
Delta R.T.: -0.015 min
Response: 133871
Conc: 3.40 ng/ml

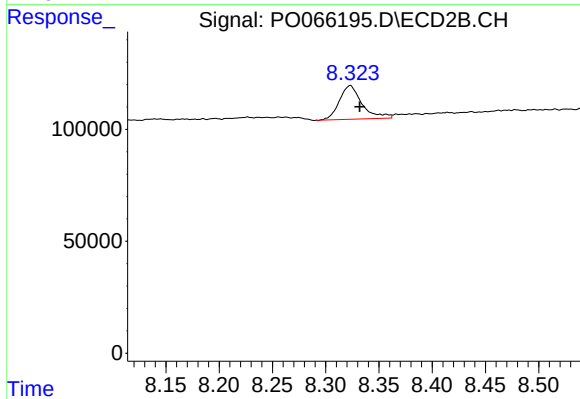

#2 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.009 min
Response: 223324
Conc: 3.81 ng/ml