

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020320\
 Data File : P0066197.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2020 11:10
 Operator : DD\AJ
 Sample : L1329-14 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40634

Manual Integrations
 APPROVED

mohammad
 2/5/2020 3:27:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 16:42:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.428	150466	98736	5.165m	2.414 #
2) SA Decachlor...	9.644	8.322	152500	200261	3.870	3.417

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020320\
Data File : P0066197.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2020 11:10
Operator : DD\AJ
Sample : L1329-14 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
40634


Manual Integrations
APPROVED

mohammad
2/5/2020 3:27:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 16:42:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

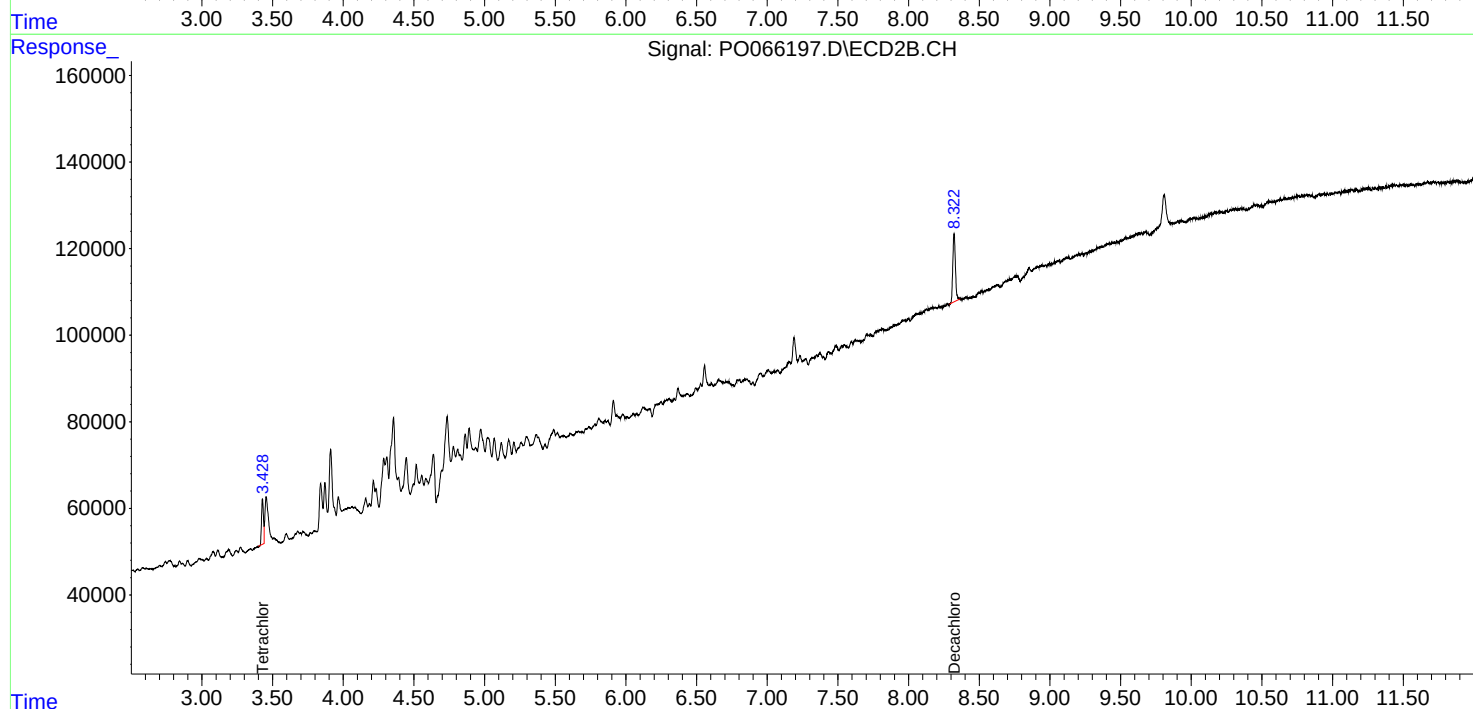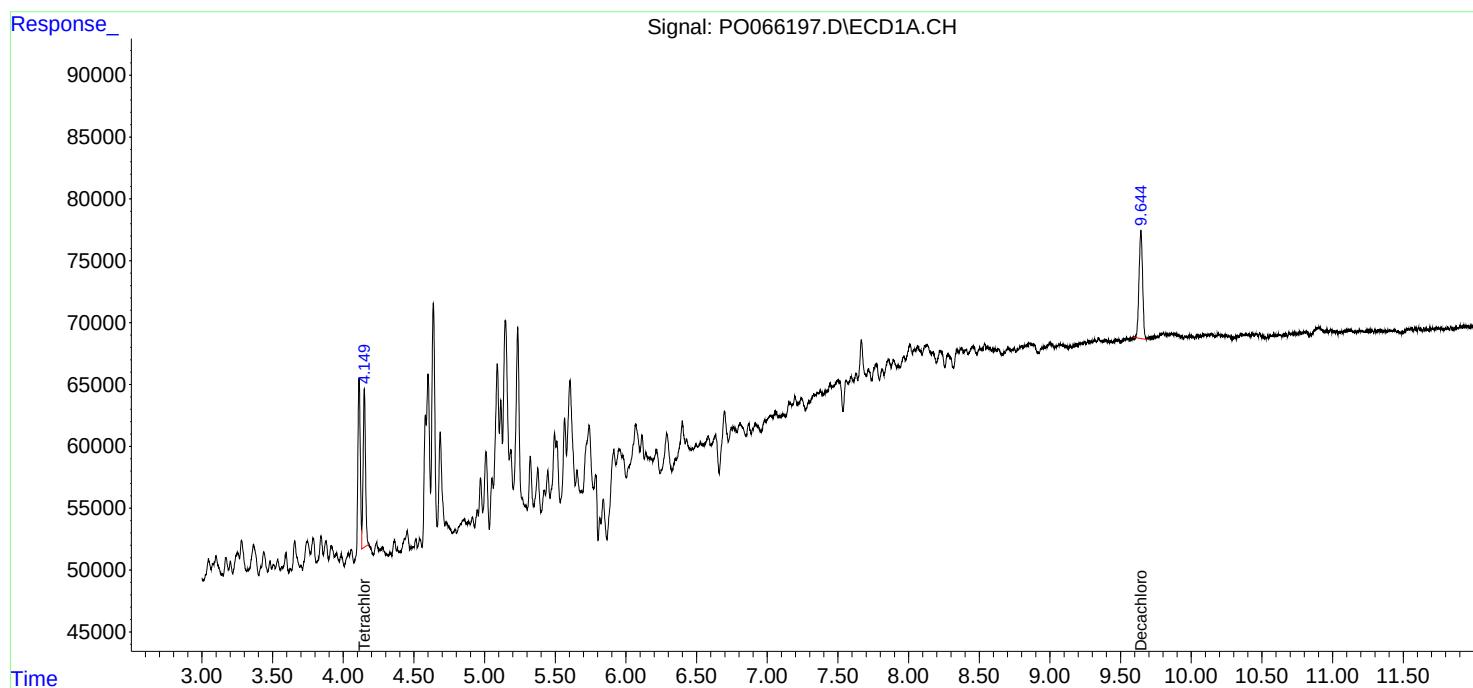

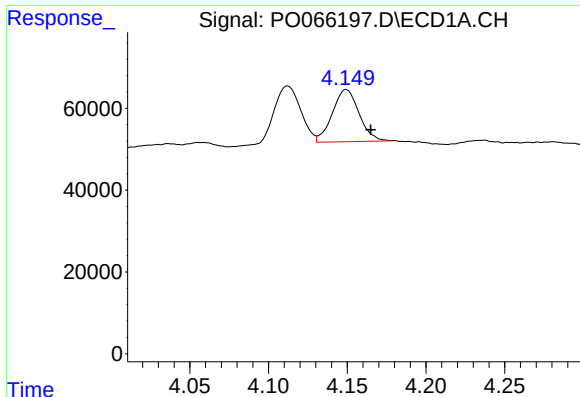


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: -0.016 min
Response: 150466
Conc: 5.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40634


Manual Integrations
APPROVED

mohammad
2/5/2020 3:27:55 PM

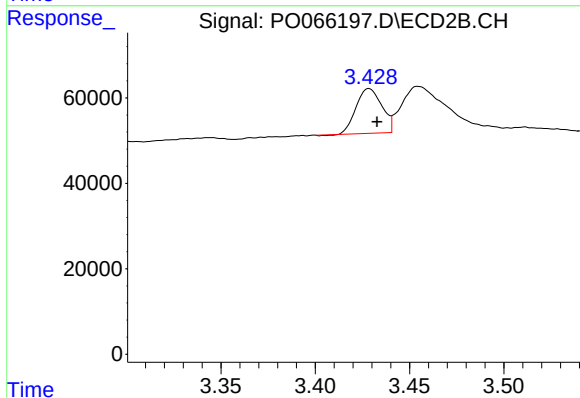


#1 Tetrachloro-m-xylene

R.T.: 3.428 min
Delta R.T.: -0.004 min
Response: 98736
Conc: 2.41 ng/ml

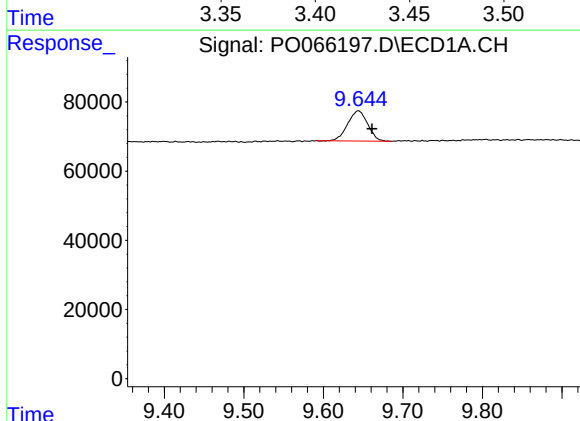

#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.017 min
Response: 152500
Conc: 3.87 ng/ml

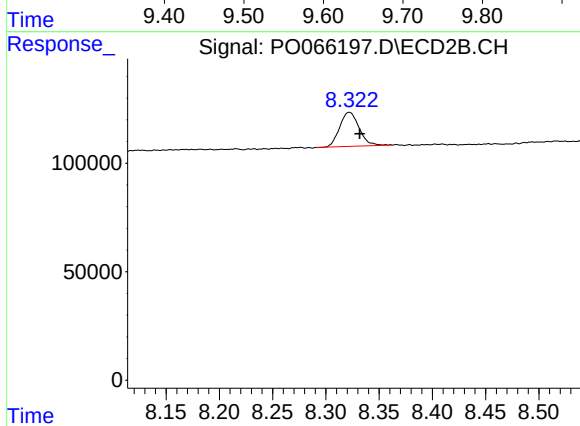

#2 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.010 min
Response: 200261
Conc: 3.42 ng/ml