

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020320\
 Data File : P0066203.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2020 13:50
 Operator : DD\AJ
 Sample : L1332-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KIT-SINK-1ST-DRAW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 16:43:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.426	430985	617394	14.795	15.094
2) SA Decachlor...	9.641	8.322	542350	757697	13.762	12.928

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020320\
Data File : P0066203.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2020 13:50
Operator : DD\AJ
Sample : L1332-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KIT-SINK-1ST-DRAW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 16:43:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

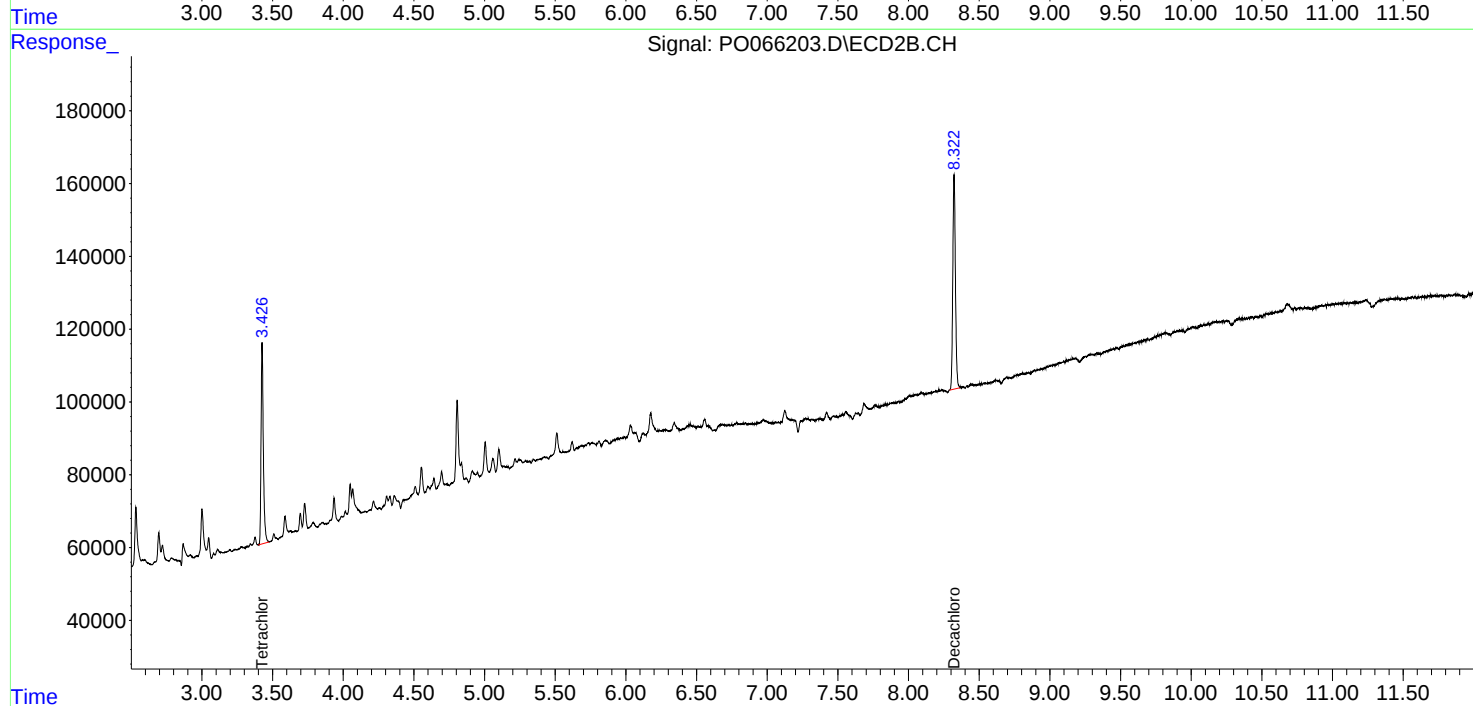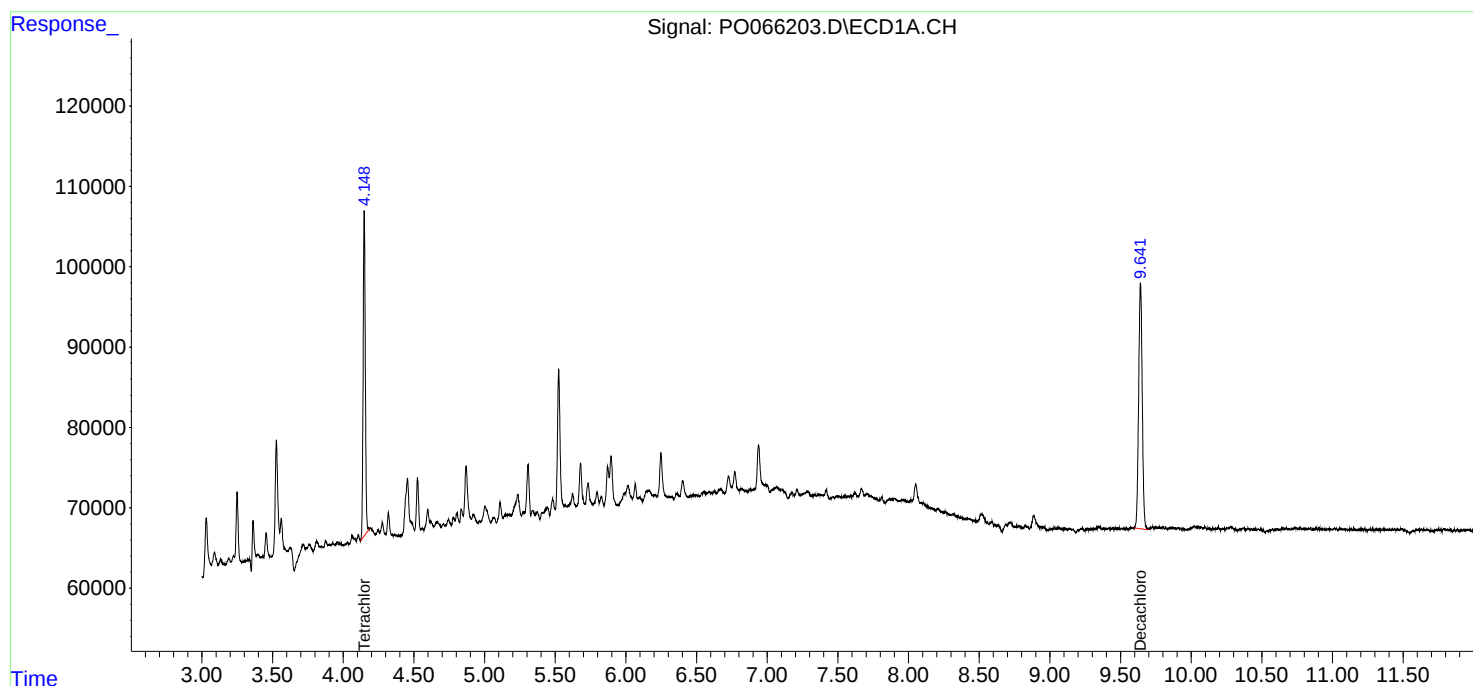


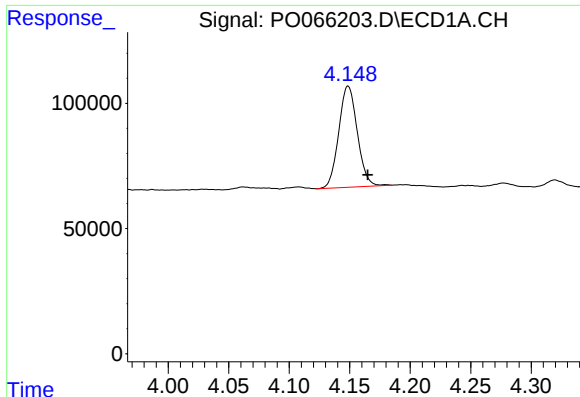

#1 Tetrachloro-m-xylene


R.T.: 4.149 min
Delta R.T.: -0.016 min
Response: 430985
Conc: 14.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
KIT-SINK-1ST-DRAW

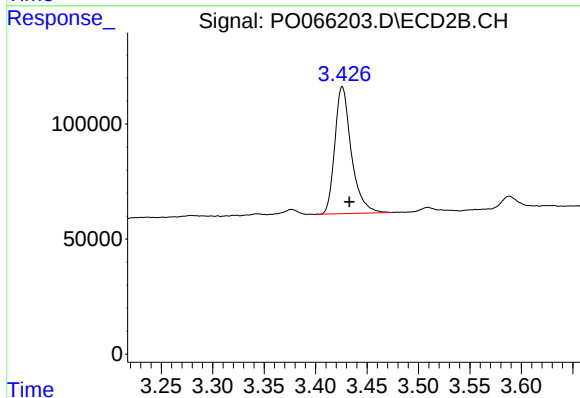


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: -0.007 min
Response: 617394
Conc: 15.09 ng/ml

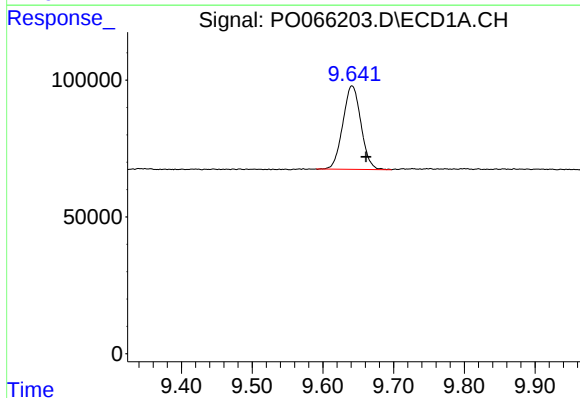

#2 Decachlorobiphenyl

R.T.: 9.641 min
Delta R.T.: -0.020 min
Response: 542350
Conc: 13.76 ng/ml

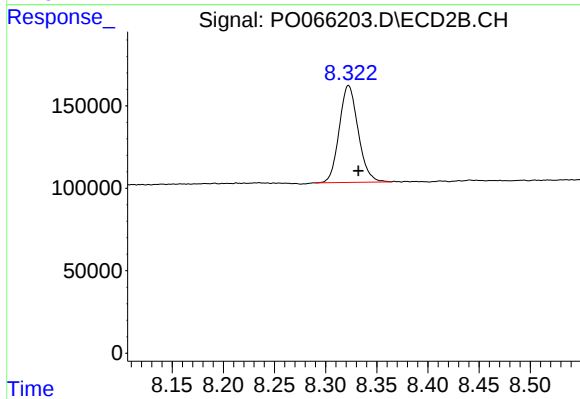

#2 Decachlorobiphenyl

R.T.: 8.322 min
Delta R.T.: -0.010 min
Response: 757697
Conc: 12.93 ng/ml