

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075425.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2021 11:09
 Operator : AJ/MA
 Sample : M1264-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-01-F

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:49:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 13:05:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.994	2029090	1019536	20.050m	21.209
2) SA Decachlor...	10.942	9.245	1279465	666043	13.261	13.721m
Target Compounds						
26) L6 AR-1254-1	7.162	6.103	1459213	910188	338.574	293.877
27) L6 AR-1254-2	7.391	6.262	2880149	1260858	427.185	469.534
28) L6 AR-1254-3	7.776	6.678	4146153	2347937	601.231	550.642
29) L6 AR-1254-4	8.072	6.916	3704631	1678019	612.790	575.710
30) L6 AR-1254-5	8.501	7.342	5512379	8242461	986.136m	2123.728 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO075425.D
Data File : PO075425.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2021 11:09
Operator : AJ/MA
Sample : M1264-07
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-01-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 13:05:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

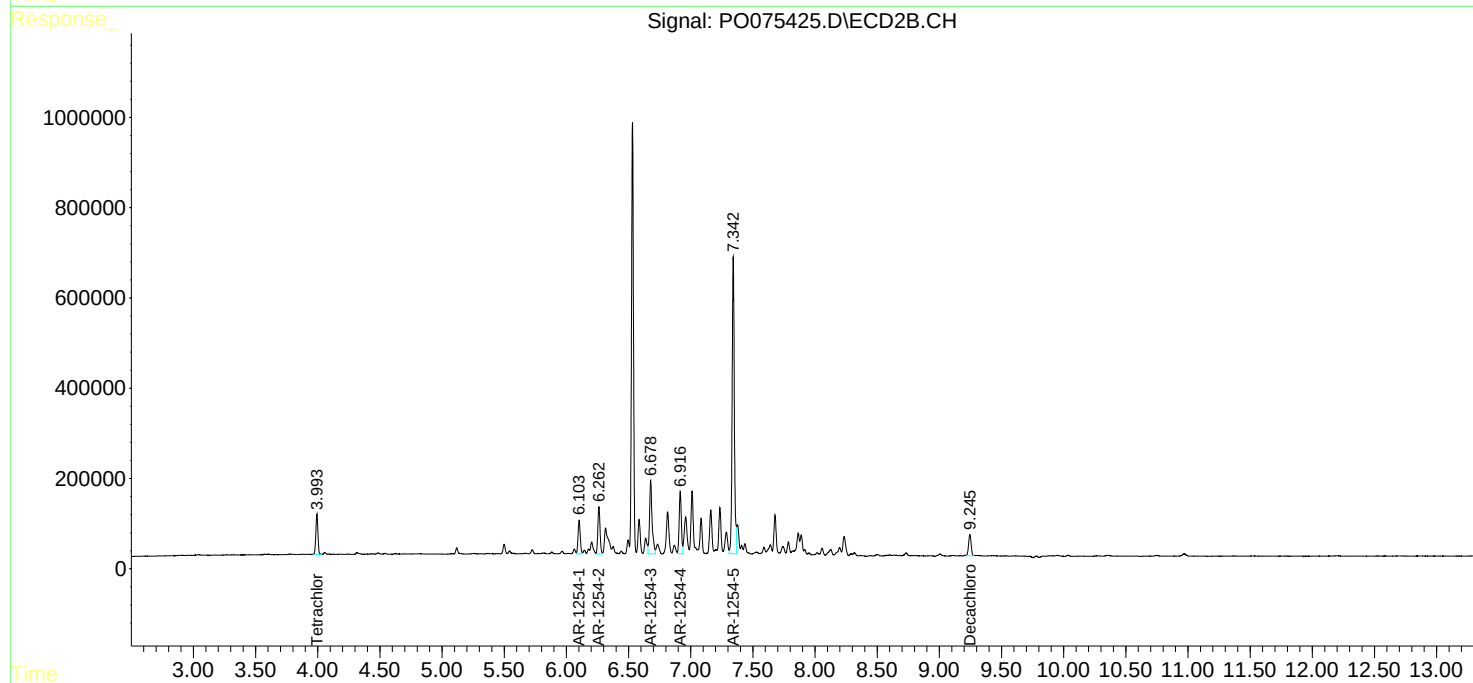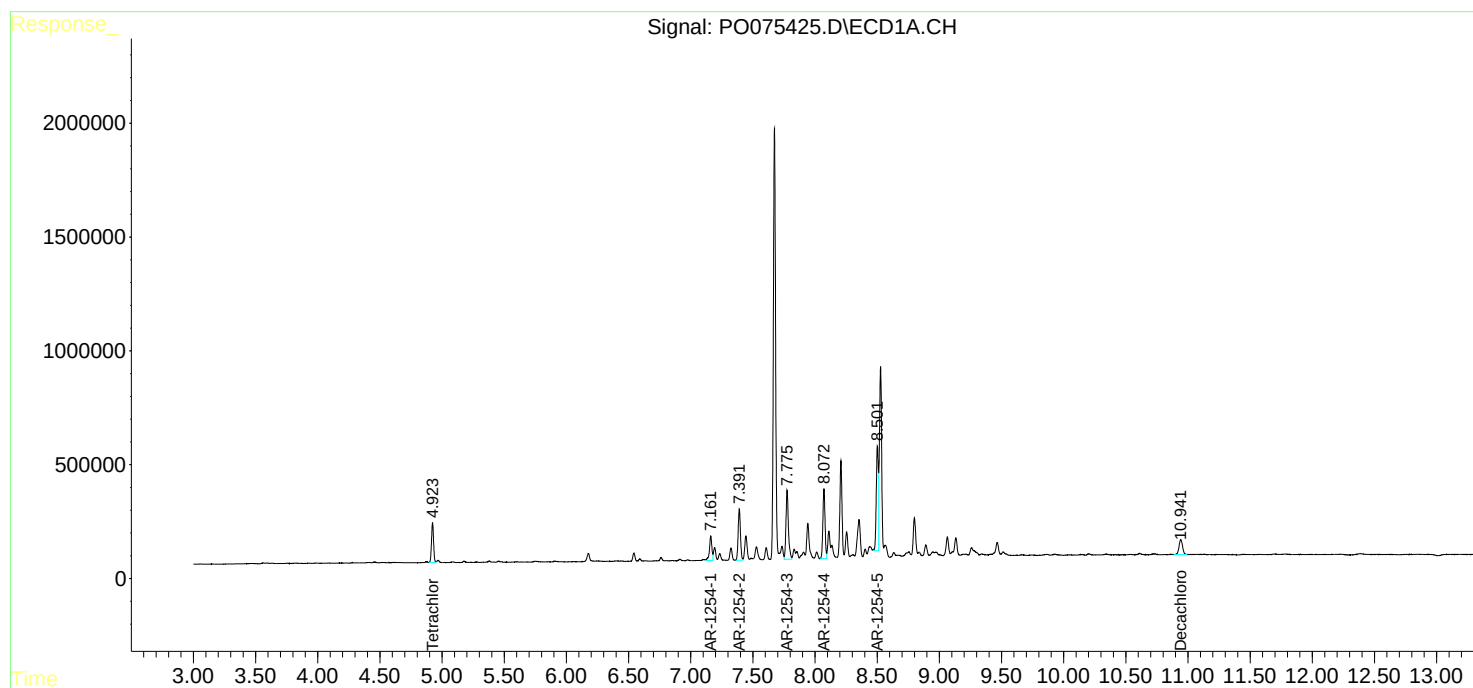

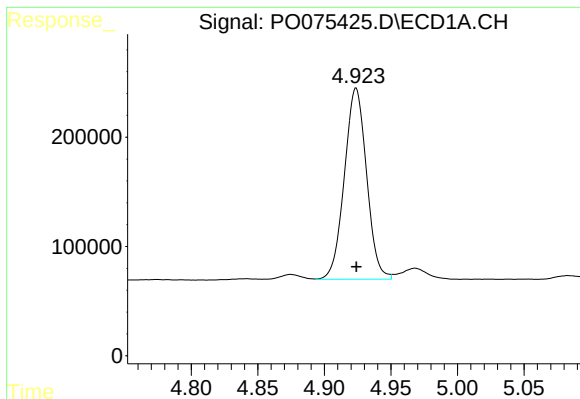


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 2029090
Conc: 20.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S1-01-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:36 PM

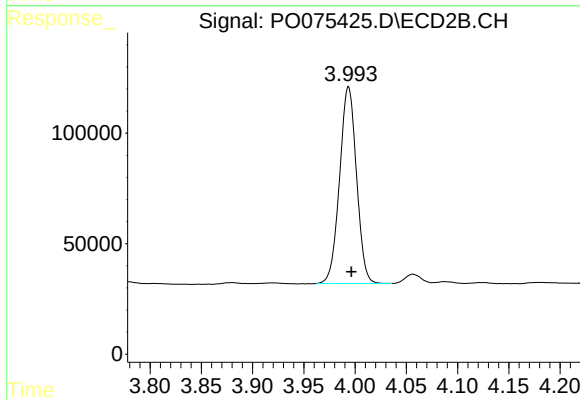


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.003 min
Response: 1019536
Conc: 21.21 ng/ml

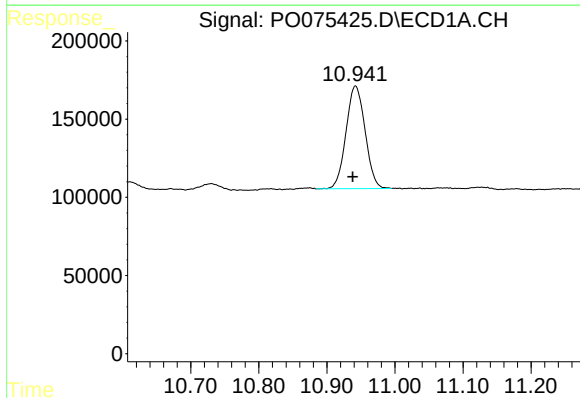


#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: 0.004 min
Response: 1279465
Conc: 13.26 ng/ml

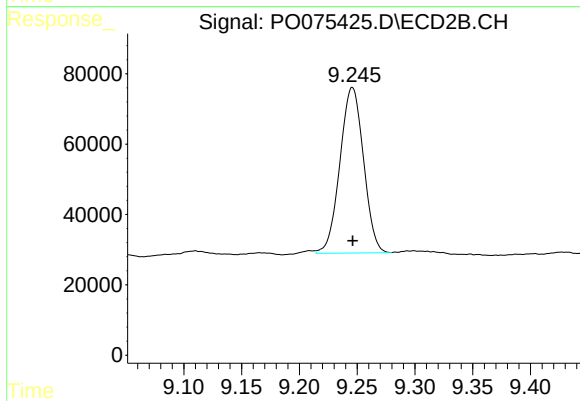

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: 0.000 min
Response: 666043
Conc: 13.72 ng/ml m

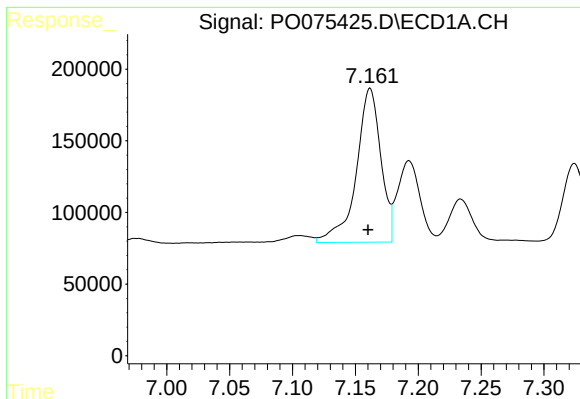


#26 AR-1254-1

R.T.: 7.162 min
Delta R.T.: 0.002 min
Response: 1459213
Conc: 338.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:36 PM

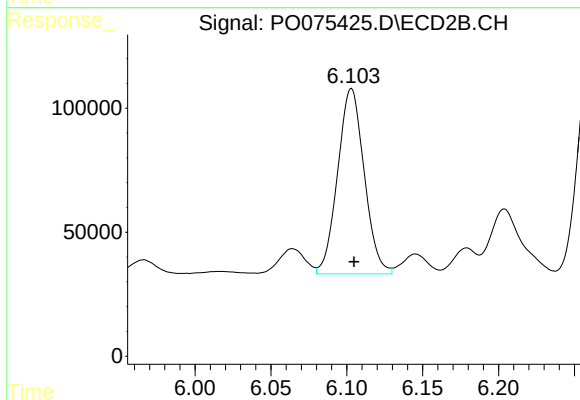


#26 AR-1254-1

R.T.: 6.103 min
Delta R.T.: -0.002 min
Response: 910188
Conc: 293.88 ng/ml

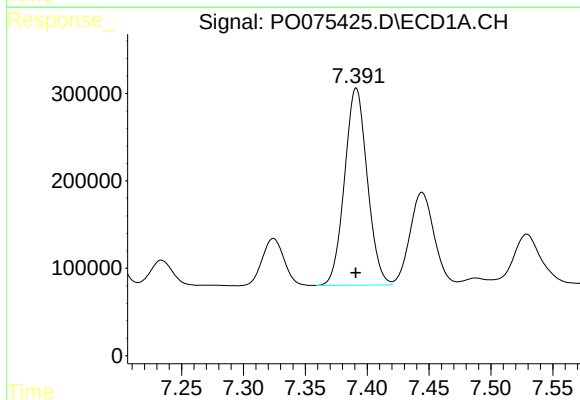


#27 AR-1254-2

R.T.: 7.391 min
Delta R.T.: 0.000 min
Response: 2880149
Conc: 427.19 ng/ml

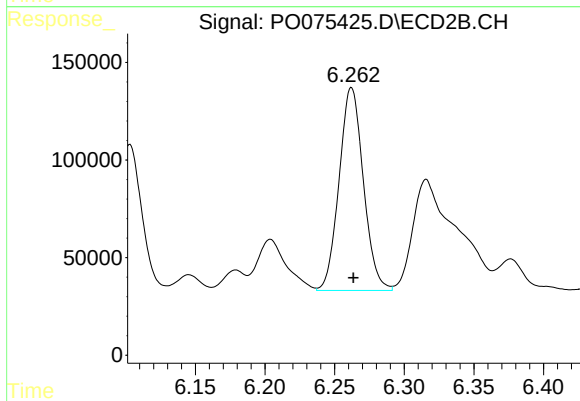

#27 AR-1254-2

R.T.: 6.262 min
Delta R.T.: -0.001 min
Response: 1260858
Conc: 469.53 ng/ml

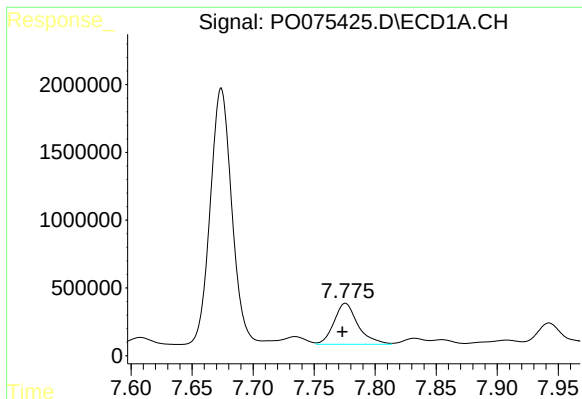


#28 AR-1254-3

R.T.: 7.776 min
Delta R.T.: 0.002 min
Response: 4146153
Conc: 601.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:36 PM

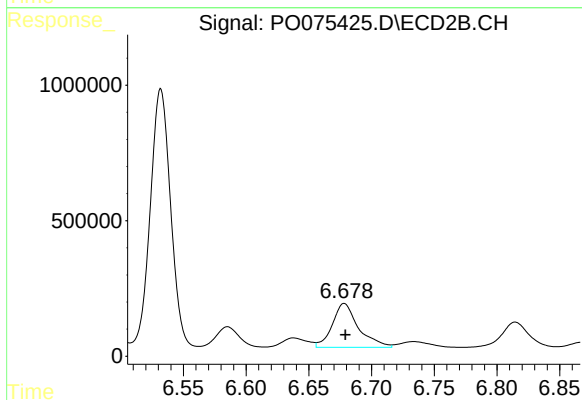


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 2347937
Conc: 550.64 ng/ml

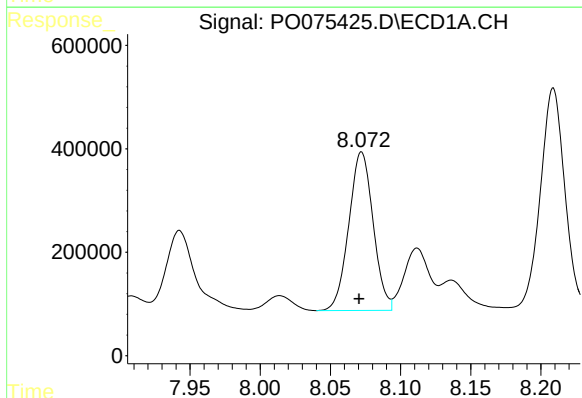


#29 AR-1254-4

R.T.: 8.072 min
Delta R.T.: 0.002 min
Response: 3704631
Conc: 612.79 ng/ml

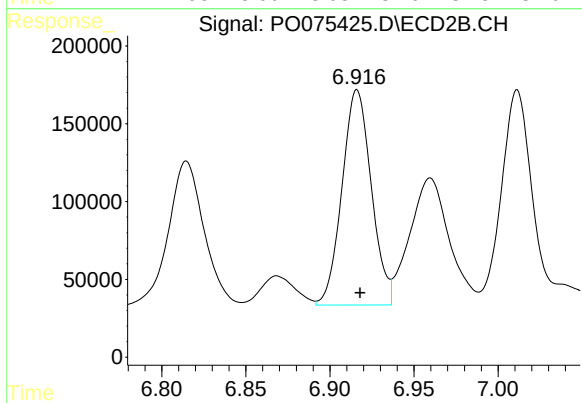

#29 AR-1254-4

R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 1678019
Conc: 575.71 ng/ml

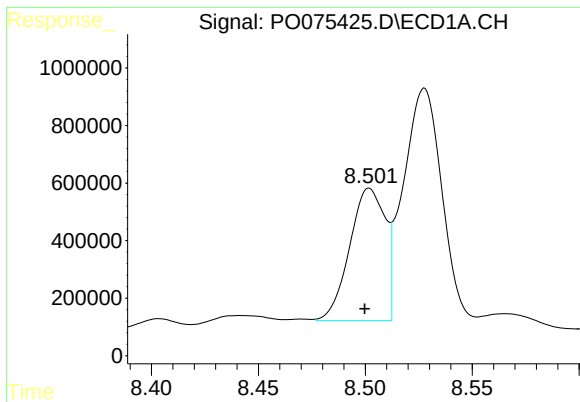


#30 AR-1254-5

R.T.: 8.501 min
Delta R.T.: 0.002 min
Response: 5512379
Conc: 986.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S1-01-F

Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:36 PM

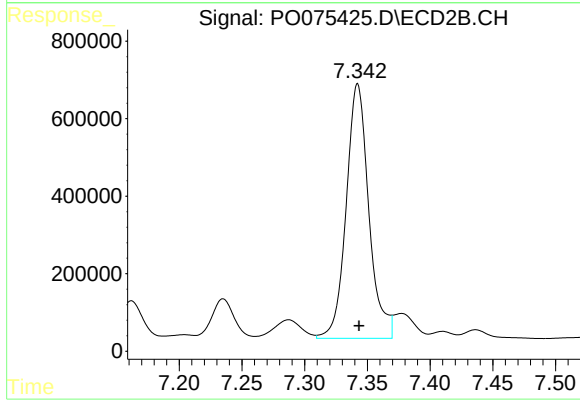

#30 AR-1254-5

R.T.: 7.342 min
Delta R.T.: -0.001 min
Response: 8242461
Conc: 2123.73 ng/ml