

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075430.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2021 12:34
 Operator : AJ/MA
 Sample : M1264-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-16

Manual Integrations
 APPROVED

Ankita

2/4/2021 1:49:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 13:09:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.994	2166334	1083527	21.406	22.540
2) SA Decachlor...	10.941	9.245	1515465	767975	15.707	15.821m
Target Compounds						
26) L6 AR-1254-1	7.160	6.103	1108501	723252	257.200	233.520
27) L6 AR-1254-2	7.390	6.262	2622677	1187853	388.997	442.347
28) L6 AR-1254-3	7.774	6.678	3655572	2237720	530.092	524.794
29) L6 AR-1254-4	8.071	6.916	3428930	1580695	567.186	542.319
30) L6 AR-1254-5	8.502	7.342	5886811	10031796	1053.119	2584.762 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075430.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2021 12:34
Operator : AJ/MA
Sample : M1264-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
DUP-16



Manual Integrations
APPROVED


Ankita

2/4/2021 1:49:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 13:09:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

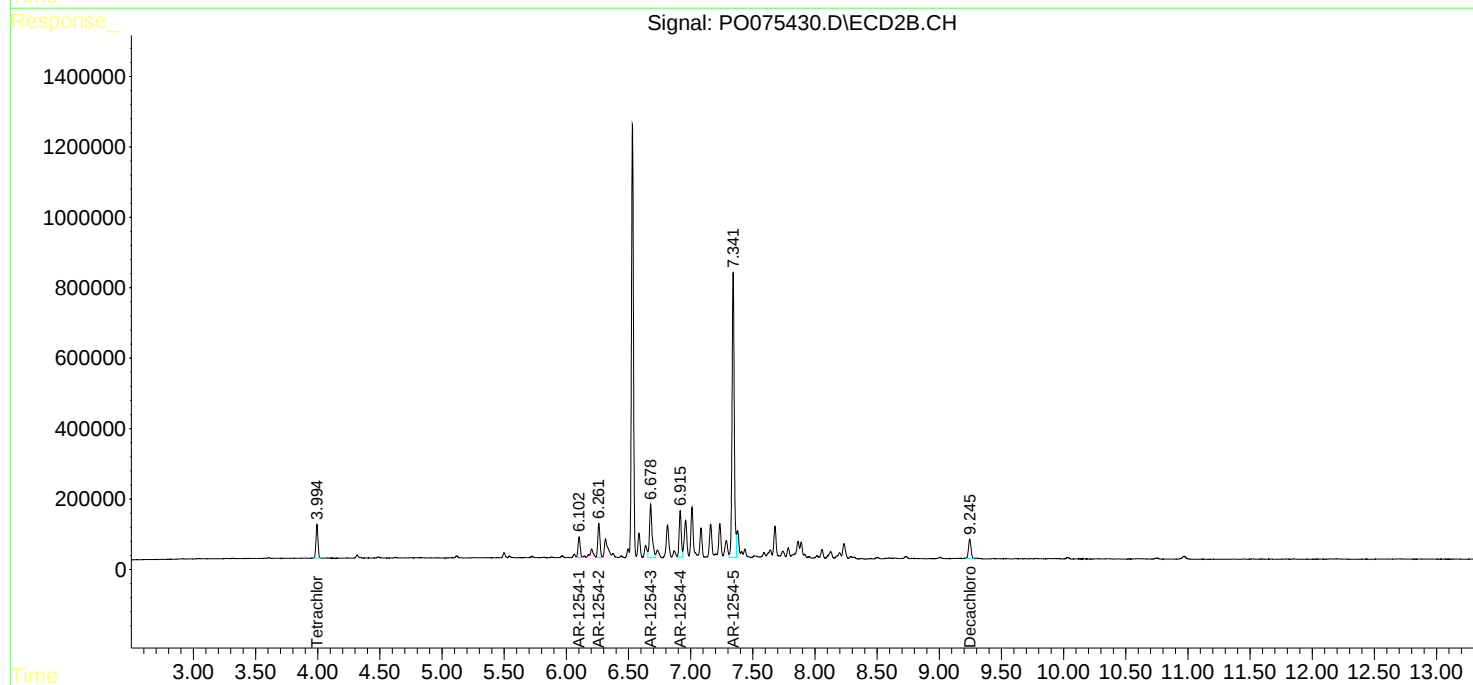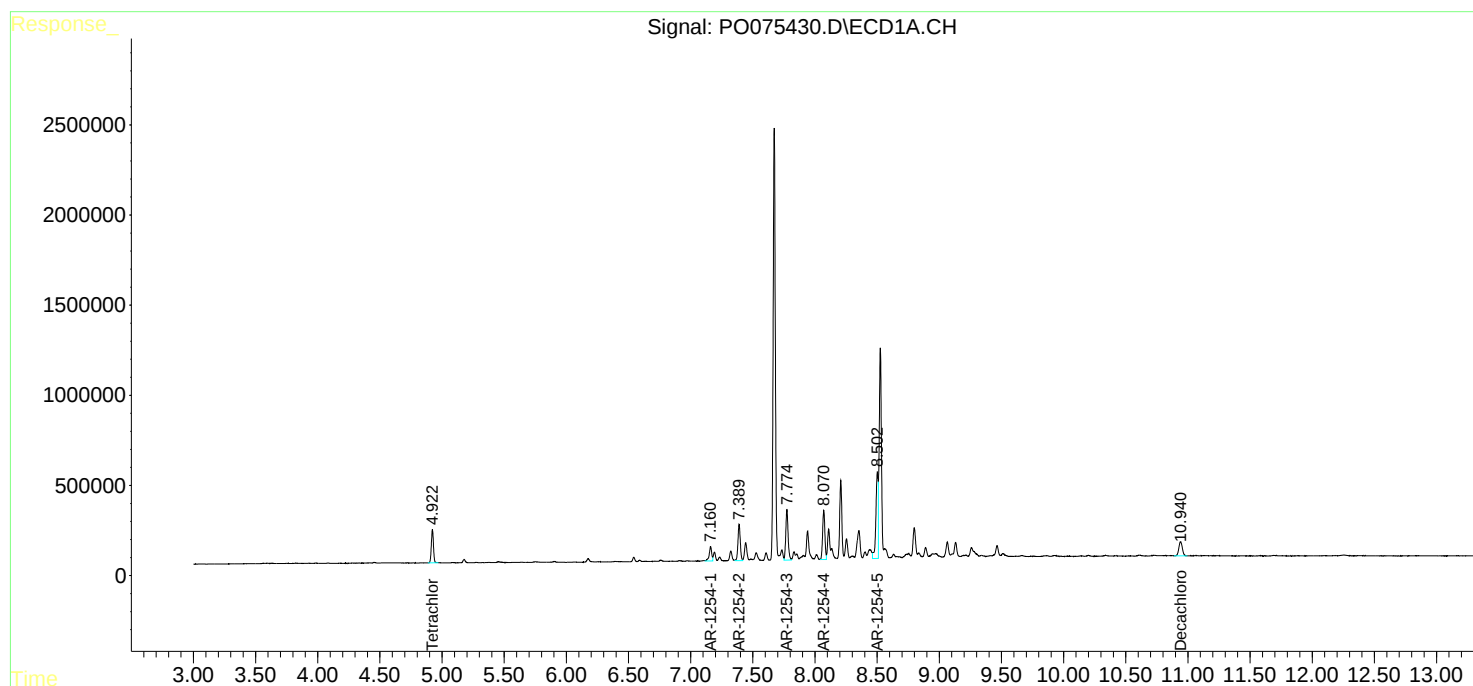

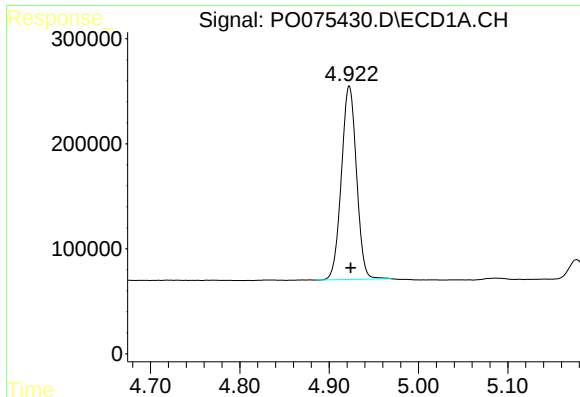

#1 Tetrachloro-m-xylene


R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 2166334
Conc: 21.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-16

Manual Integrations
APPROVED


Ankita

2/4/2021 1:49:41 PM

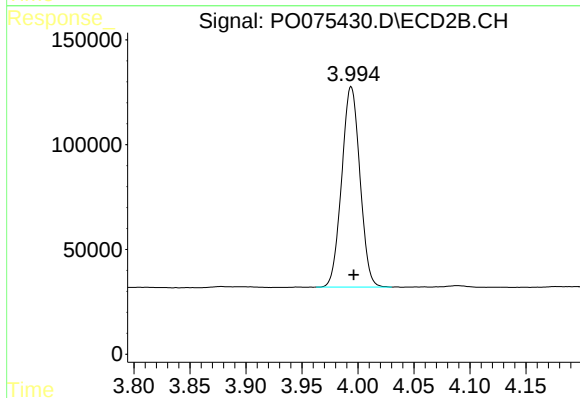


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1083527
Conc: 22.54 ng/ml

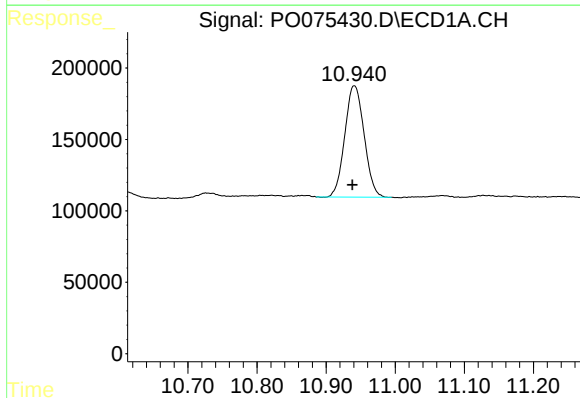


#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: 0.003 min
Response: 1515465
Conc: 15.71 ng/ml

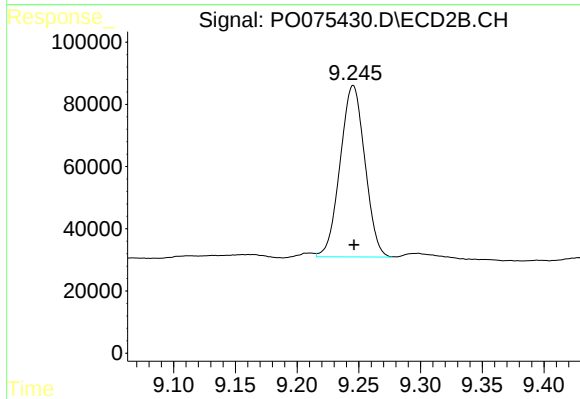

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.001 min
Response: 767975
Conc: 15.82 ng/ml m

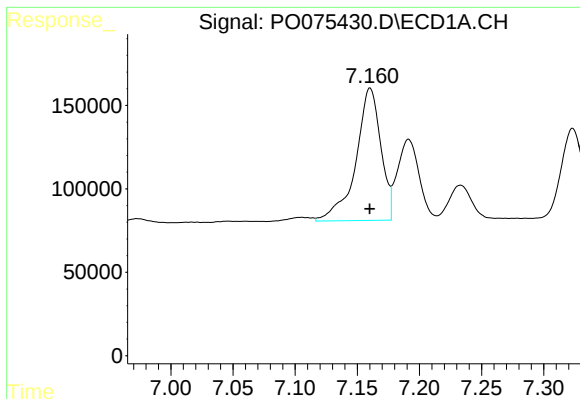

#26 AR-1254-1


R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 1108501
Conc: 257.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-16

Manual Integrations
APPROVED


Ankita

2/4/2021 1:49:41 PM

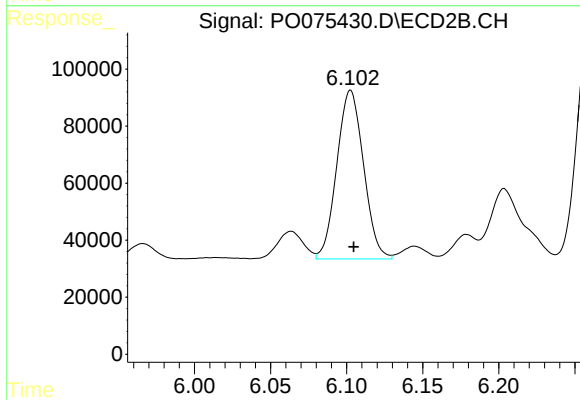


#26 AR-1254-1

R.T.: 6.103 min
Delta R.T.: -0.002 min
Response: 723252
Conc: 233.52 ng/ml

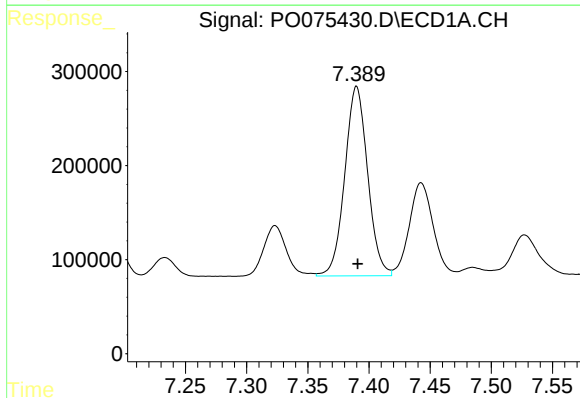


#27 AR-1254-2

R.T.: 7.390 min
Delta R.T.: 0.000 min
Response: 2622677
Conc: 389.00 ng/ml

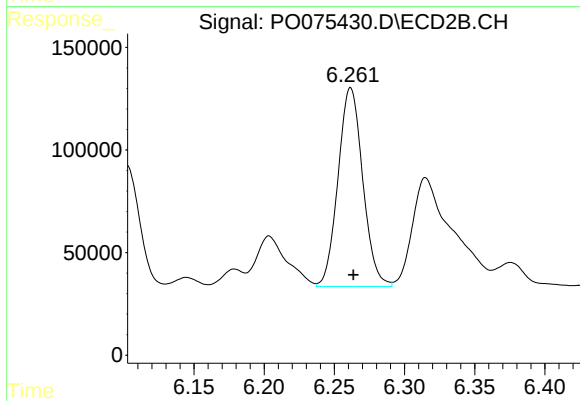

#27 AR-1254-2

R.T.: 6.262 min
Delta R.T.: -0.002 min
Response: 1187853
Conc: 442.35 ng/ml

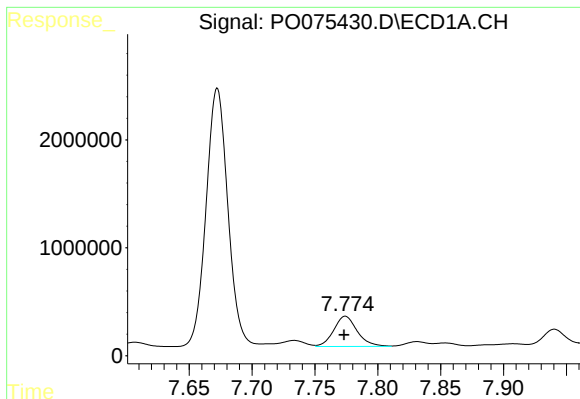

#28 AR-1254-3


R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 3655572
Conc: 530.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-16

Manual Integrations
APPROVED


Ankita

2/4/2021 1:49:41 PM

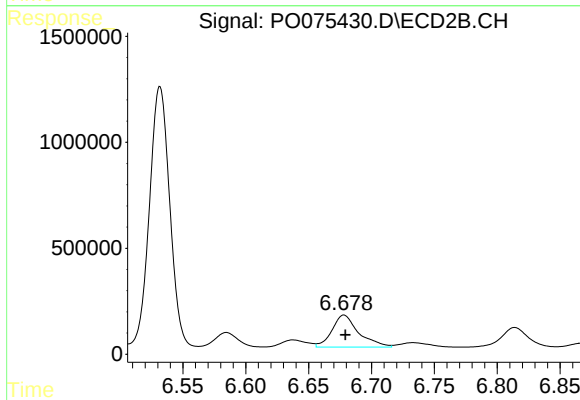


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: -0.001 min
Response: 2237720
Conc: 524.79 ng/ml

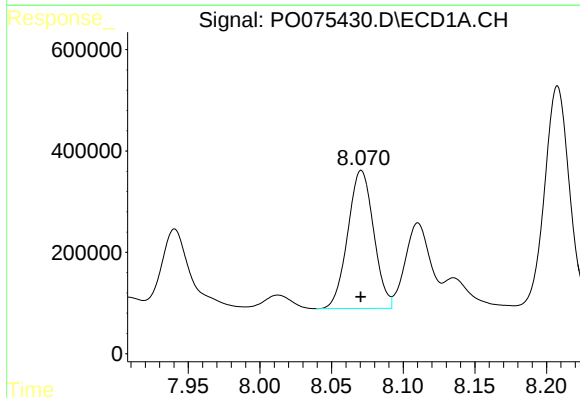


#29 AR-1254-4

R.T.: 8.071 min
Delta R.T.: 0.000 min
Response: 3428930
Conc: 567.19 ng/ml

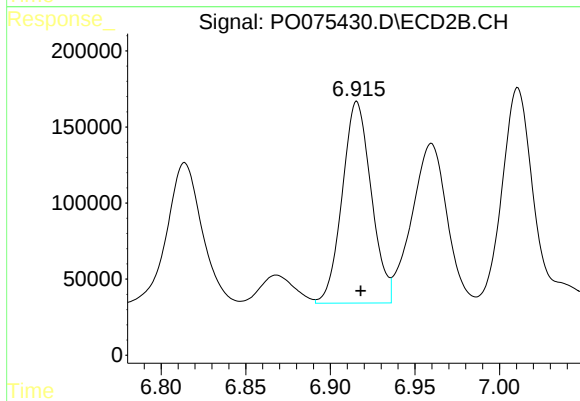

#29 AR-1254-4

R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 1580695
Conc: 542.32 ng/ml

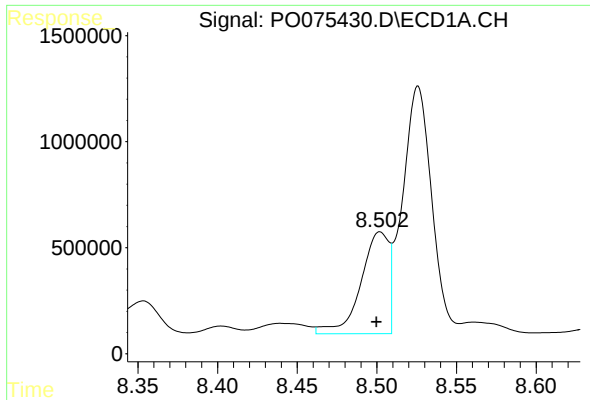


#30 AR-1254-5

R.T.: 8.502 min
Delta R.T.: 0.002 min
Response: 5886811
Conc: 1053.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-16

Manual Integrations
APPROVED

Ankita

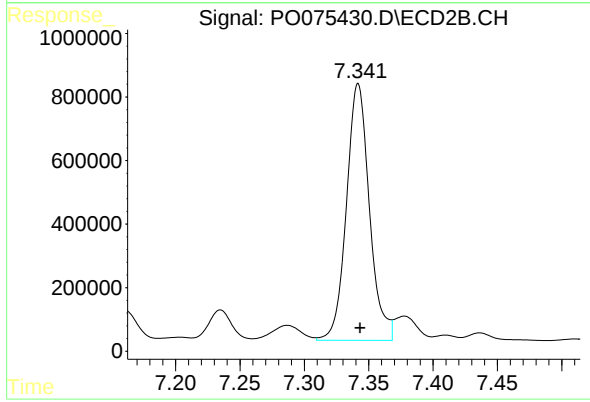

#30 AR-1254-5

R.T.: 7.342 min
Delta R.T.: -0.001 min
Response: 10031796
Conc: 2584.76 ng/ml

2/4/2021 1:49:41 PM