

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075432.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2021 13:08
 Operator : AJ/MA
 Sample : M1265-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-02-F

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:49:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 13:29:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.994	2237736	1106026	22.112m	23.008
2) SA Decachlor...	10.942	9.243	1503799	1088540	15.586	22.425m#
Target Compounds						
26) L6 AR-1254-1	7.161	6.103	900234	674659	208.877	217.830
27) L6 AR-1254-2	7.390	6.262	2369843	1018985	351.496	379.462
28) L6 AR-1254-3	7.775	6.679	3383862	2076862	490.691	487.069
29) L6 AR-1254-4	8.072	6.917	3664082	1703731	606.082	584.532
30) L6 AR-1254-5	8.502	7.342	6699013	9034966	1198.418	2327.922 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075432.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2021 13:08
Operator : AJ/MA
Sample : M1265-05
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S3-02-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 13:29:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

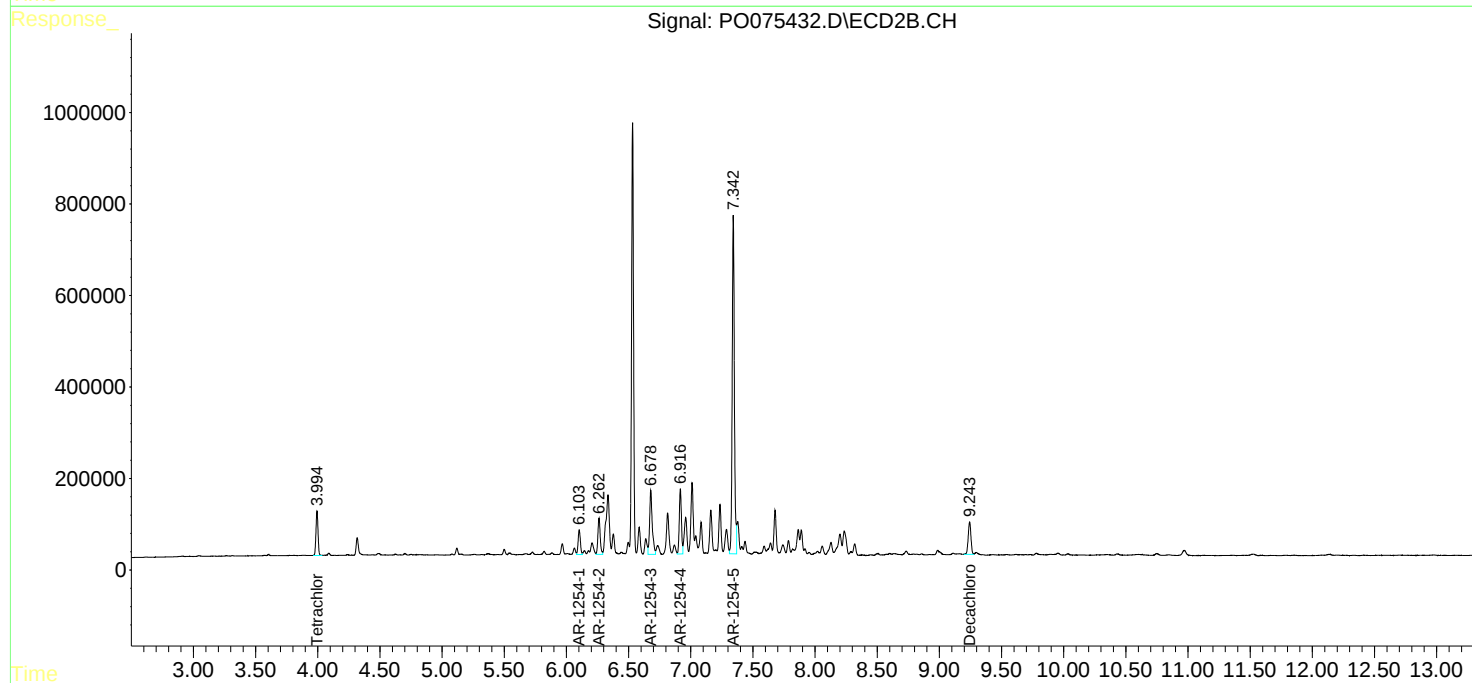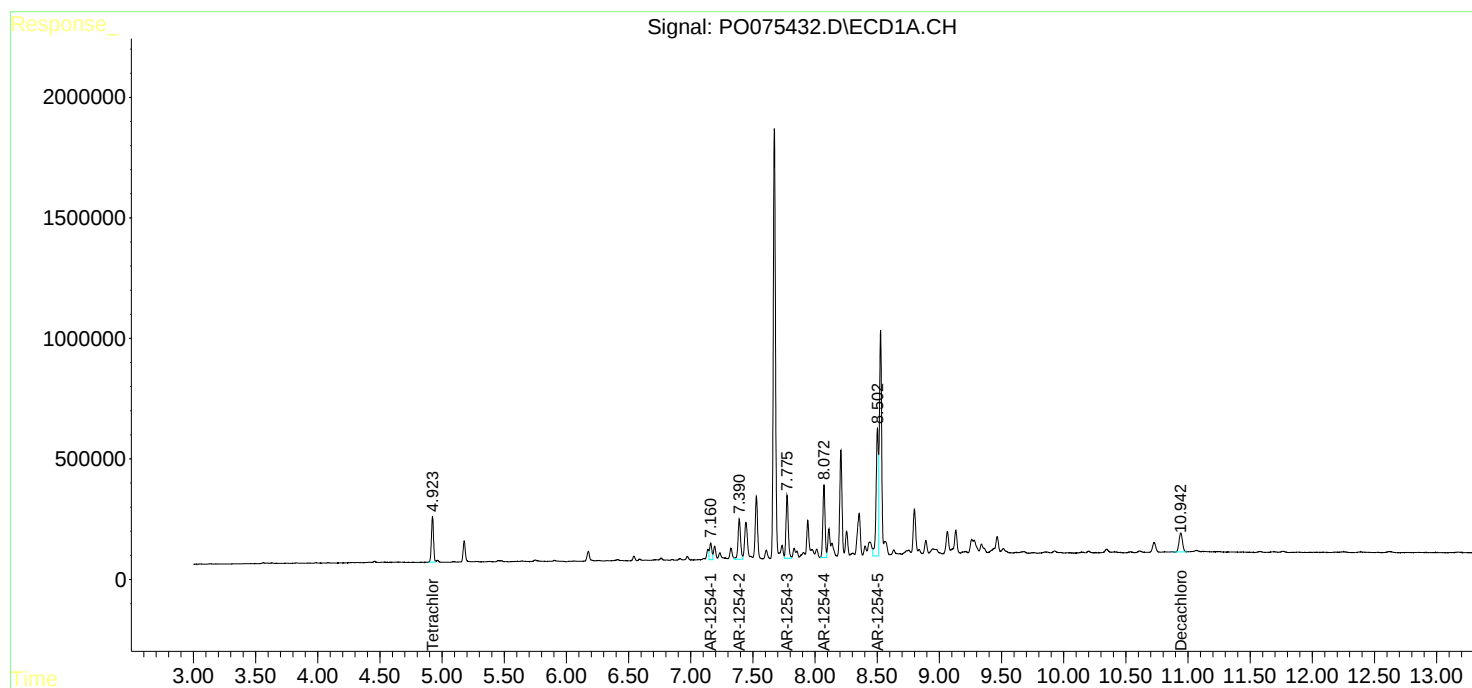

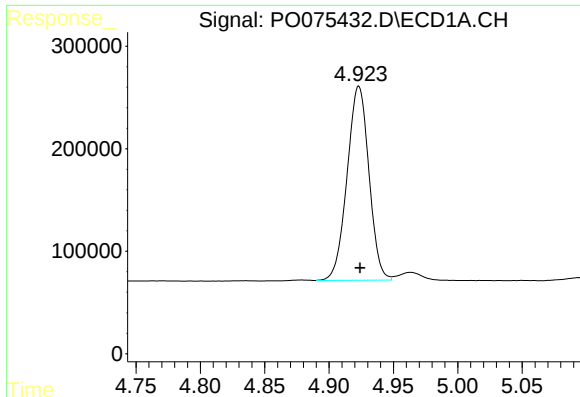


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 2237736
Conc: 22.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-02-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:45 PM

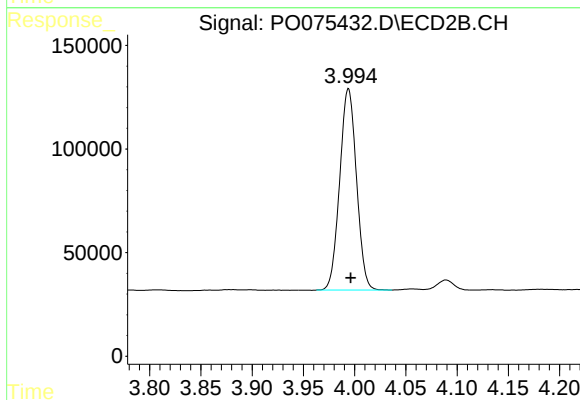


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1106026
Conc: 23.01 ng/ml

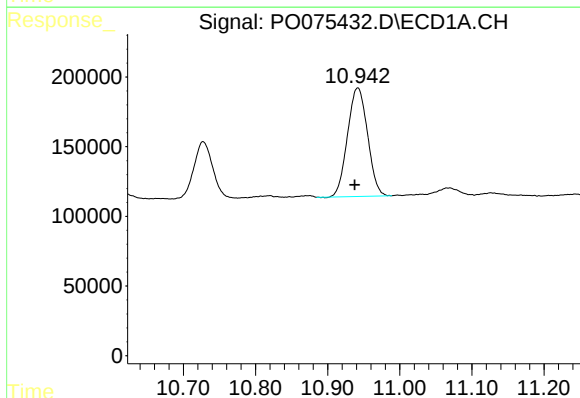


#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: 0.004 min
Response: 1503799
Conc: 15.59 ng/ml

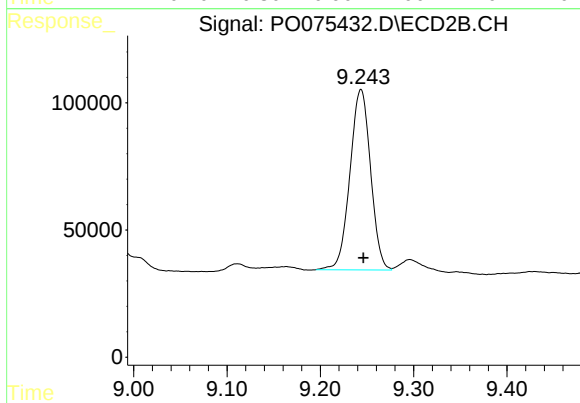

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 1088540
Conc: 22.42 ng/ml m

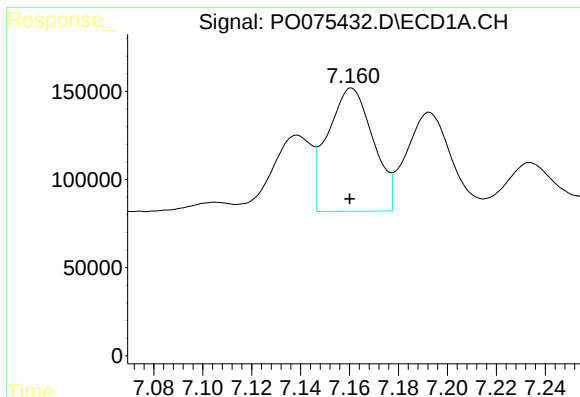


#26 AR-1254-1

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 900234
Conc: 208.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-02-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:45 PM

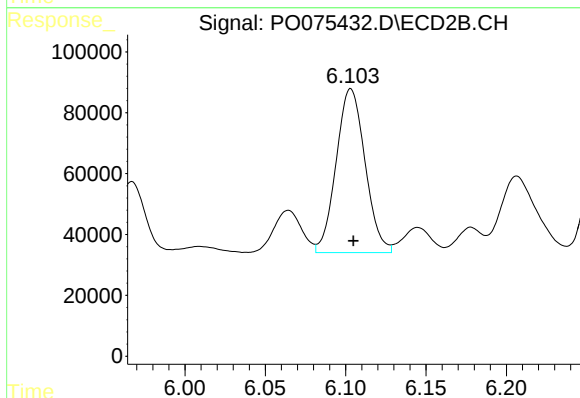


#26 AR-1254-1

R.T.: 6.103 min
Delta R.T.: -0.002 min
Response: 674659
Conc: 217.83 ng/ml

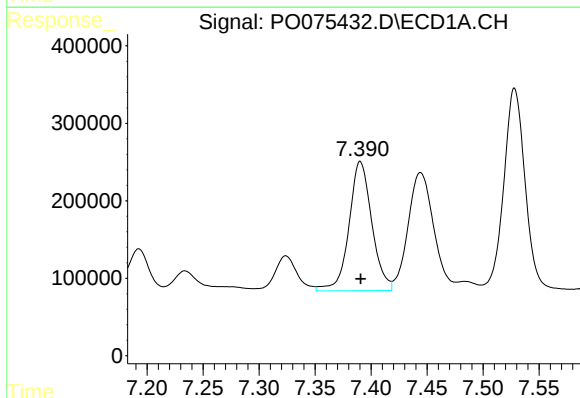


#27 AR-1254-2

R.T.: 7.390 min
Delta R.T.: 0.000 min
Response: 2369843
Conc: 351.50 ng/ml

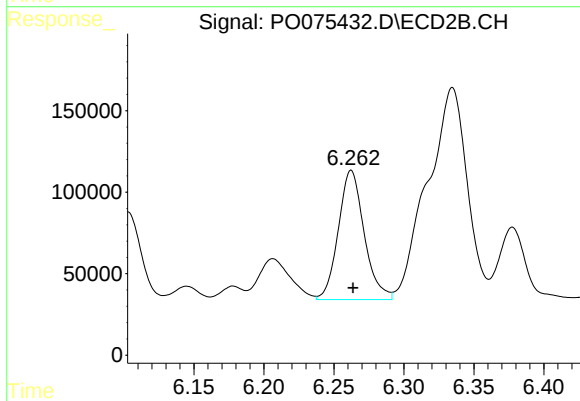

#27 AR-1254-2

R.T.: 6.262 min
Delta R.T.: -0.001 min
Response: 1018985
Conc: 379.46 ng/ml

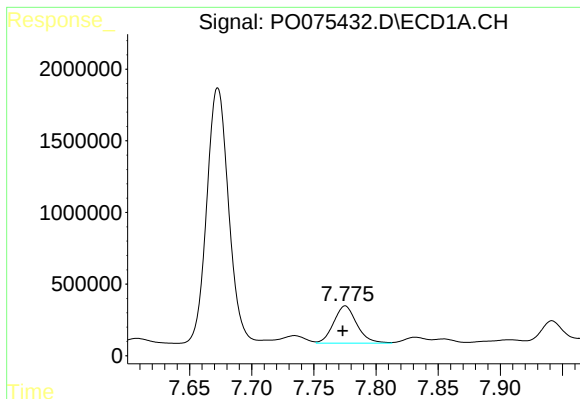


#28 AR-1254-3

R.T.: 7.775 min
Delta R.T.: 0.002 min
Response: 3383862
Conc: 490.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-02-F


Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:45 PM

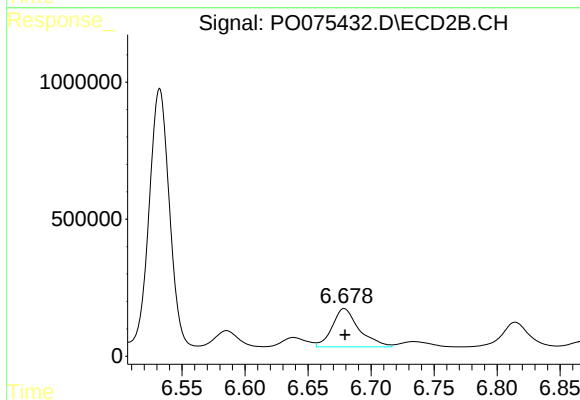


#28 AR-1254-3

R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 2076862
Conc: 487.07 ng/ml

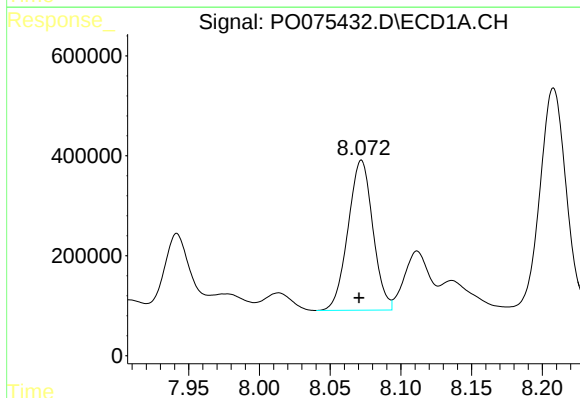


#29 AR-1254-4

R.T.: 8.072 min
Delta R.T.: 0.002 min
Response: 3664082
Conc: 606.08 ng/ml

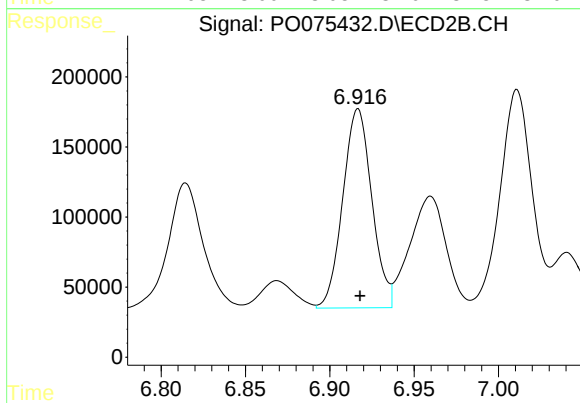

#29 AR-1254-4

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 1703731
Conc: 584.53 ng/ml

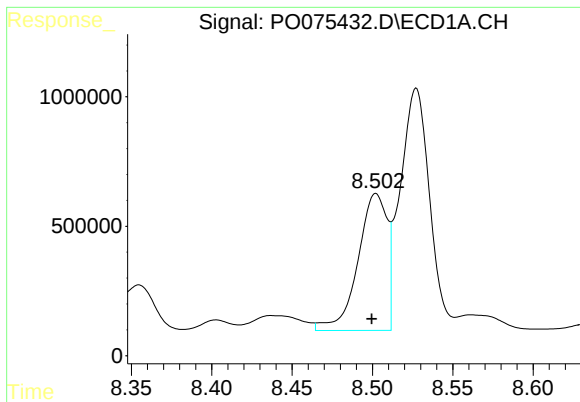


#30 AR-1254-5

R.T.: 8.502 min
Delta R.T.: 0.002 min
Response: 6699013
Conc: 1198.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-02-F

Manual Integrations
APPROVED

Ankita
2/4/2021 1:49:45 PM

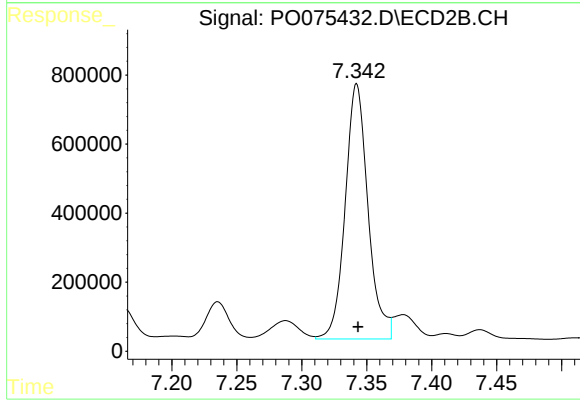

#30 AR-1254-5

R.T.: 7.342 min
Delta R.T.: -0.001 min
Response: 9034966
Conc: 2327.92 ng/ml