

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075440.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2021 15:25
 Operator : AJ/MA
 Sample : M1257-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 72-11938-2-POLES

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:50:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 16:54:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.995	2263402	1102862	22.365	22.942
2) SA Decachlor...	10.943	9.246	2403597	1181854	24.912	24.347
Target Compounds						
26) L6 AR-1254-1	7.161	6.103	56158	51816	13.030m	16.730 #
27) L6 AR-1254-2	7.390	6.261	128400	63342	19.044m	23.588
28) L6 AR-1254-3	7.776	6.678	242710	150290	35.195	35.246
29) L6 AR-1254-4	8.073	6.917	351969	94429	58.220	32.398 #
30) L6 AR-1254-5	8.502	7.342	368377	198160	65.901m	51.057

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075440.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2021 15:25
Operator : AJ/MA
Sample : M1257-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
72-11938-2-POLES


Manual Integrations
APPROVED

Ankita
2/4/2021 1:50:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 16:54:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

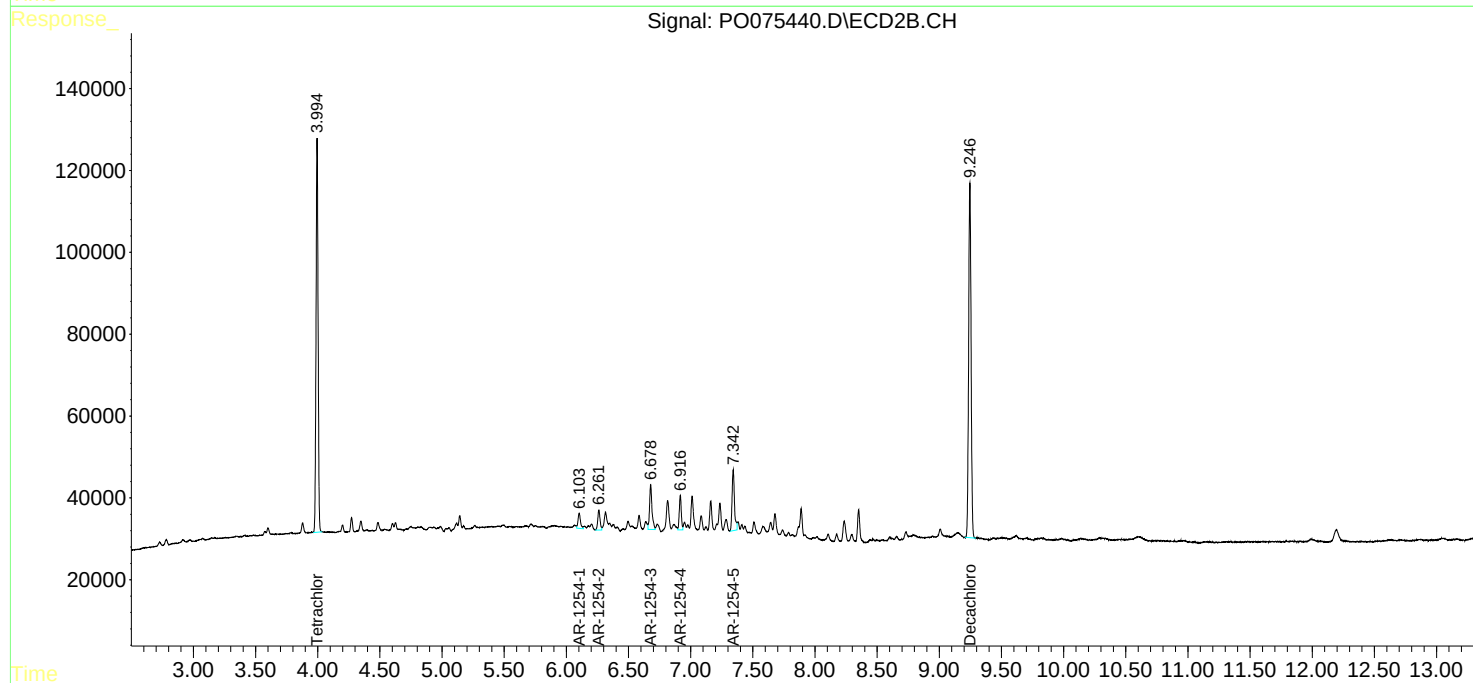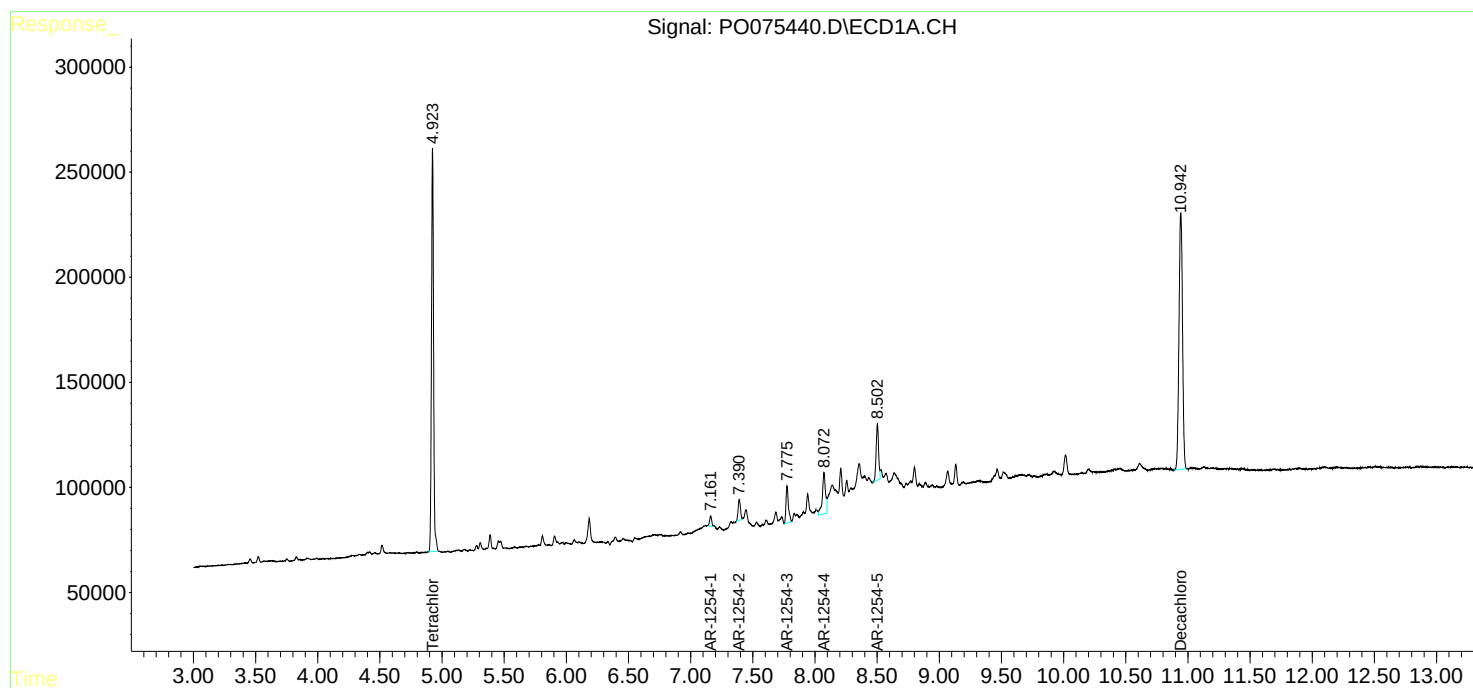

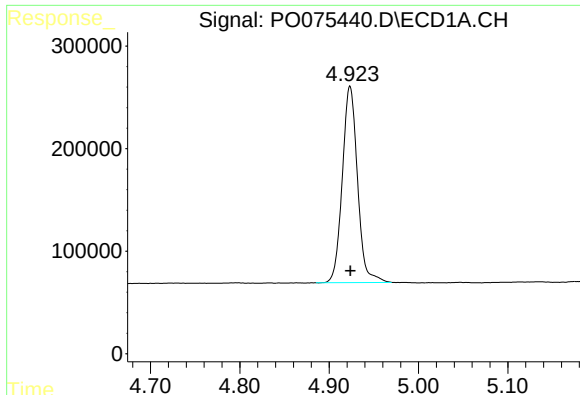


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 2263402
Conc: 22.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
72-11938-2-POLES


Manual Integrations
APPROVED

Ankita
2/4/2021 1:50:09 PM

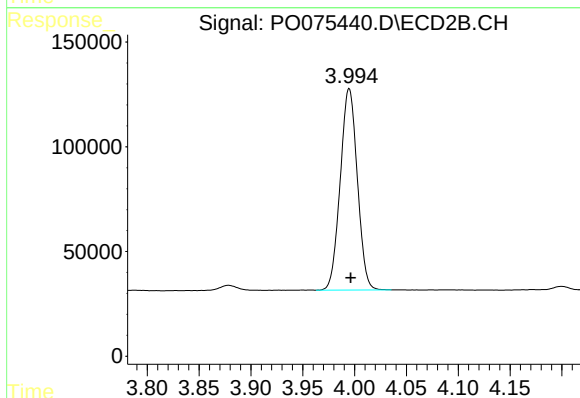


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.001 min
Response: 1102862
Conc: 22.94 ng/ml

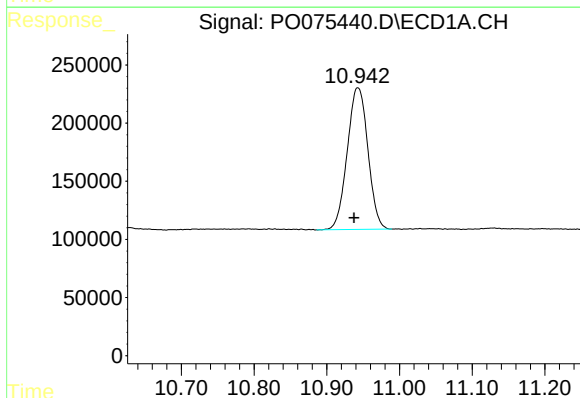


#2 Decachlorobiphenyl

R.T.: 10.943 min
Delta R.T.: 0.005 min
Response: 2403597
Conc: 24.91 ng/ml

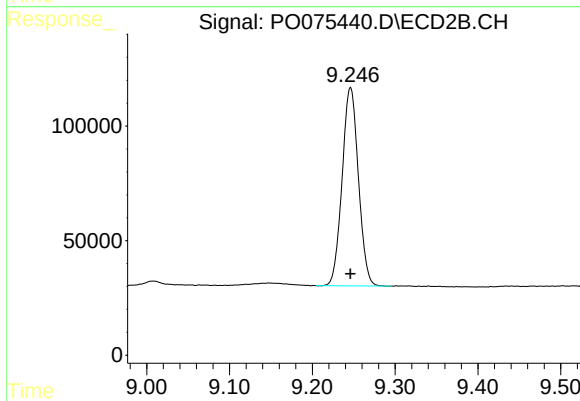

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: 0.000 min
Response: 1181854
Conc: 24.35 ng/ml

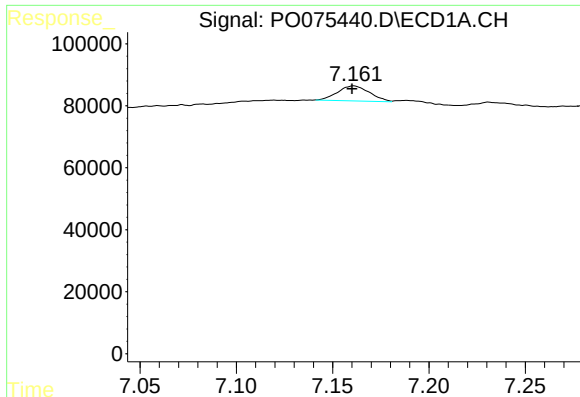


#26 AR-1254-1

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 56158
Conc: 13.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
72-11938-2-POLES


Manual Integrations
APPROVED

Ankita
2/4/2021 1:50:09 PM

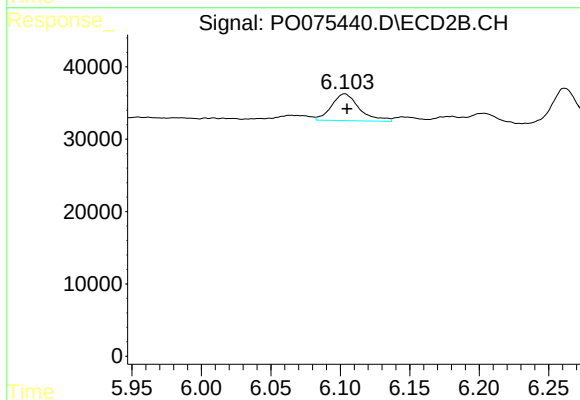


#26 AR-1254-1

R.T.: 6.103 min
Delta R.T.: -0.001 min
Response: 51816
Conc: 16.73 ng/ml

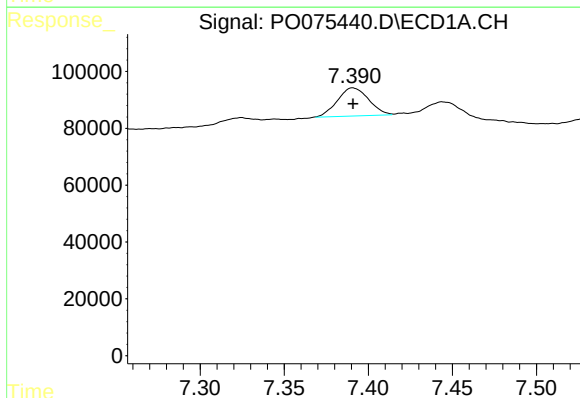


#27 AR-1254-2

R.T.: 7.390 min
Delta R.T.: 0.000 min
Response: 128400
Conc: 19.04 ng/ml m

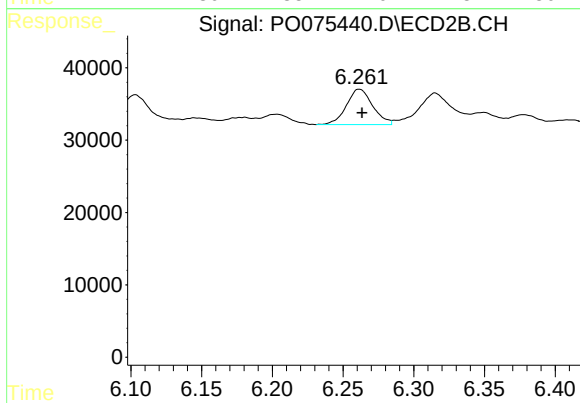

#27 AR-1254-2

R.T.: 6.261 min
Delta R.T.: -0.002 min
Response: 63342
Conc: 23.59 ng/ml

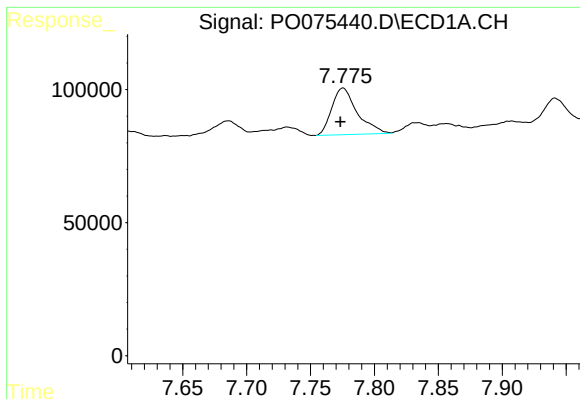


#28 AR-1254-3

R.T.: 7.776 min
Delta R.T.: 0.002 min
Response: 242710
Conc: 35.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
72-11938-2-POLES


Manual Integrations
APPROVED

Ankita
2/4/2021 1:50:09 PM

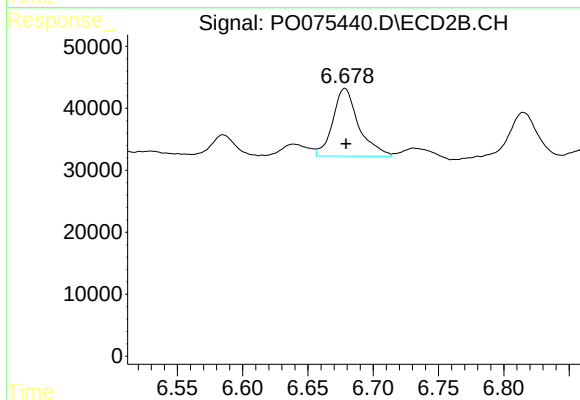


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 150290
Conc: 35.25 ng/ml

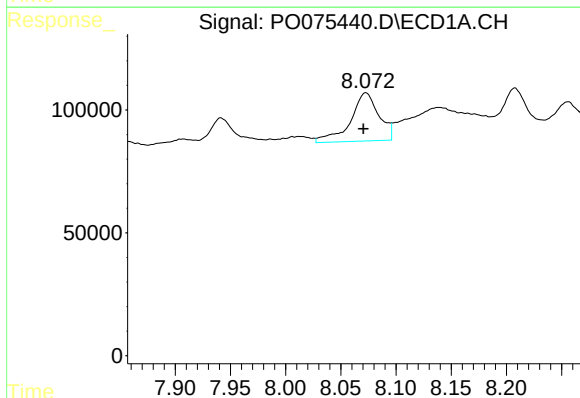


#29 AR-1254-4

R.T.: 8.073 min
Delta R.T.: 0.002 min
Response: 351969
Conc: 58.22 ng/ml

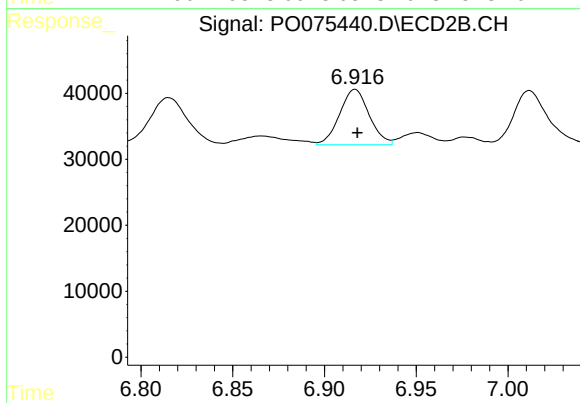

#29 AR-1254-4

R.T.: 6.917 min
Delta R.T.: -0.001 min
Response: 94429
Conc: 32.40 ng/ml

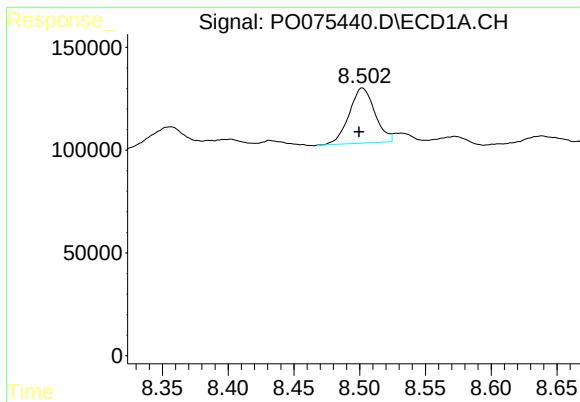


#30 AR-1254-5

R.T.: 8.502 min
Delta R.T.: 0.002 min
Response: 368377
Conc: 65.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
72-11938-2-POLES

Manual Integrations
APPROVED

Ankita
2/4/2021 1:50:09 PM

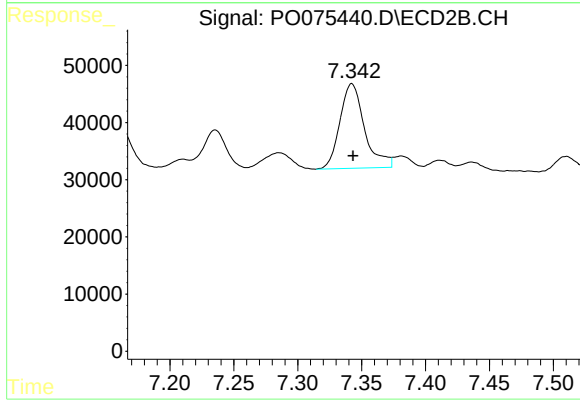

#30 AR-1254-5

R.T.: 7.342 min
Delta R.T.: 0.000 min
Response: 198160
Conc: 51.06 ng/ml