

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075467.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2021 23:42
 Operator : AJ/MA
 Sample : M1293-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT-4

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:51:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:50:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.997	1720034	700113	16.996m	14.564
2) SA Decachlor...	10.952	9.245	1060319	567767	10.990m	11.697m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
Data File : P0075467.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2021 23:42
Operator : AJ/MA
Sample : M1293-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/4/2021 1:51:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:50:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

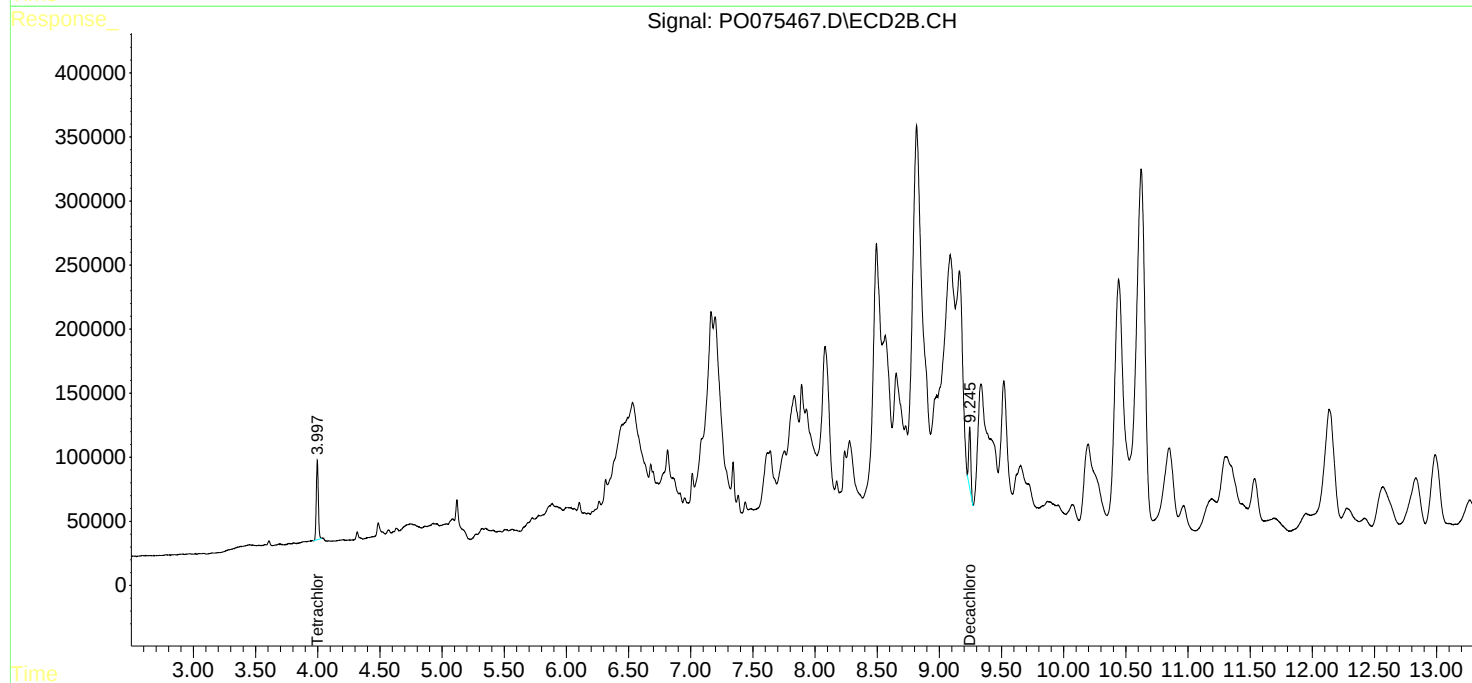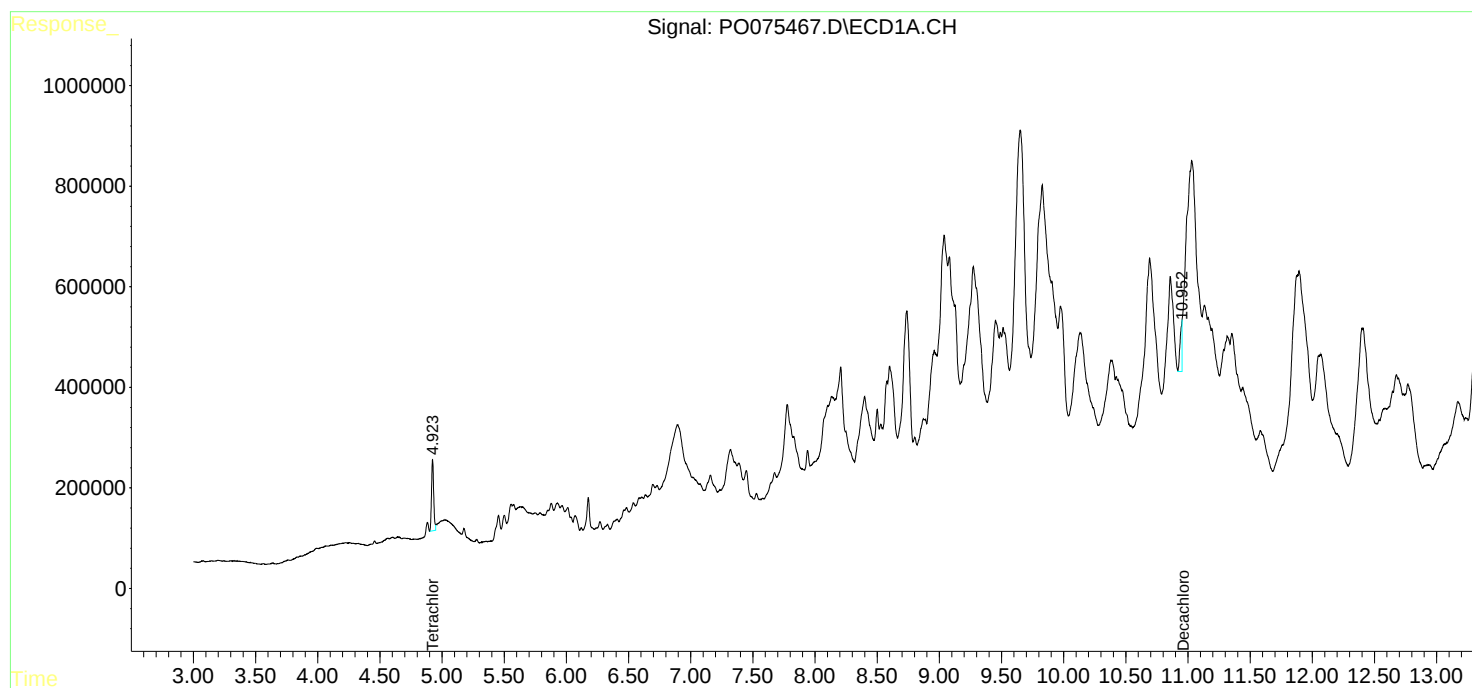

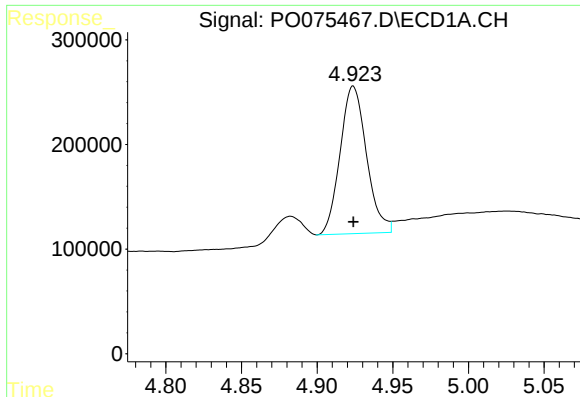


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 1720034
Conc: 17.00 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/4/2021 1:51:31 PM

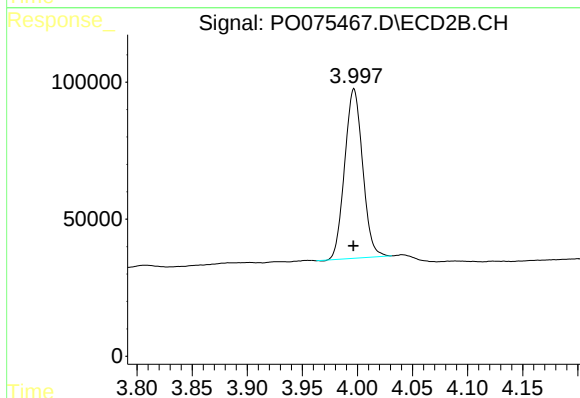


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: 0.000 min
Response: 700113
Conc: 14.56 ng/ml

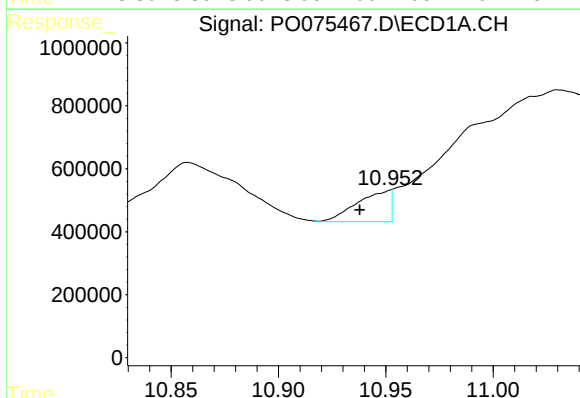

#2 Decachlorobiphenyl

R.T.: 10.952 min
Delta R.T.: 0.014 min
Response: 1060319
Conc: 10.99 ng/ml m

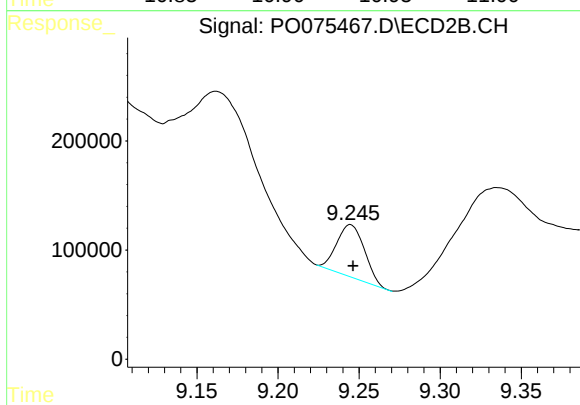

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.001 min
Response: 567767
Conc: 11.70 ng/ml m