

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075482.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 4:50
 Operator : AJ/MA
 Sample : M1292-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-003-0205

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:52:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 06:46:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.995	2328510	1153795	23.009	24.002
2) SA Decachlor...	10.941	9.245	2267979	1086711	23.507	22.387
Target Compounds						
36) L8 AR-1262-1	8.573	7.342	298622	24456	34.220m	11.212 #
37) L8 AR-1262-2	9.131	7.889	274540	154957	18.155	20.206
38) L8 AR-1262-3	9.440	8.173	408849	198060	39.136	59.849 #
39) L8 AR-1262-4	9.537	8.238	398010	217724	53.850	37.919 #
40) L8 AR-1262-5	10.200	8.731	323074	122200	62.298	44.423 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075482.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 4:50
Operator : AJ/MA
Sample : M1292-06
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
OU421-003-0205


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 06:46:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

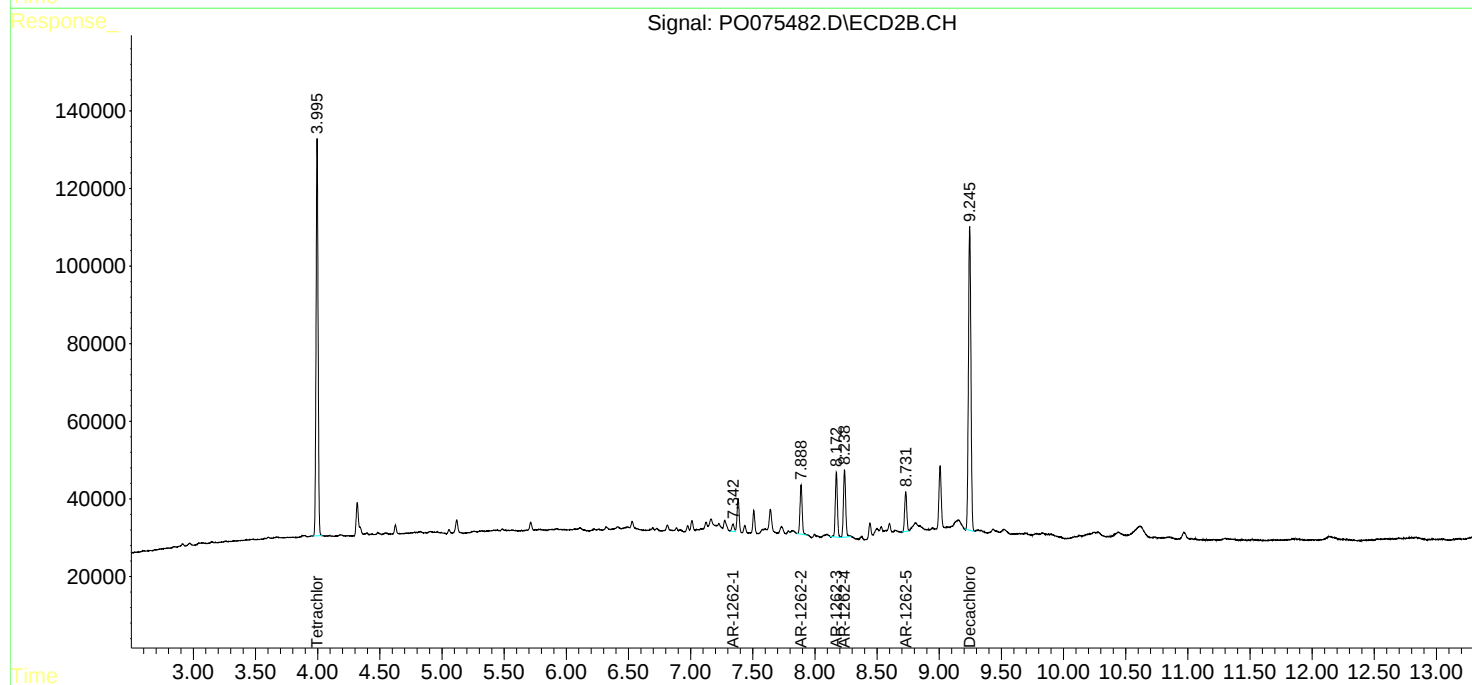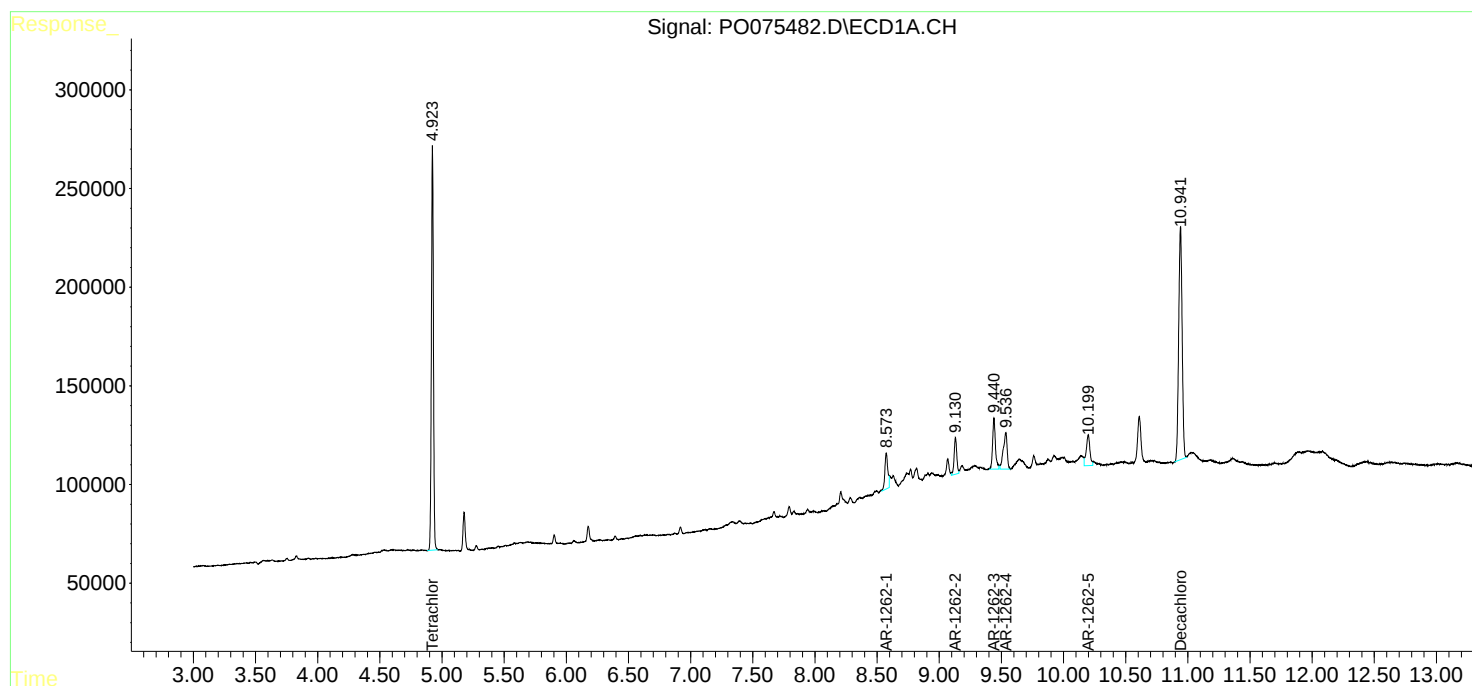

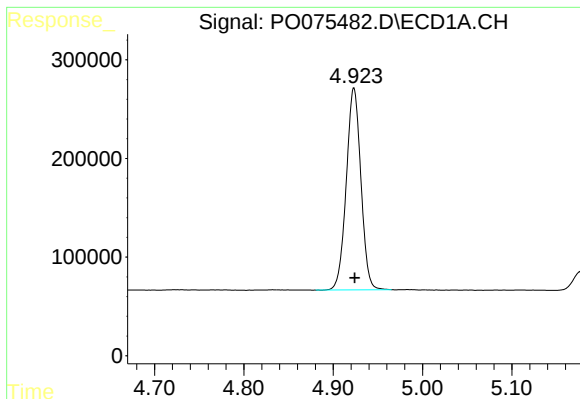


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 2328510
Conc: 23.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-0205


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:13 PM

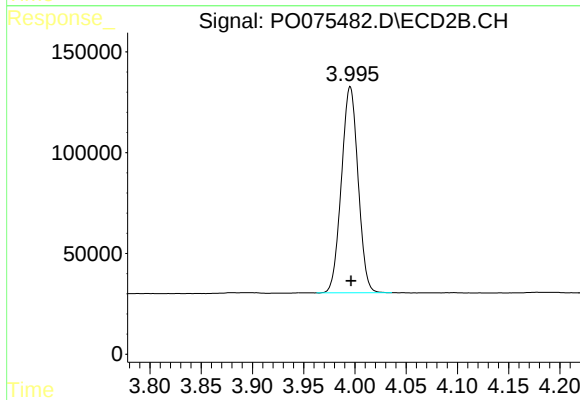


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 1153795
Conc: 24.00 ng/ml

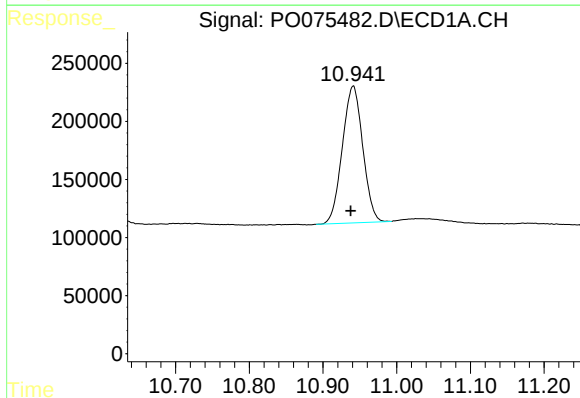


#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: 0.003 min
Response: 2267979
Conc: 23.51 ng/ml

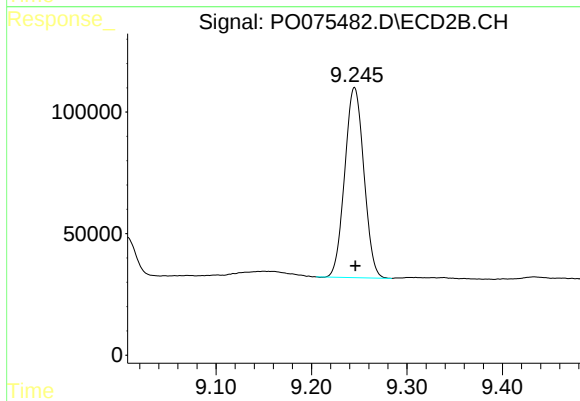

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.001 min
Response: 1086711
Conc: 22.39 ng/ml

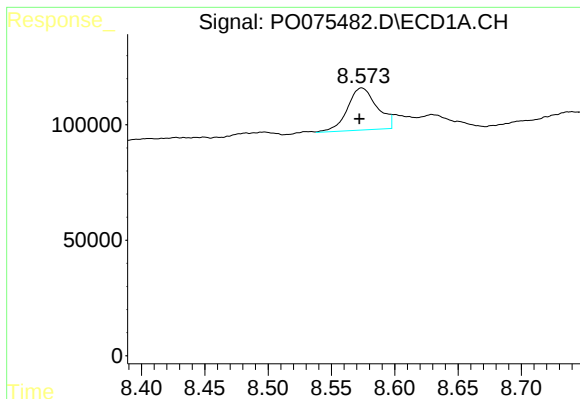


#36 AR-1262-1

R.T.: 8.573 min
Delta R.T.: 0.001 min
Response: 298622
Conc: 34.22 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-003-0205


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:13 PM

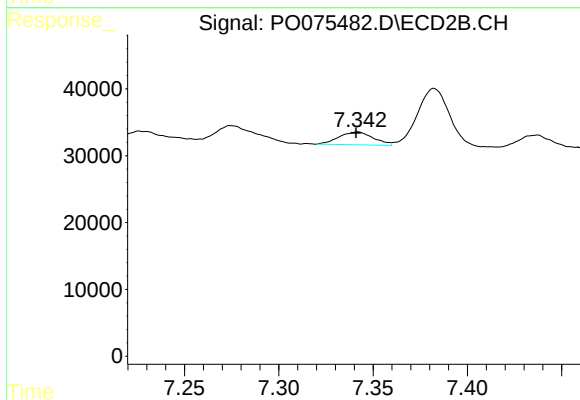


#36 AR-1262-1

R.T.: 7.342 min
Delta R.T.: 0.001 min
Response: 24456
Conc: 11.21 ng/ml

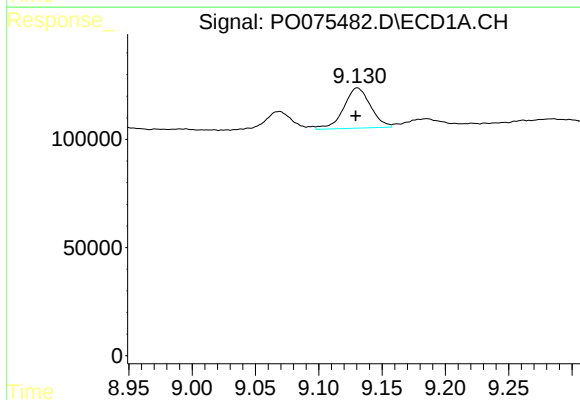


#37 AR-1262-2

R.T.: 9.131 min
Delta R.T.: 0.001 min
Response: 274540
Conc: 18.16 ng/ml

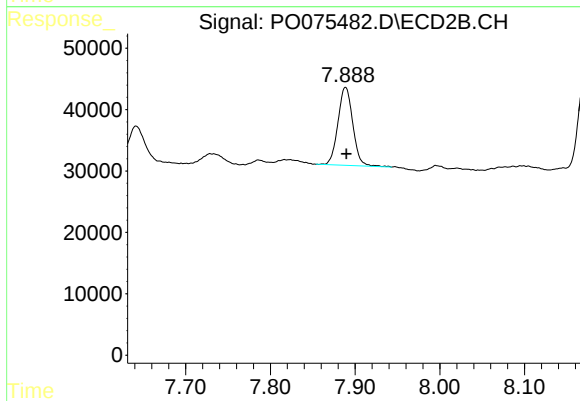

#37 AR-1262-2

R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 154957
Conc: 20.21 ng/ml

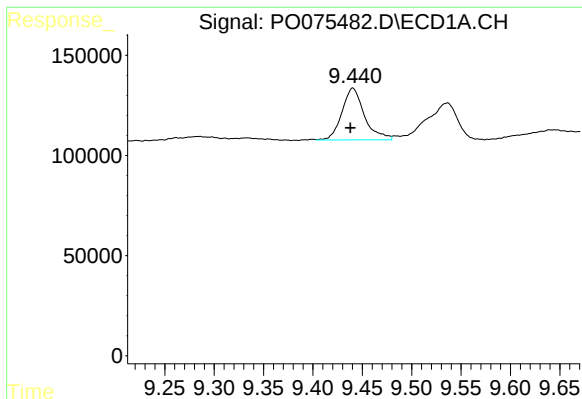


#38 AR-1262-3

R.T.: 9.440 min
Delta R.T.: 0.002 min
Response: 408849
Conc: 39.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-0205


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:13 PM

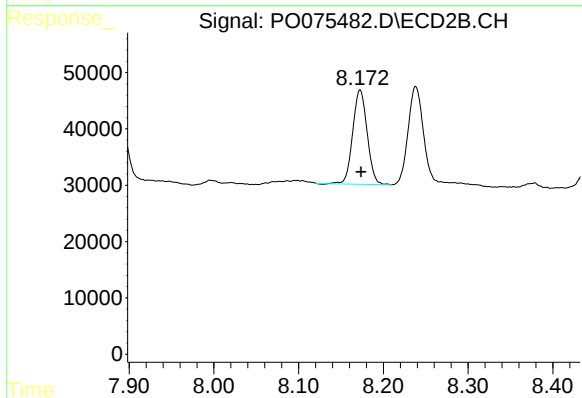


#38 AR-1262-3

R.T.: 8.173 min
Delta R.T.: -0.001 min
Response: 198060
Conc: 59.85 ng/ml

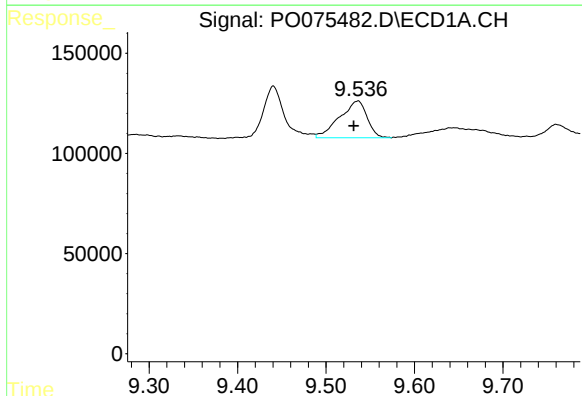


#39 AR-1262-4

R.T.: 9.537 min
Delta R.T.: 0.005 min
Response: 398010
Conc: 53.85 ng/ml

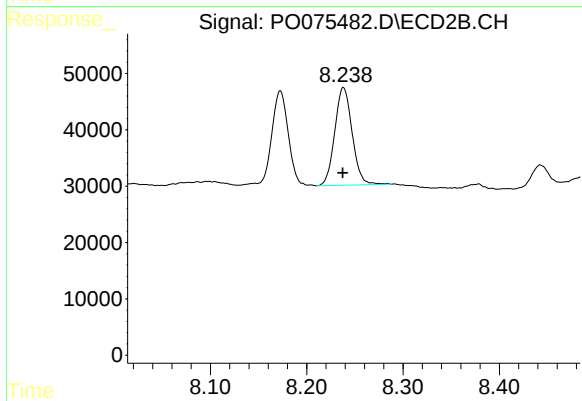

#39 AR-1262-4

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 217724
Conc: 37.92 ng/ml

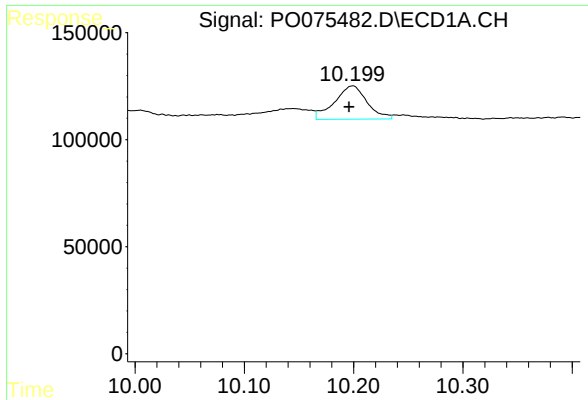


#40 AR-1262-5

R.T.: 10.200 min
Delta R.T.: 0.004 min
Response: 323074
Conc: 62.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-0205

Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:13 PM

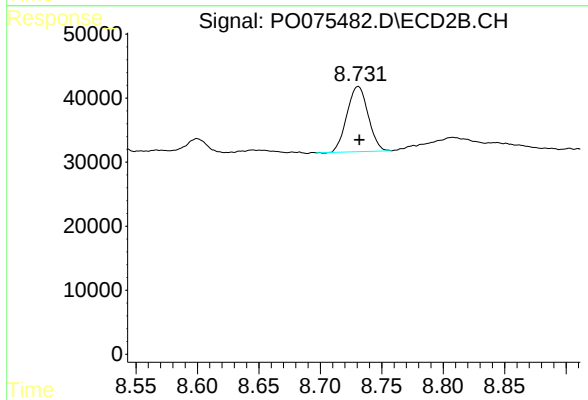

#40 AR-1262-5

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 122200
Conc: 44.42 ng/ml