

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0020321\
 Data File : P0075483.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 5:07
 Operator : AJ/MA
 Sample : M1292-07
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-003-0510

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:52:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 06:47:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.924	3.995	2473932	1200561	24.445	24.974
2)	SA Decachlor...	10.940	9.245	2368544	1137966	24.549	23.443
Target Compounds							
36)	L8 AR-1262-1	8.574	7.341	363284	275153	41.630m	126.147 #
37)	L8 AR-1262-2	9.131	7.888	452415	237120	29.918	30.919
38)	L8 AR-1262-3	9.440	8.172	645565	352111	61.795	106.400 #
39)	L8 AR-1262-4	9.535	8.239	622860	348633	84.271	60.718 #
40)	L8 AR-1262-5	10.198	8.731	370669	181346	71.476	65.924

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075483.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 5:07
Operator : AJ/MA
Sample : M1292-07
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
OU421-003-0510


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 06:47:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

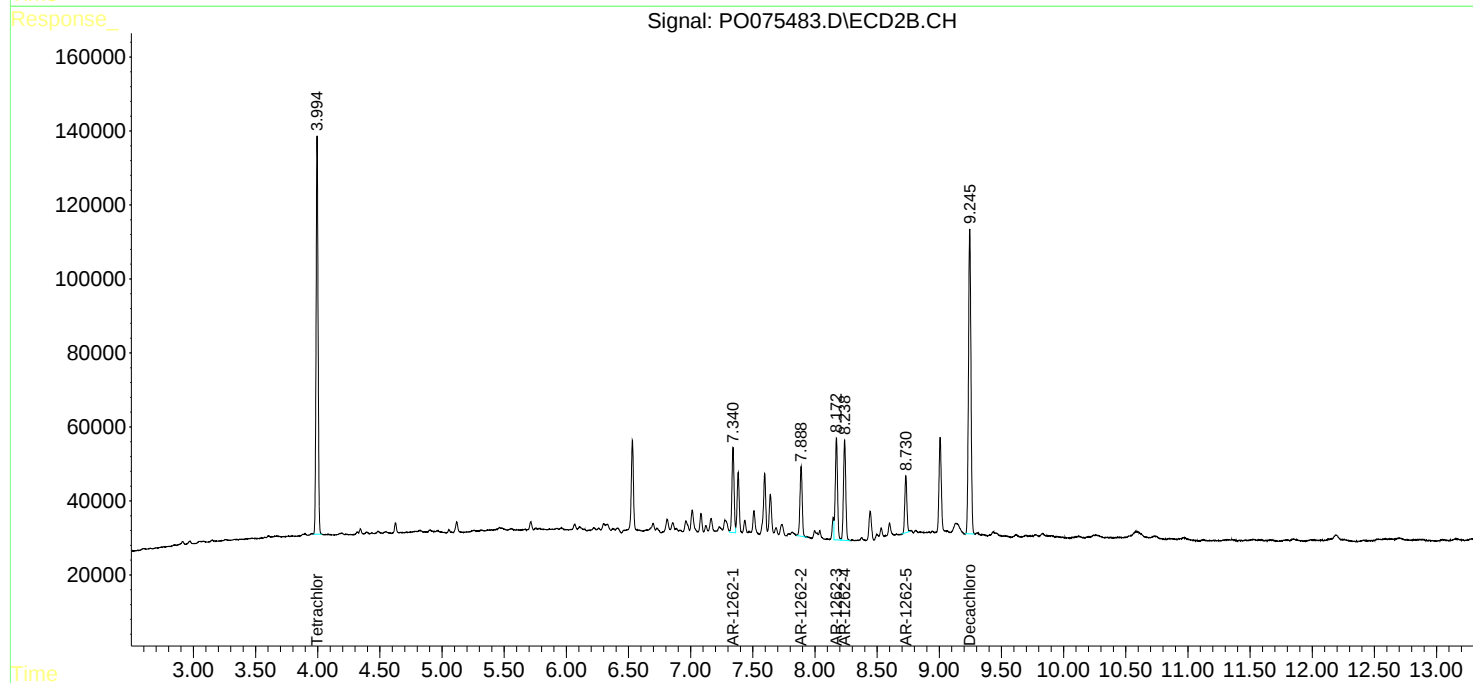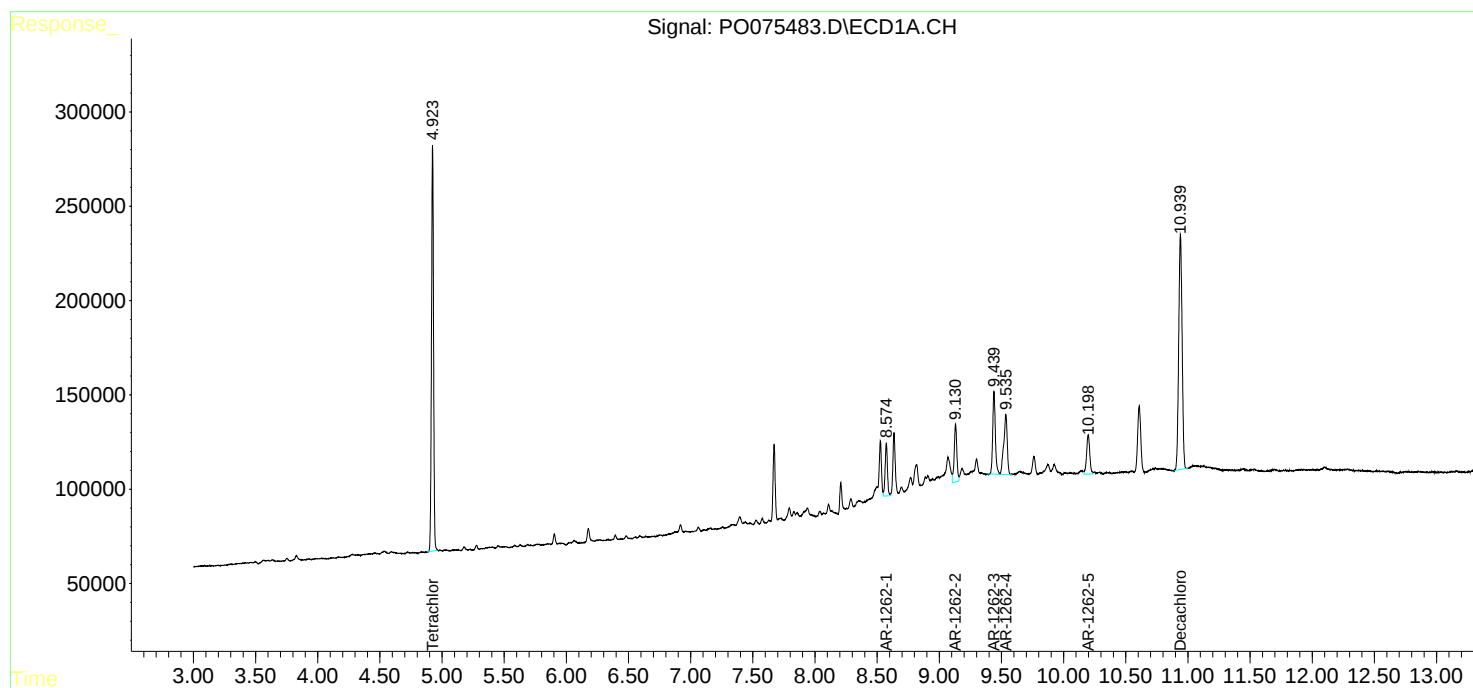

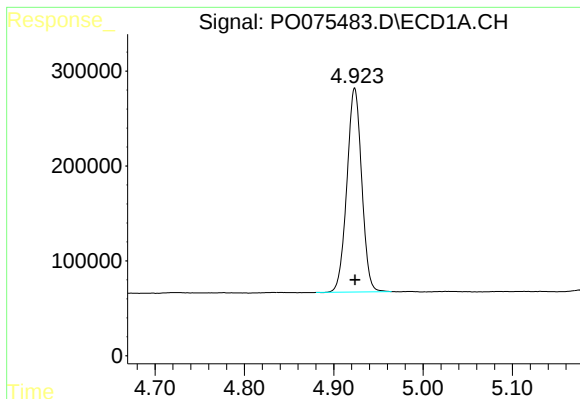


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 2473932
Conc: 24.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-0510


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:15 PM

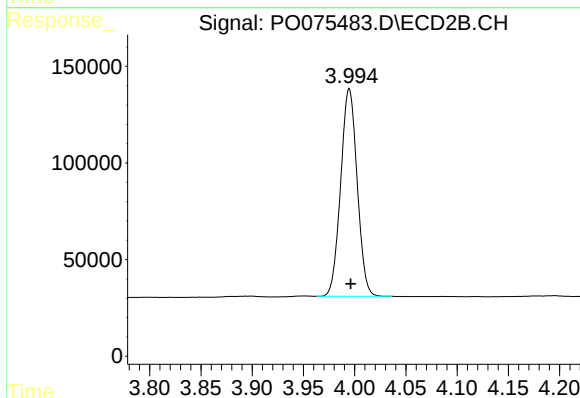


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: -0.002 min
Response: 1200561
Conc: 24.97 ng/ml

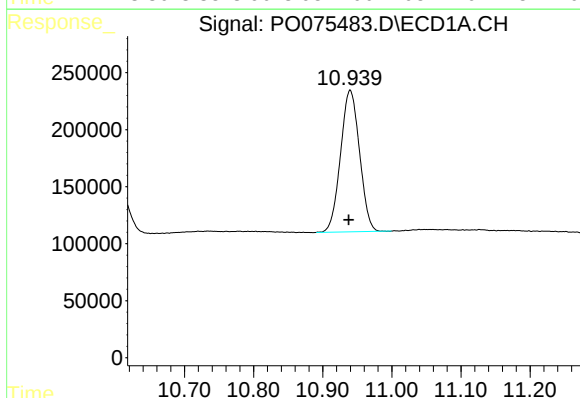


#2 Decachlorobiphenyl

R.T.: 10.940 min
Delta R.T.: 0.002 min
Response: 2368544
Conc: 24.55 ng/ml

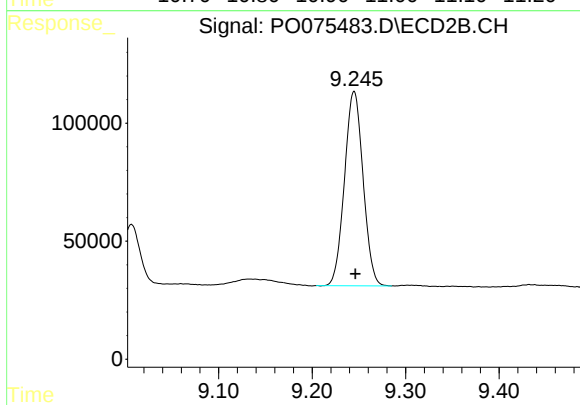

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.001 min
Response: 1137966
Conc: 23.44 ng/ml

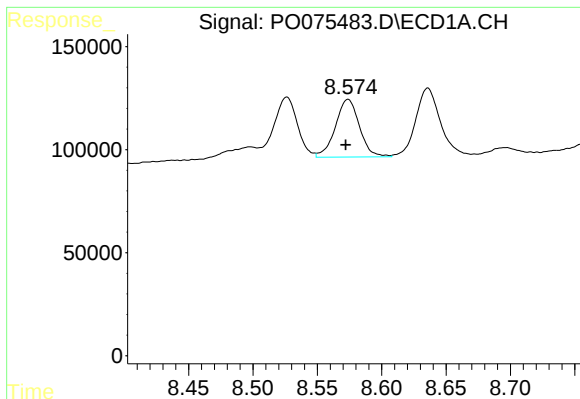


#36 AR-1262-1

R.T.: 8.574 min
Delta R.T.: 0.002 min
Response: 363284
Conc: 41.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-003-0510


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:15 PM

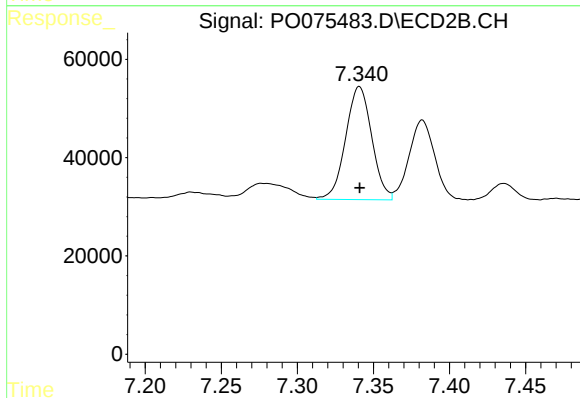


#36 AR-1262-1

R.T.: 7.341 min
Delta R.T.: 0.000 min
Response: 275153
Conc: 126.15 ng/ml

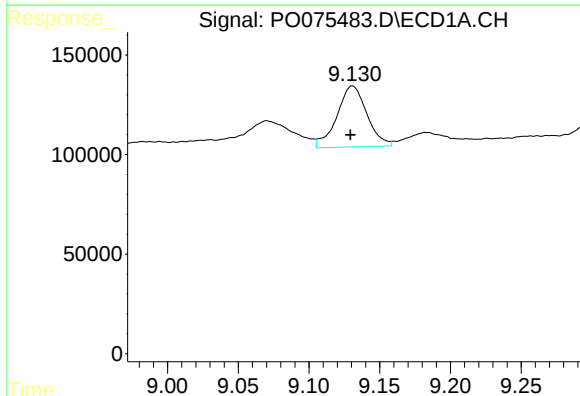


#37 AR-1262-2

R.T.: 9.131 min
Delta R.T.: 0.001 min
Response: 452415
Conc: 29.92 ng/ml

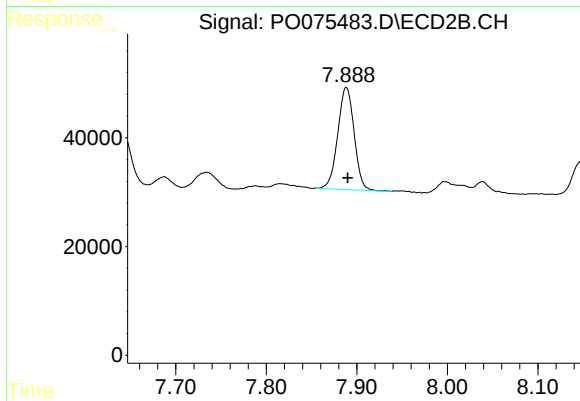

#37 AR-1262-2

R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 237120
Conc: 30.92 ng/ml

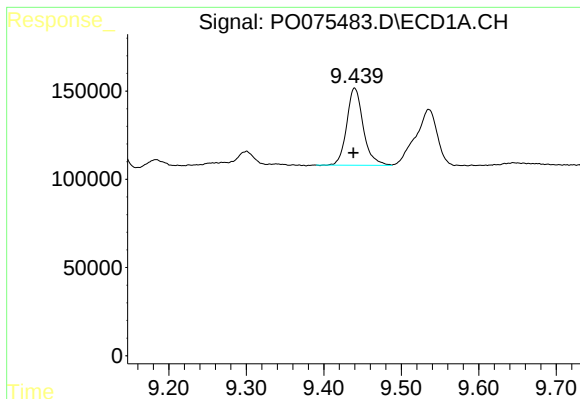


#38 AR-1262-3

R.T.: 9.440 min
Delta R.T.: 0.002 min
Response: 645565
Conc: 61.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-0510


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:15 PM

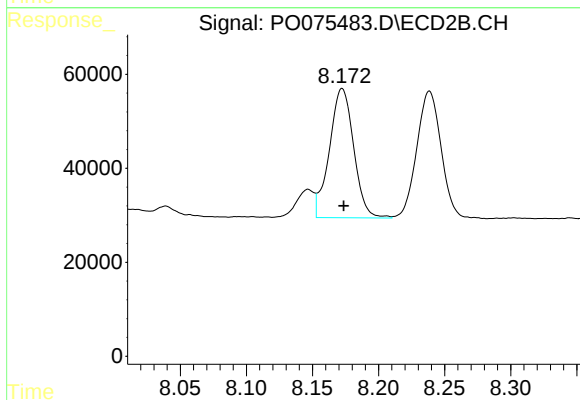


#38 AR-1262-3

R.T.: 8.172 min
Delta R.T.: -0.001 min
Response: 352111
Conc: 106.40 ng/ml

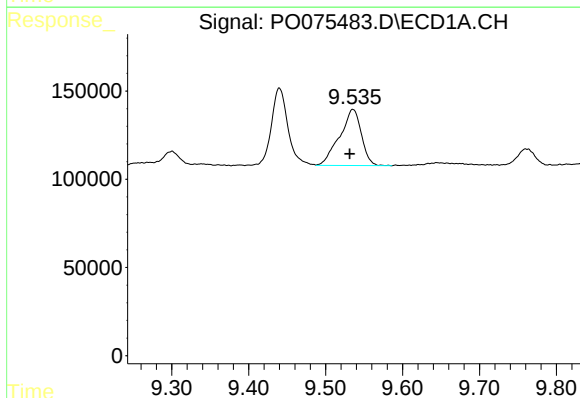


#39 AR-1262-4

R.T.: 9.535 min
Delta R.T.: 0.004 min
Response: 622860
Conc: 84.27 ng/ml

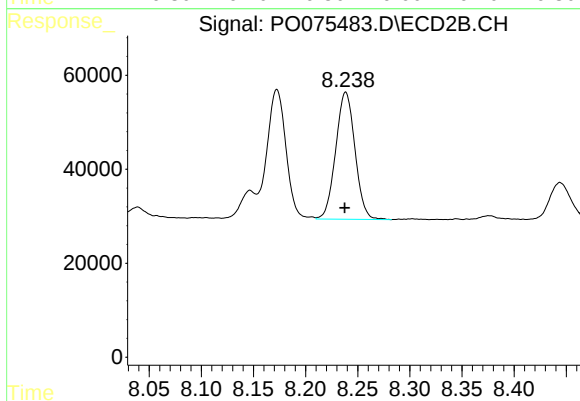

#39 AR-1262-4

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 348633
Conc: 60.72 ng/ml

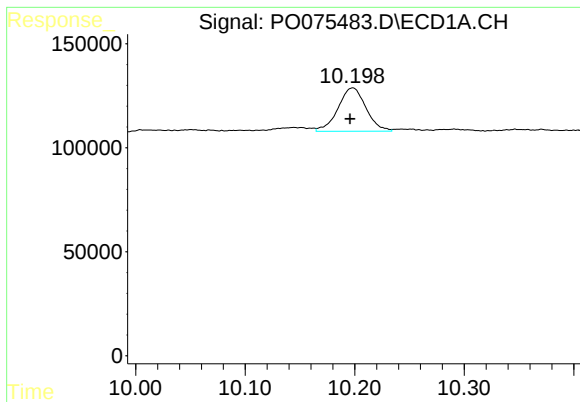


#40 AR-1262-5

R.T.: 10.198 min
Delta R.T.: 0.002 min
Response: 370669
Conc: 71.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-0510

Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:15 PM

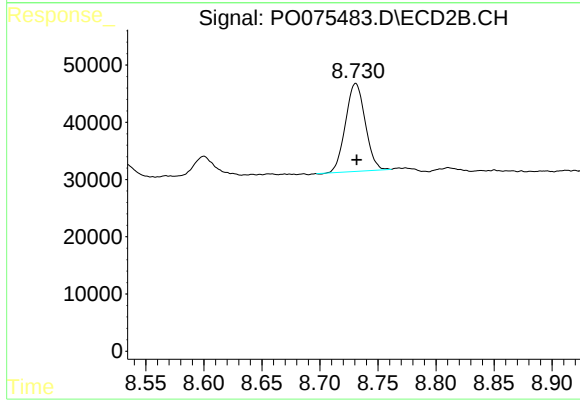

#40 AR-1262-5

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 181346
Conc: 65.92 ng/ml