

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075484.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 5:24
 Operator : AJ/MA
 Sample : M1292-08
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-003-1015

Manual Integrations
 APPROVED

Ankita
 2/4/2021 1:52:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 06:47:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.994	2700709	1298433	26.686	27.010
2) SA Decachlor...	10.936	9.243	3548633	1676329	36.780	34.534
Target Compounds						
36) L8 AR-1262-1	8.571	7.339	163388	126389	18.723m	57.944 #
37) L8 AR-1262-2	9.129	7.888	182926	148863	12.097m	19.411m#
38) L8 AR-1262-3	9.437	8.170	332106	183345	31.790	55.402m#
39) L8 AR-1262-4	9.533	8.236	322238	184636	43.598	32.156 #
40) L8 AR-1262-5	10.196	8.729	224932	102143	43.374	37.131

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075484.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 5:24
Operator : AJ/MA
Sample : M1292-08
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 06:47:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

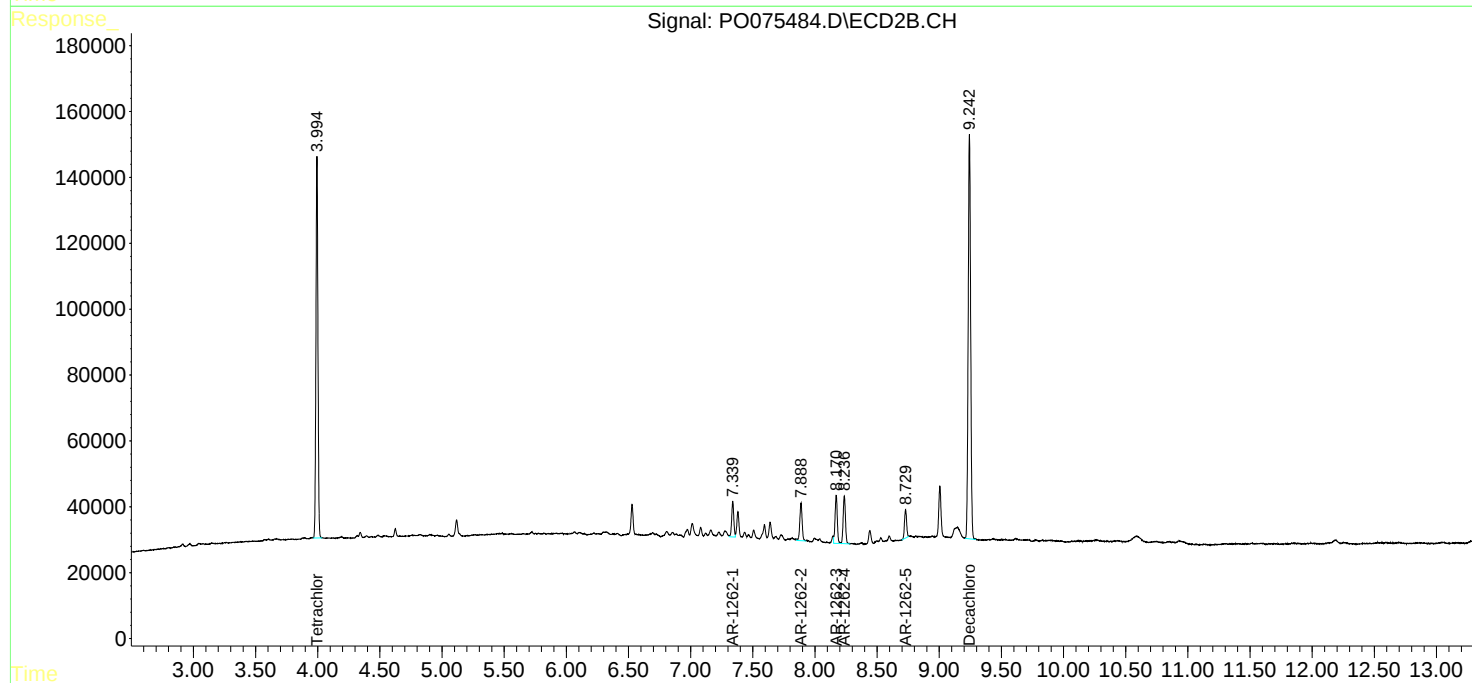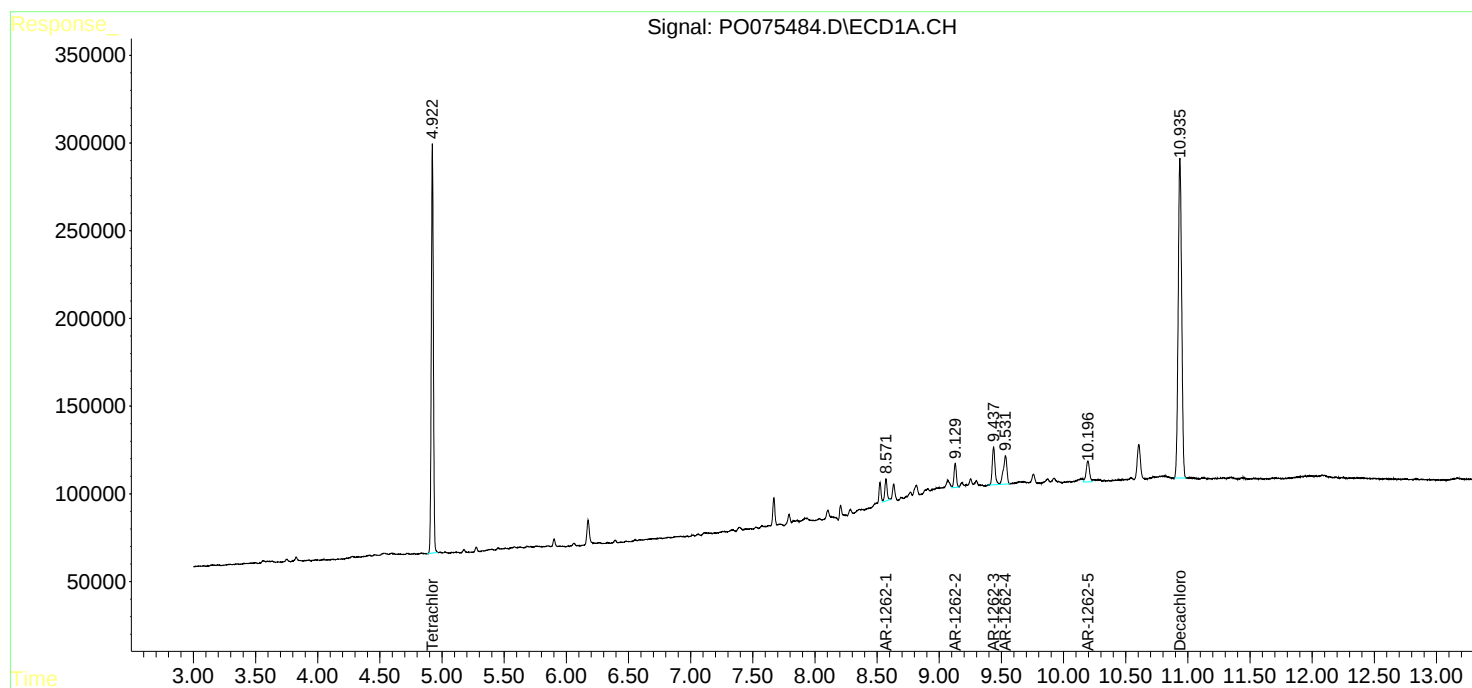

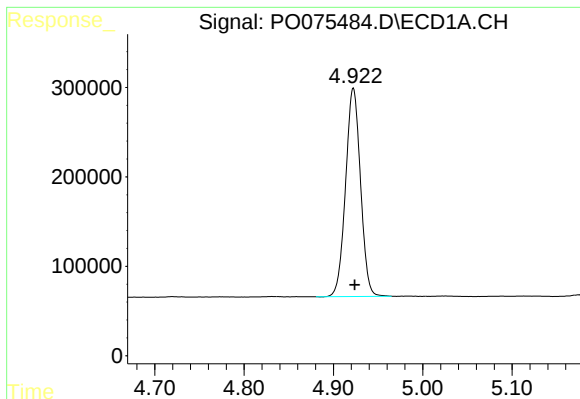


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 2700709
Conc: 26.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:17 PM

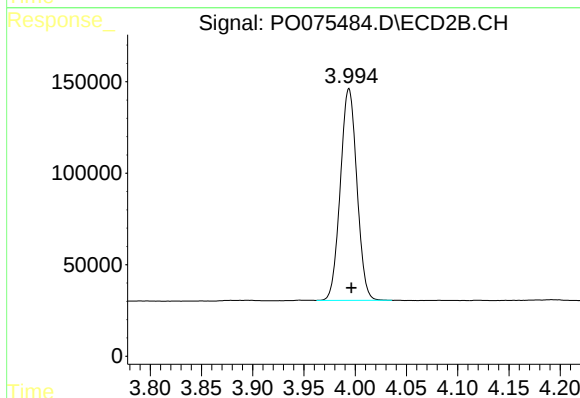


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1298433
Conc: 27.01 ng/ml

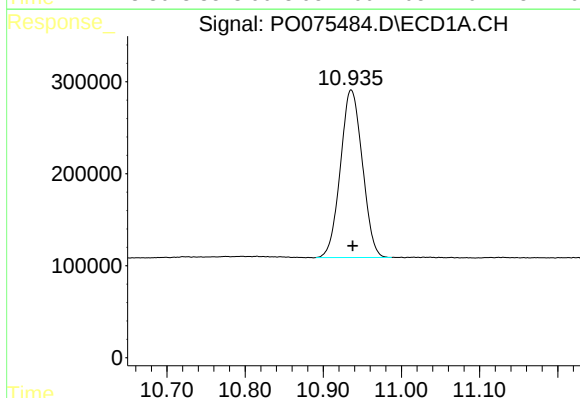


#2 Decachlorobiphenyl

R.T.: 10.936 min
Delta R.T.: -0.002 min
Response: 3548633
Conc: 36.78 ng/ml

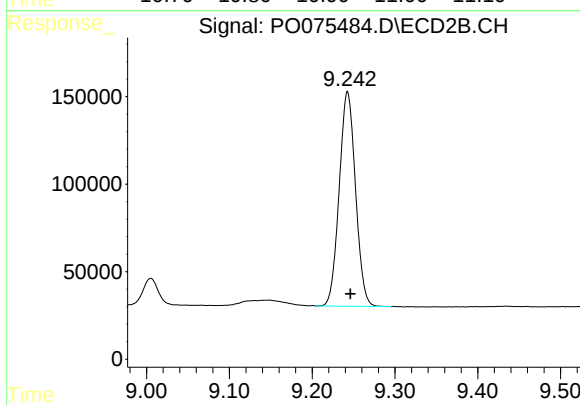

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 1676329
Conc: 34.53 ng/ml

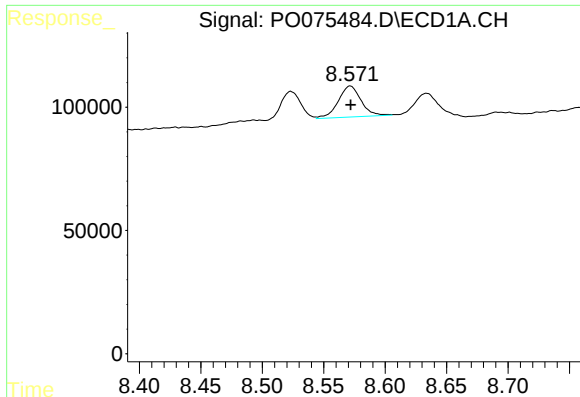


#36 AR-1262-1

R.T.: 8.571 min
Delta R.T.: -0.001 min
Response: 163388
Conc: 18.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:17 PM

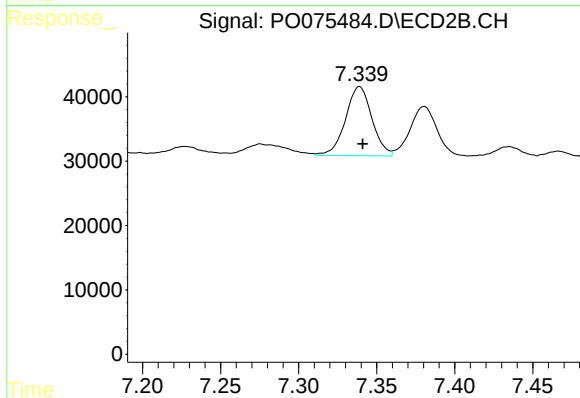


#36 AR-1262-1

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 126389
Conc: 57.94 ng/ml

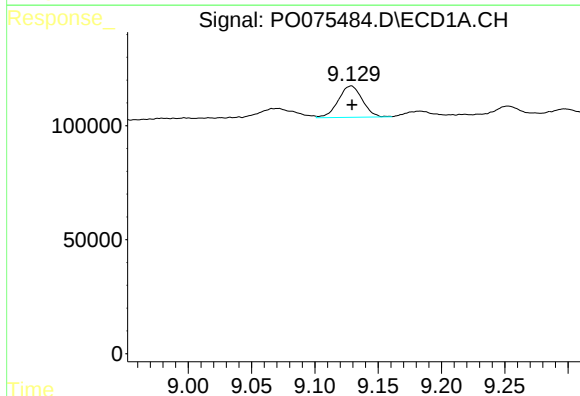


#37 AR-1262-2

R.T.: 9.129 min
Delta R.T.: 0.000 min
Response: 182926
Conc: 12.10 ng/ml m

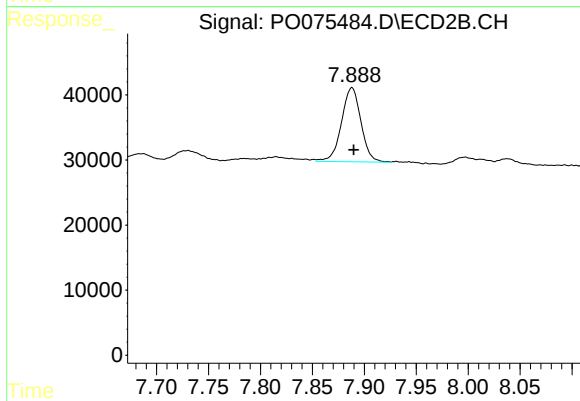

#37 AR-1262-2

R.T.: 7.888 min
Delta R.T.: -0.002 min
Response: 148863
Conc: 19.41 ng/ml m

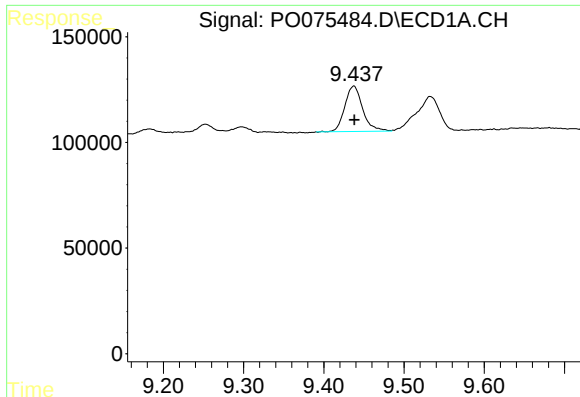


#38 AR-1262-3

R.T.: 9.437 min
Delta R.T.: 0.000 min
Response: 332106
Conc: 31.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:17 PM

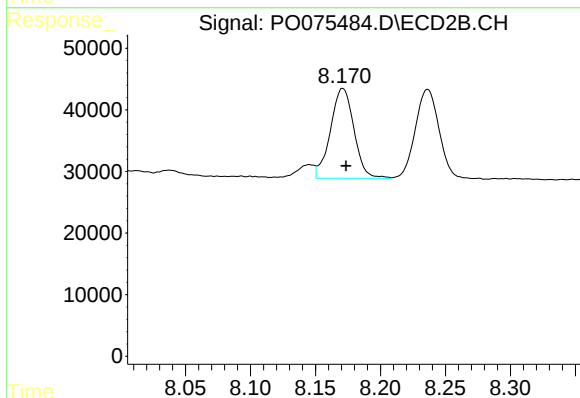


#38 AR-1262-3

R.T.: 8.170 min
Delta R.T.: -0.003 min
Response: 183345
Conc: 55.40 ng/ml m

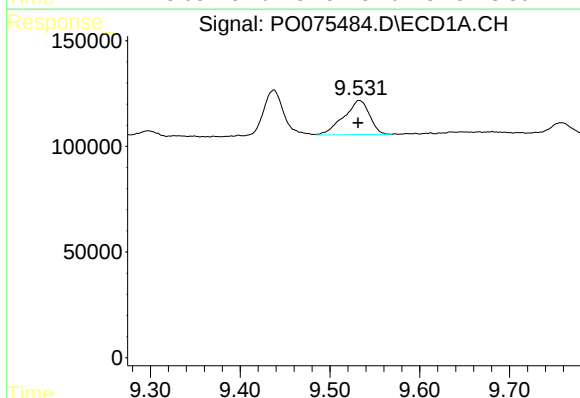


#39 AR-1262-4

R.T.: 9.533 min
Delta R.T.: 0.001 min
Response: 322238
Conc: 43.60 ng/ml

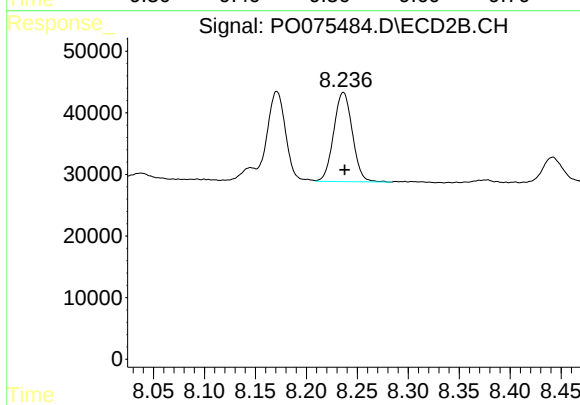

#39 AR-1262-4

R.T.: 8.236 min
Delta R.T.: -0.001 min
Response: 184636
Conc: 32.16 ng/ml

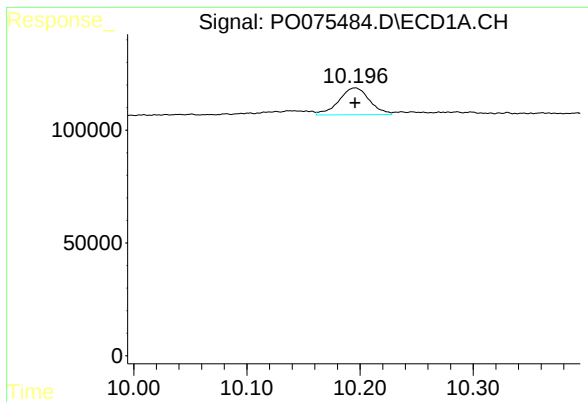


#40 AR-1262-5

R.T.: 10.196 min
Delta R.T.: 0.000 min
Response: 224932
Conc: 43.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-003-1015

Manual Integrations
APPROVED

Ankita
2/4/2021 1:52:17 PM

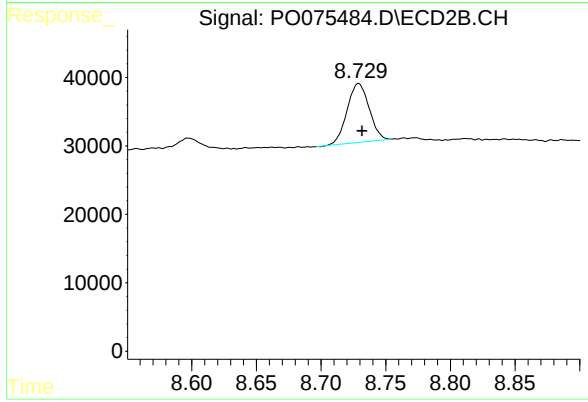

#40 AR-1262-5

R.T.: 8.729 min
Delta R.T.: -0.003 min
Response: 102143
Conc: 37.13 ng/ml