

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075496.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 9:58
 Operator : AJ/MA
 Sample : M1292-15
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-010-0510

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:26:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 14:19:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.994	2411822	1173182	23.832	24.405
2) SA Decachlor...	10.937	9.243	2441770	1196990	25.308	24.659
Target Compounds						
36) L8 AR-1262-1	8.572	7.339	497750	68978	57.039m	31.623 #
37) L8 AR-1262-2	9.129	7.887	330368	196823	21.847m	25.665
38) L8 AR-1262-3	9.437	8.171	752597	380990	72.041	115.126 #
39) L8 AR-1262-4	9.534	8.237	774014	419159	104.722	73.001 #
40) L8 AR-1262-5	10.195	8.729	354322	196493	68.324	71.430

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020321\
Data File : PO075496.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 9:58
Operator : AJ/MA
Sample : M1292-15
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OU421-010-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 14:19:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

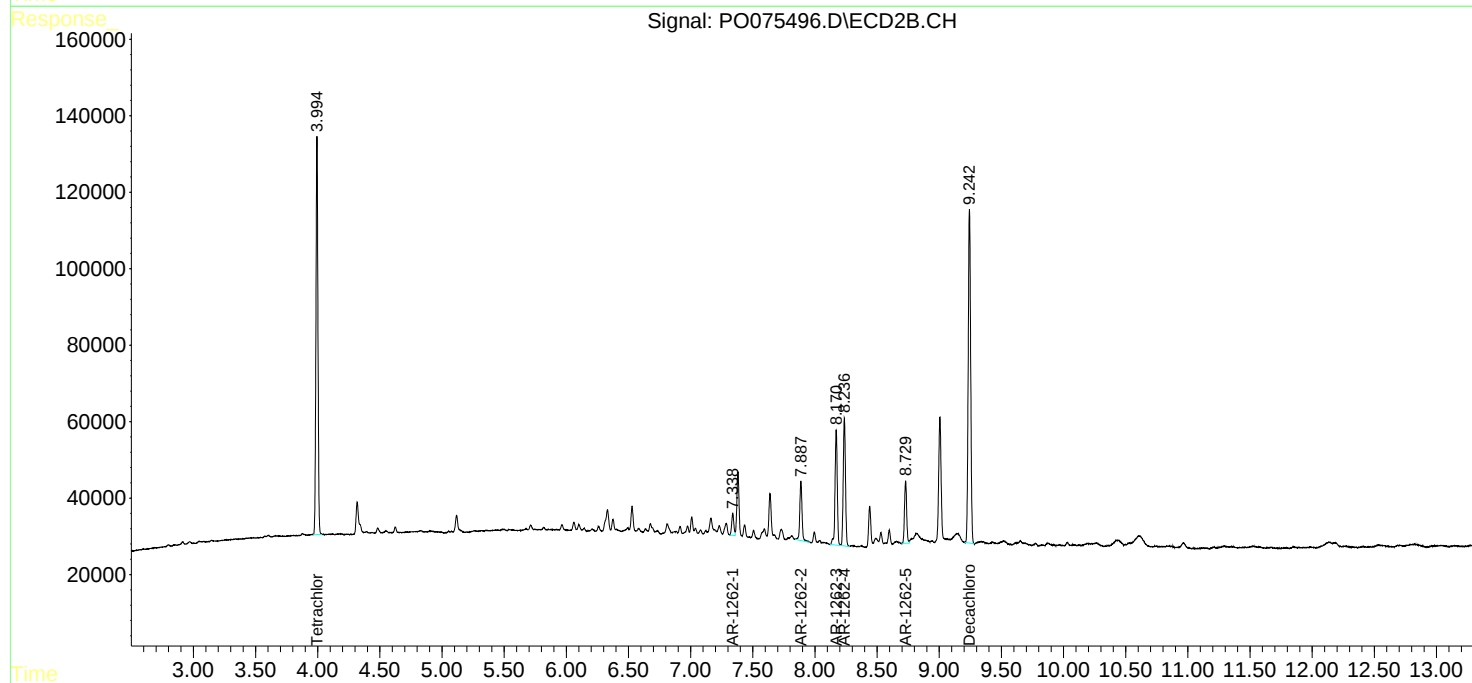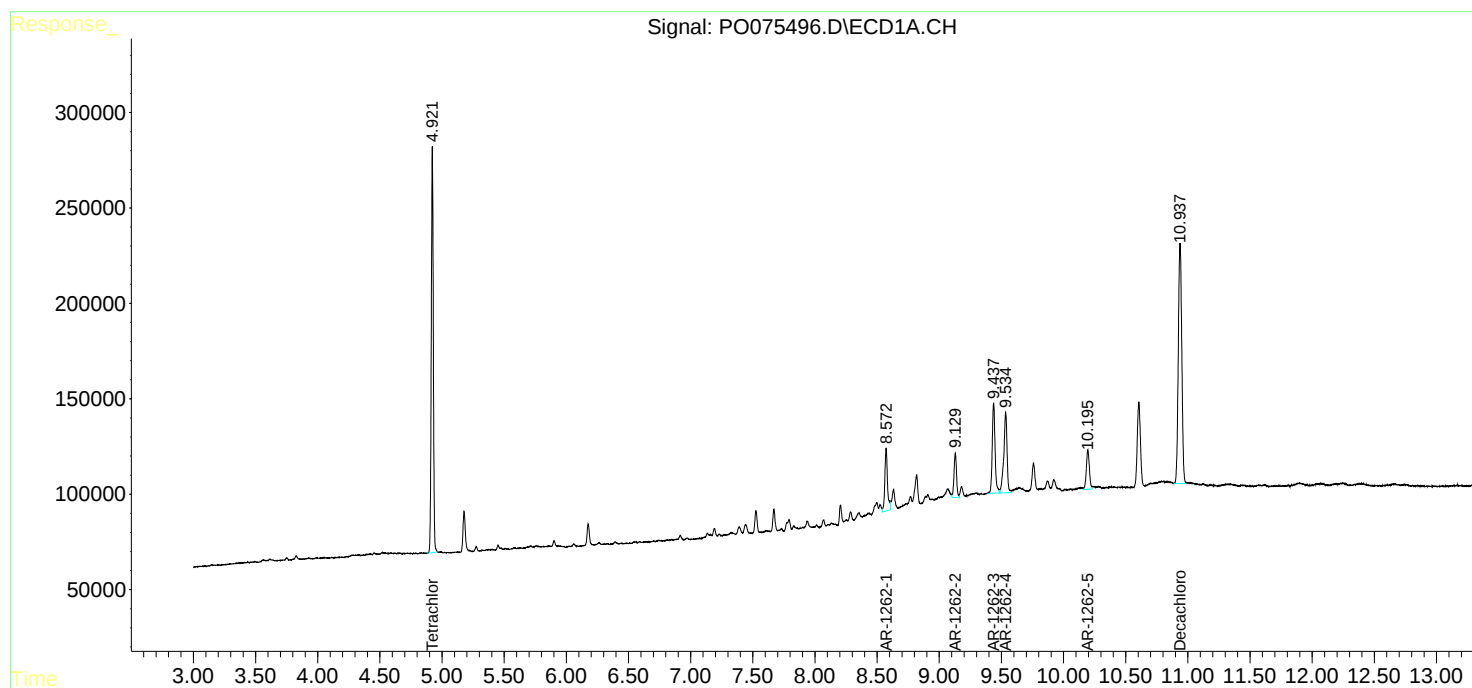

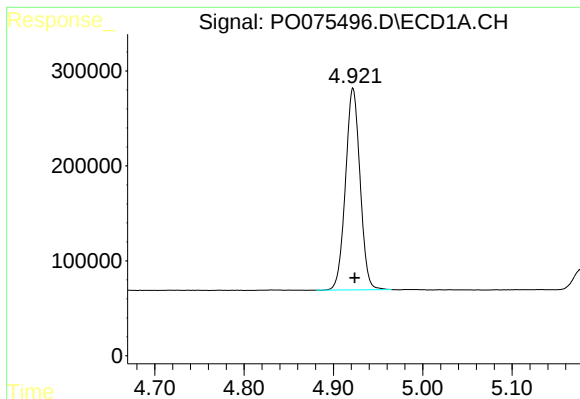


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 2411822
Conc: 23.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-010-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:24 AM

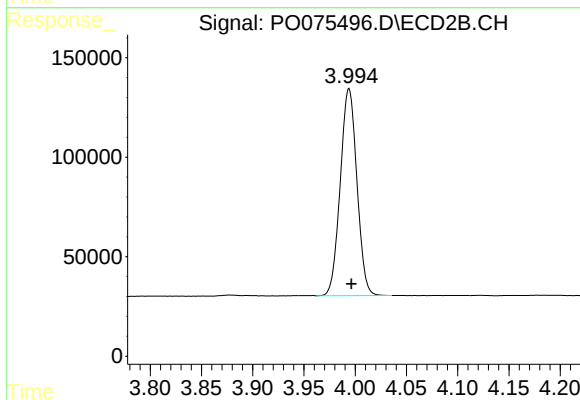


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1173182
Conc: 24.40 ng/ml

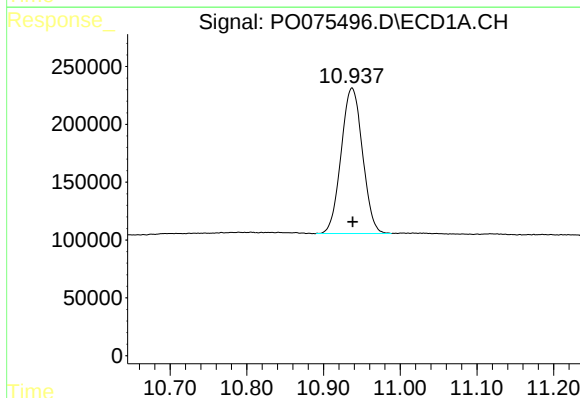


#2 Decachlorobiphenyl

R.T.: 10.937 min
Delta R.T.: 0.000 min
Response: 2441770
Conc: 25.31 ng/ml

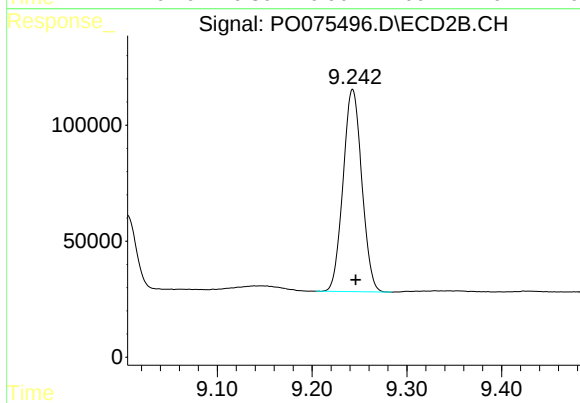

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 1196990
Conc: 24.66 ng/ml

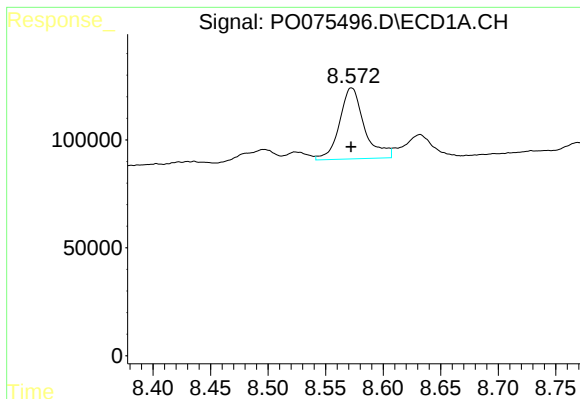


#36 AR-1262-1

R.T.: 8.572 min
Delta R.T.: 0.000 min
Response: 497750
Conc: 57.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-010-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:24 AM

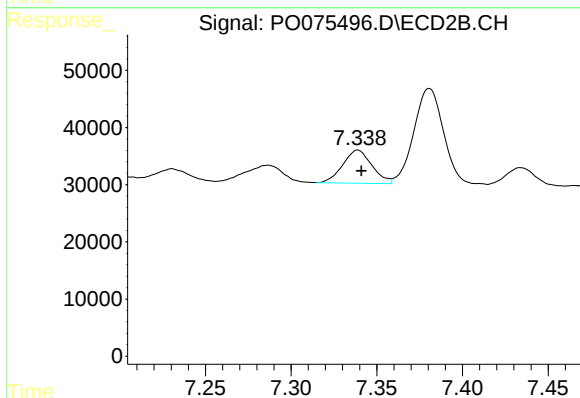


#36 AR-1262-1

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 68978
Conc: 31.62 ng/ml

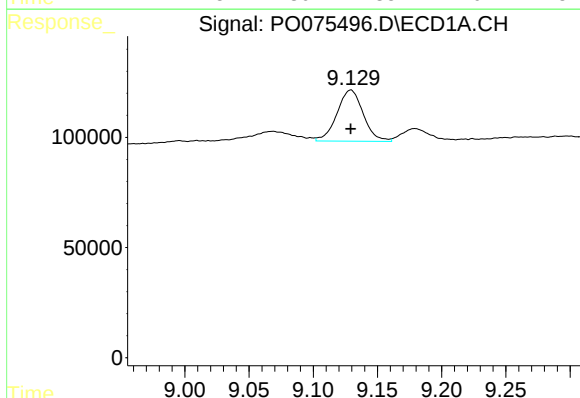


#37 AR-1262-2

R.T.: 9.129 min
Delta R.T.: 0.000 min
Response: 330368
Conc: 21.85 ng/ml m

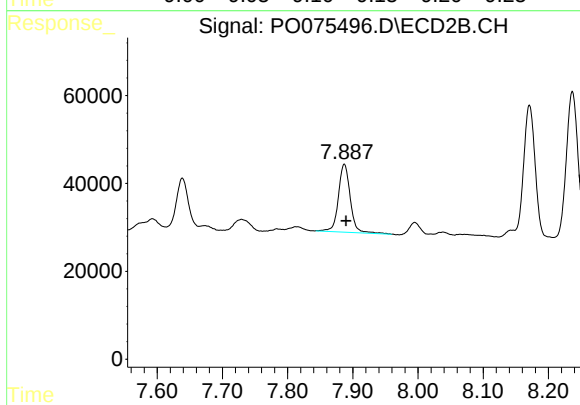

#37 AR-1262-2

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 196823
Conc: 25.66 ng/ml

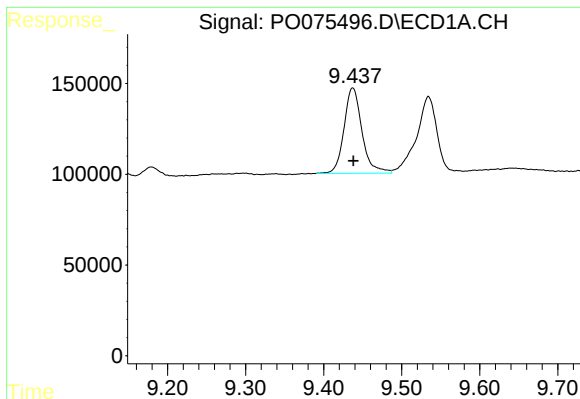


#38 AR-1262-3

R.T.: 9.437 min
Delta R.T.: 0.000 min
Response: 752597
Conc: 72.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-010-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:24 AM

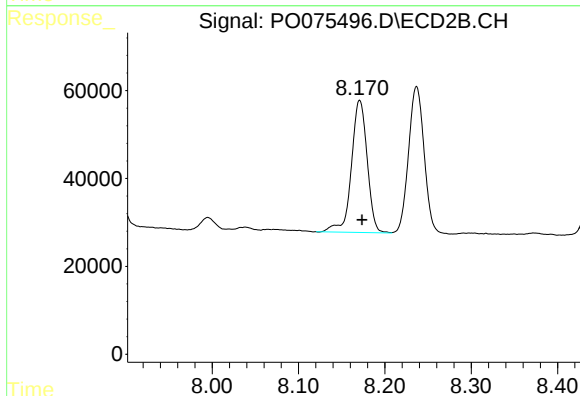


#38 AR-1262-3

R.T.: 8.171 min
Delta R.T.: -0.003 min
Response: 380990
Conc: 115.13 ng/ml

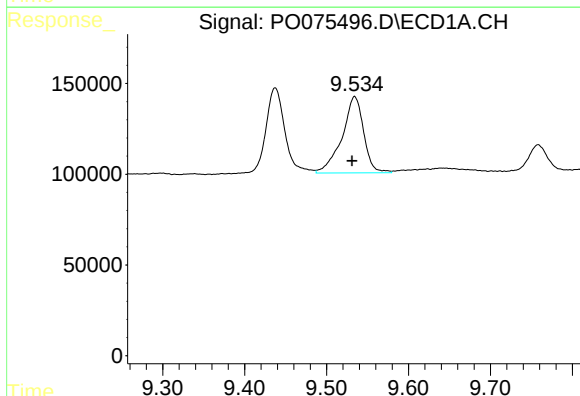


#39 AR-1262-4

R.T.: 9.534 min
Delta R.T.: 0.003 min
Response: 774014
Conc: 104.72 ng/ml

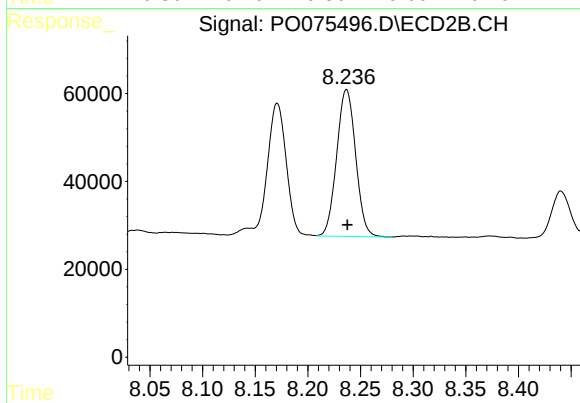

#39 AR-1262-4

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 419159
Conc: 73.00 ng/ml

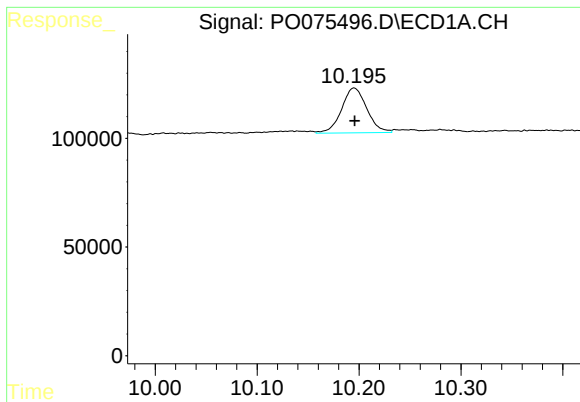


#40 AR-1262-5

R.T.: 10.195 min
Delta R.T.: 0.000 min
Response: 354322
Conc: 68.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-010-0510

Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:24 AM

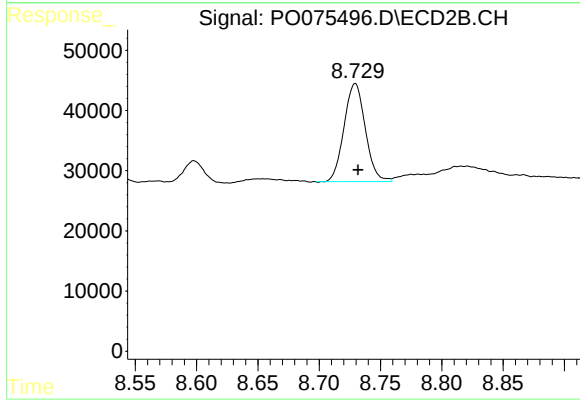

#40 AR-1262-5

R.T.: 8.729 min
Delta R.T.: -0.002 min
Response: 196493
Conc: 71.43 ng/ml