

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020321\
 Data File : P0075498.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 10:32
 Operator : AJ/MA
 Sample : M1292-17
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2021-01-28-FD04

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:26:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 14:20:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.923	3.994	2483805	1204935	24.543	25.065
2)	SA Decachlor...	10.936	9.243	2624989	1282728	27.207	26.425
Target Compounds							
36)	L8 AR-1262-1	8.571	7.337	367451	18295	42.108	8.387m#
37)	L8 AR-1262-2	9.129	7.887	347604	169398	22.987	22.089
38)	L8 AR-1262-3	9.438	8.171	606068	320580	58.014	96.872 #
39)	L8 AR-1262-4	9.534	8.237	615002	330346	83.208	57.533 #
40)	L8 AR-1262-5	10.194	8.729	386548	184672	74.538	67.133

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO075498.D
Data File : PO075498.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 10:32
Operator : AJ/MA
Sample : M1292-17
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2021-01-28-FD04


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 14:20:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

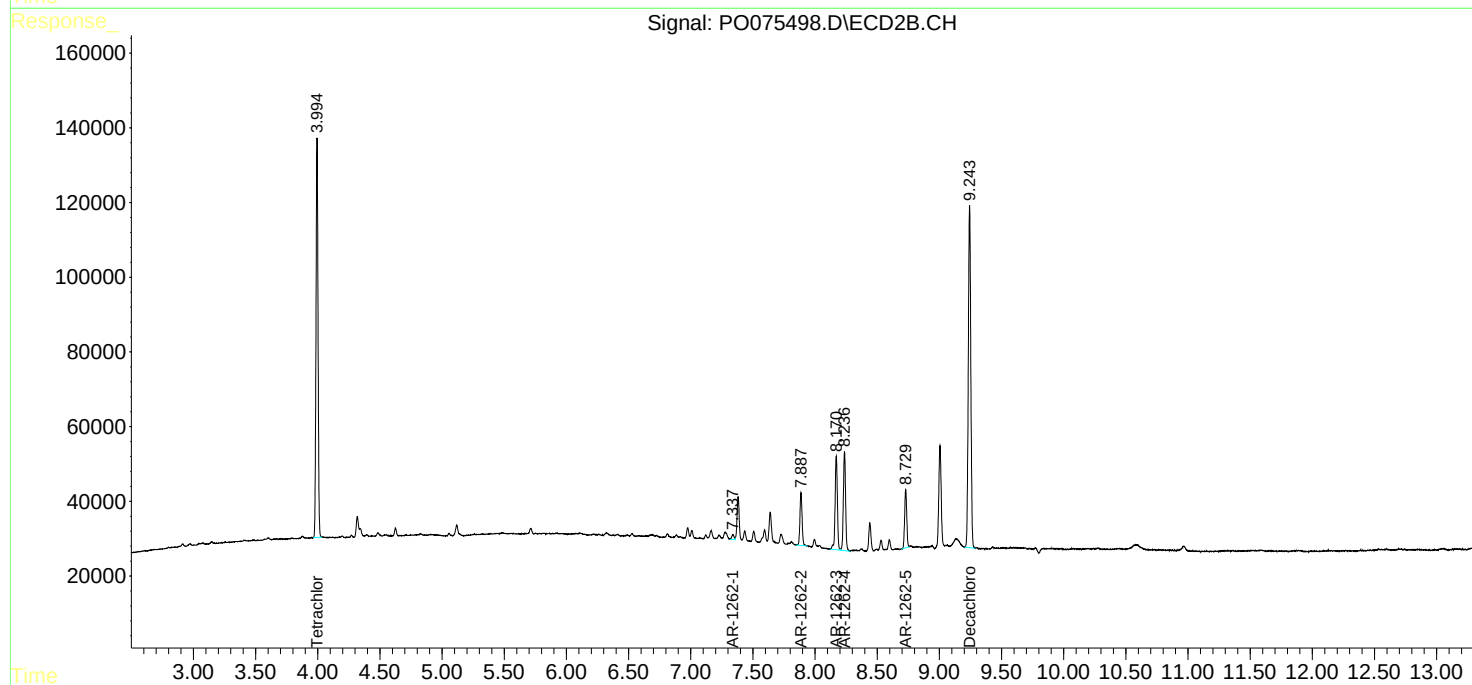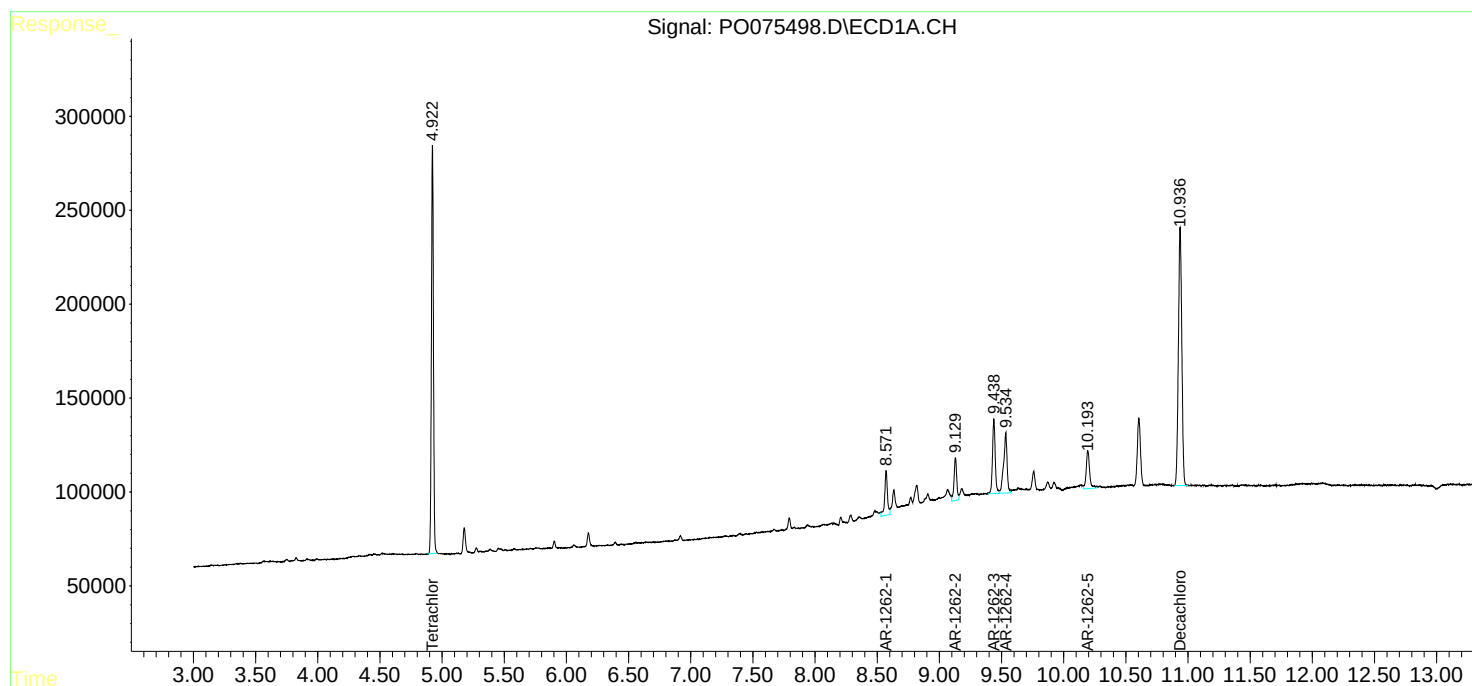

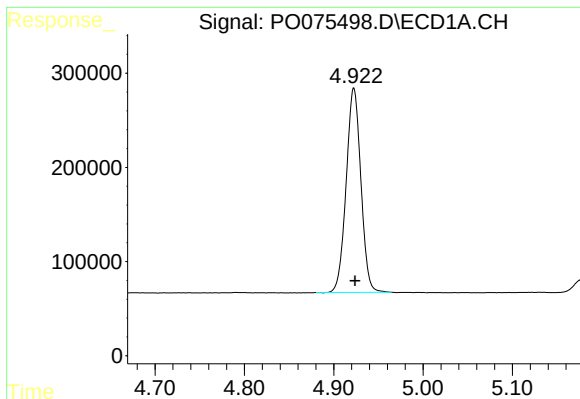


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 2483805
Conc: 24.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
2021-01-28-FD04


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:28 AM

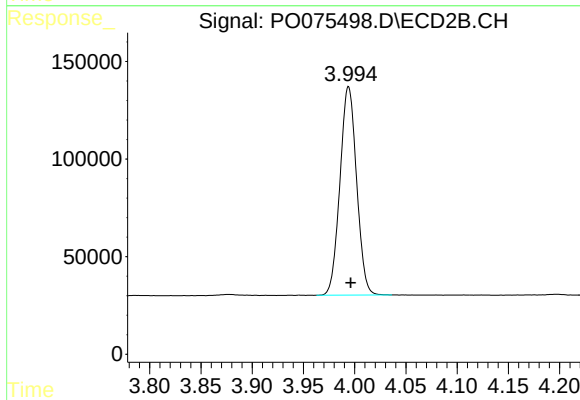


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1204935
Conc: 25.07 ng/ml

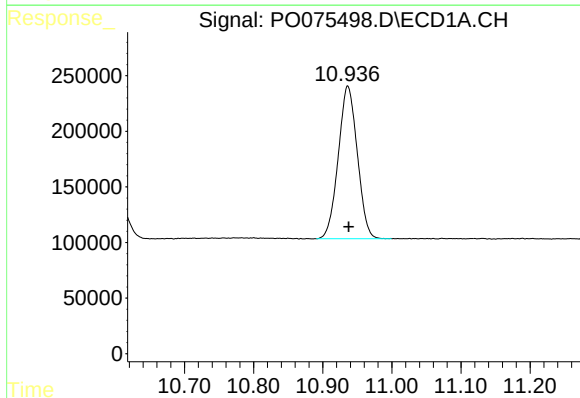


#2 Decachlorobiphenyl

R.T.: 10.936 min
Delta R.T.: -0.002 min
Response: 2624989
Conc: 27.21 ng/ml

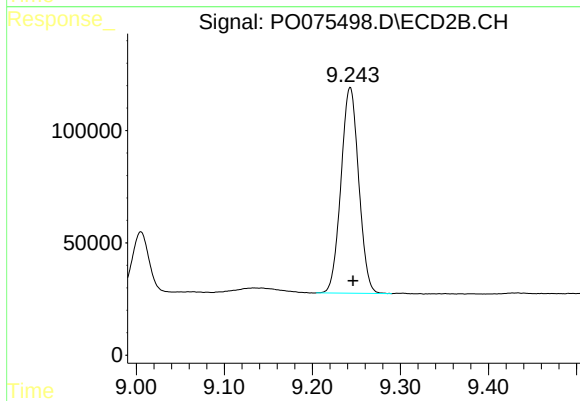

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 1282728
Conc: 26.43 ng/ml

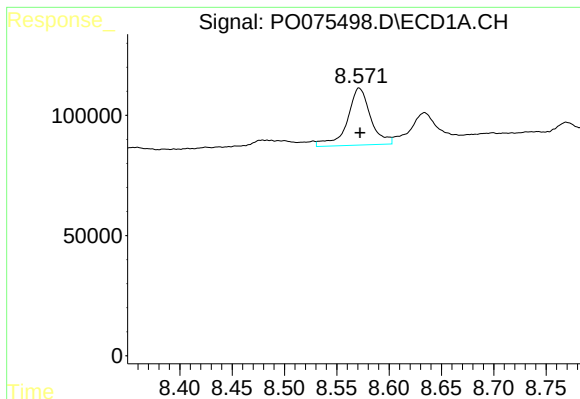


#36 AR-1262-1

R.T.: 8.571 min
Delta R.T.: 0.000 min
Response: 367451
Conc: 42.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
2021-01-28-FD04


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:28 AM

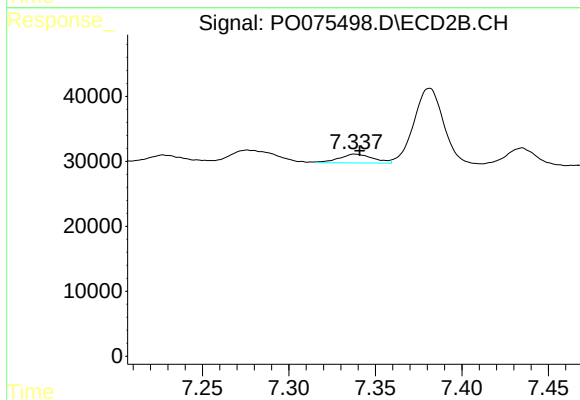


#36 AR-1262-1

R.T.: 7.337 min
Delta R.T.: -0.004 min
Response: 18295
Conc: 8.39 ng/ml m

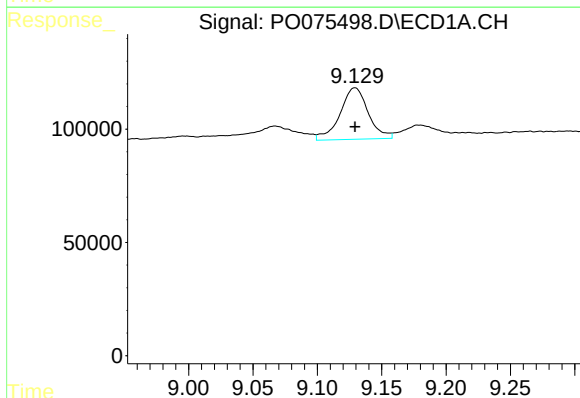


#37 AR-1262-2

R.T.: 9.129 min
Delta R.T.: 0.000 min
Response: 347604
Conc: 22.99 ng/ml

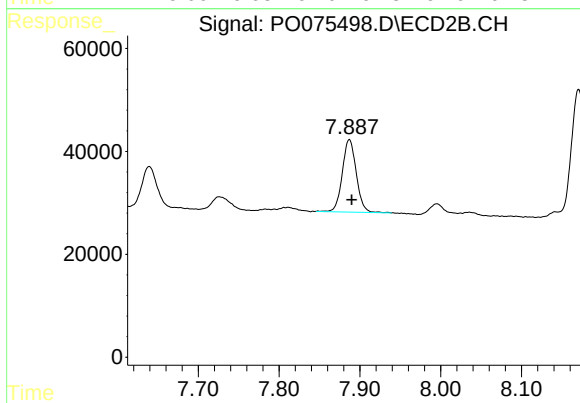

#37 AR-1262-2

R.T.: 7.887 min
Delta R.T.: -0.003 min
Response: 169398
Conc: 22.09 ng/ml

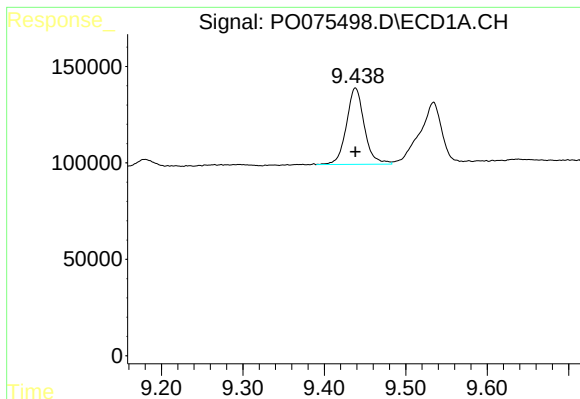


#38 AR-1262-3

R.T.: 9.438 min
Delta R.T.: 0.000 min
Response: 606068
Conc: 58.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
2021-01-28-FD04


Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:28 AM

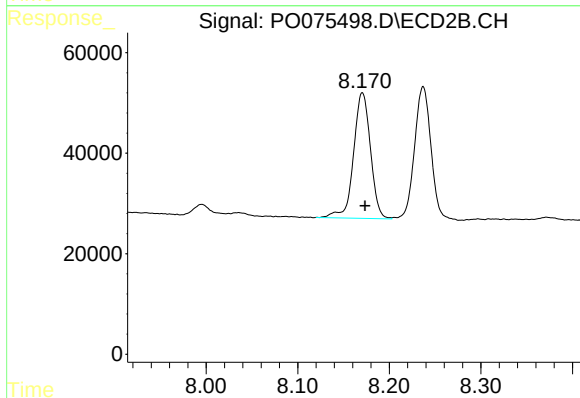


#38 AR-1262-3

R.T.: 8.171 min
Delta R.T.: -0.003 min
Response: 320580
Conc: 96.87 ng/ml

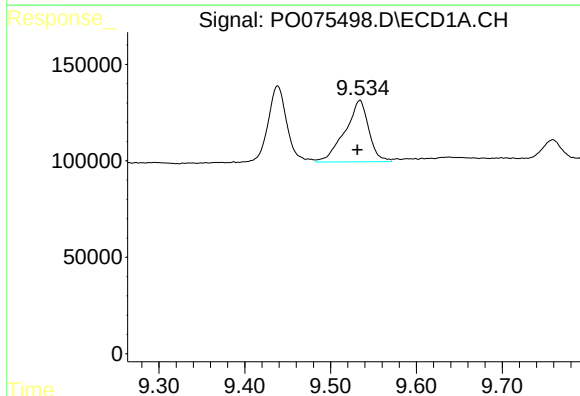


#39 AR-1262-4

R.T.: 9.534 min
Delta R.T.: 0.003 min
Response: 615002
Conc: 83.21 ng/ml

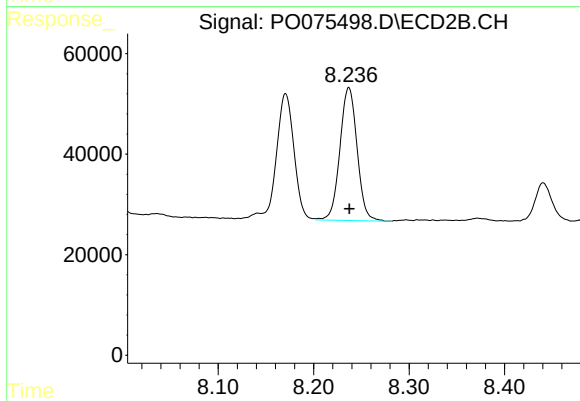

#39 AR-1262-4

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 330346
Conc: 57.53 ng/ml

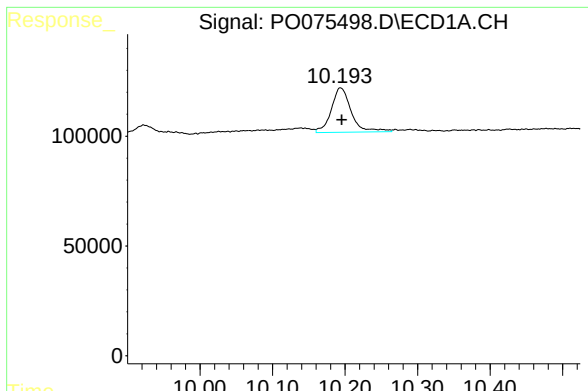


#40 AR-1262-5

R.T.: 10.194 min
Delta R.T.: -0.002 min
Response: 386548
Conc: 74.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
2021-01-28-FD04

Manual Integrations
APPROVED

Ankita
2/8/2021 8:26:28 AM

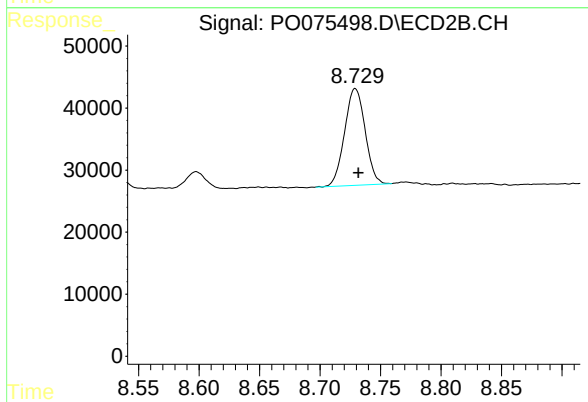

#40 AR-1262-5

R.T.: 8.729 min
Delta R.T.: -0.003 min
Response: 184672
Conc: 67.13 ng/ml