

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020322\
Data File : P0084464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2022 10:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 05:23:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 04 05:20:27 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	6.561	5.532	1173505	520046	21.753	22.411
2)	SA Decachlor...	13.806	11.525	721066	387514	19.885	21.876

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020322\
Data File : P0084464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2022 10:43
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 05:23:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 04 05:20:27 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

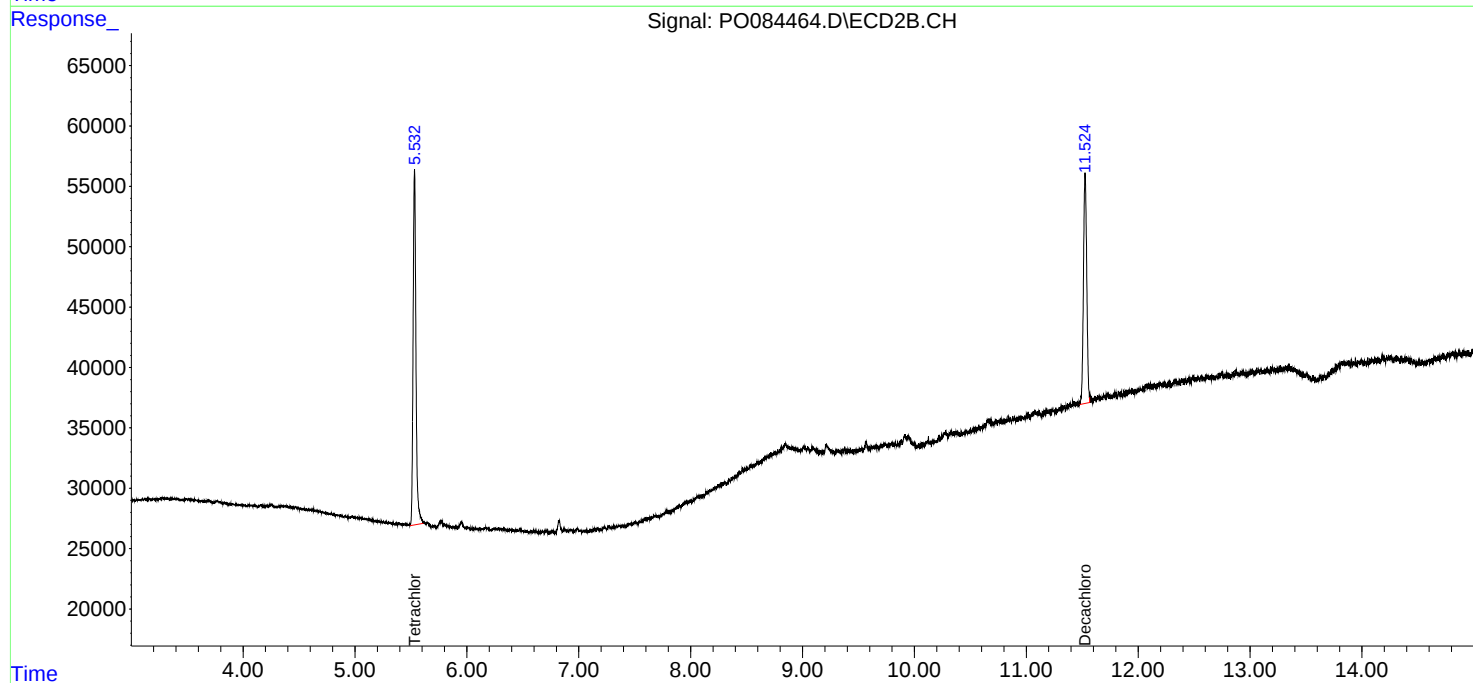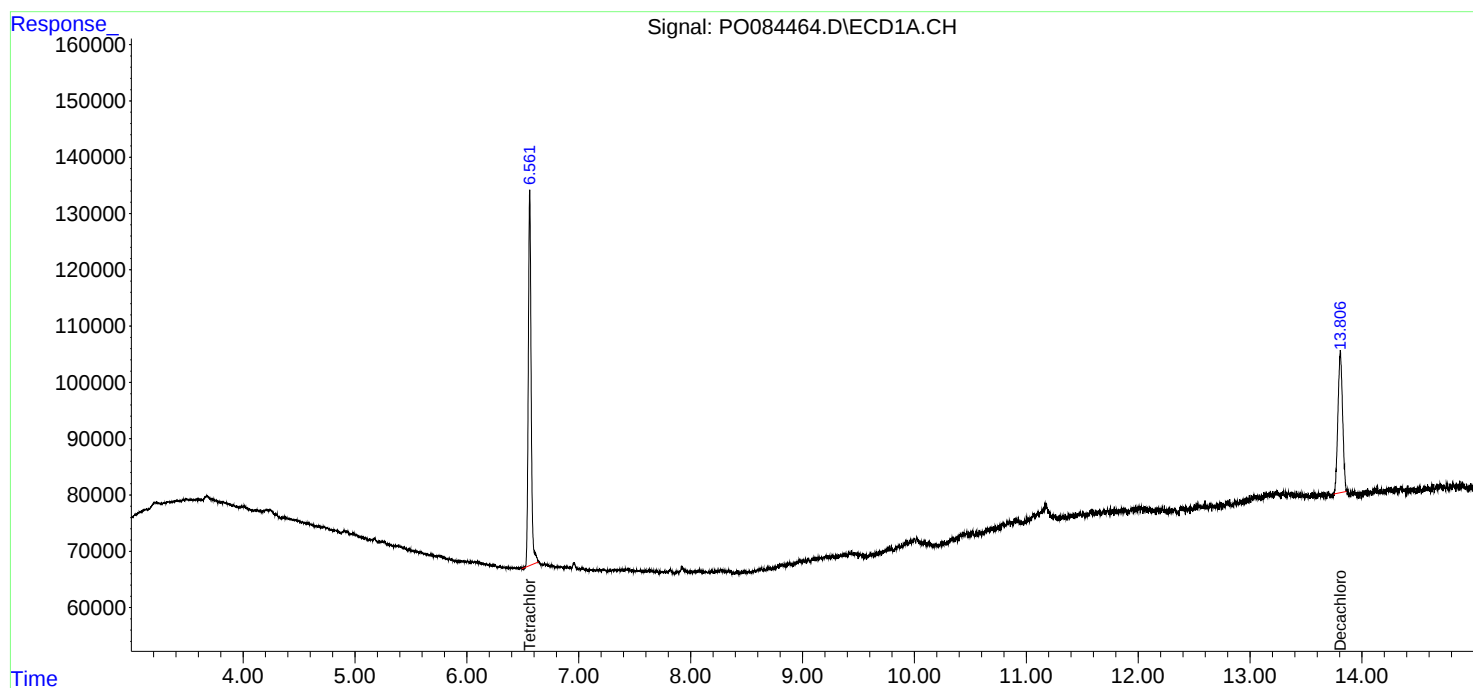


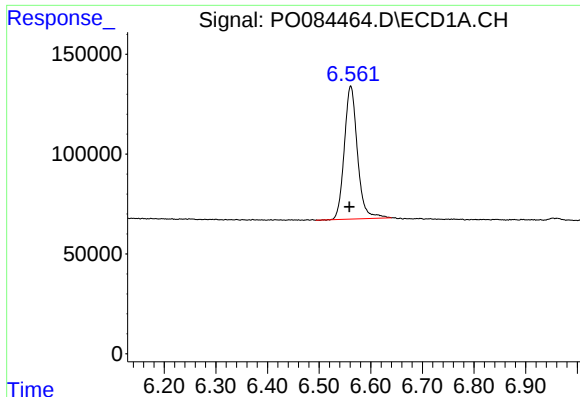

#1 Tetrachloro-m-xylene


R.T.: 6.561 min
Delta R.T.: 0.002 min
Response: 1173505
Conc: 21.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

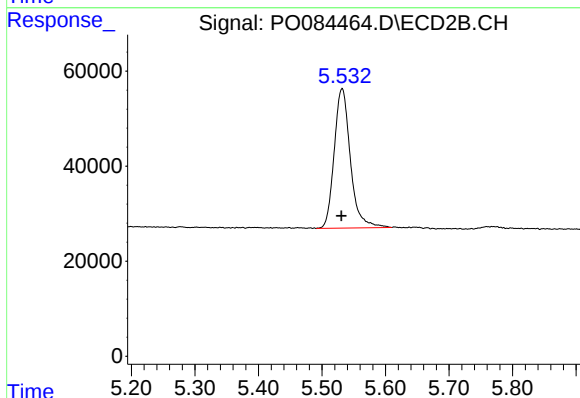


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.001 min
Response: 520046
Conc: 22.41 ng/ml

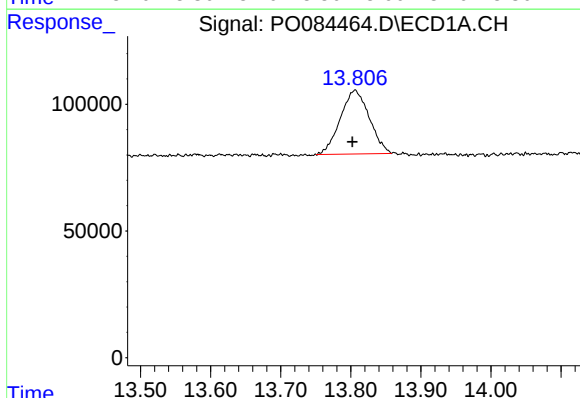

#2 Decachlorobiphenyl

R.T.: 13.806 min
Delta R.T.: 0.004 min
Response: 721066
Conc: 19.88 ng/ml

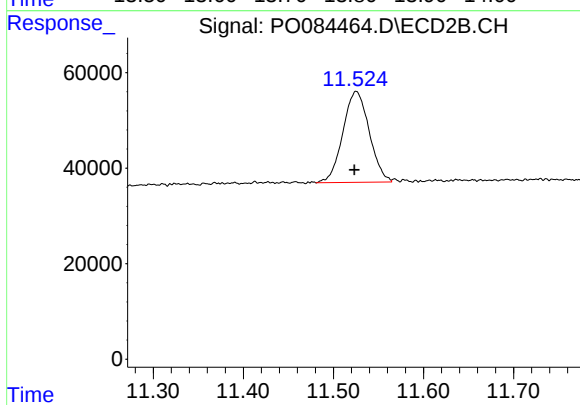

#2 Decachlorobiphenyl

R.T.: 11.525 min
Delta R.T.: 0.002 min
Response: 387514
Conc: 21.88 ng/ml