

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0020322\
 Data File : P0084476.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2022 14:29
 Operator : AJ\MA
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/04/2022
 Supervised By :Ankita Jodhani 02/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 01:23:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0020322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 04 01:22:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	6.558	5.530	314615	130466	5.449	5.243
2) SA Decachlor...	13.803	11.523	179108	89181	5.214m	5.006
Target Compounds						
16) L4 AR-1242-1	8.004	6.976	65590	38926	50.656	58.279m
17) L4 AR-1242-2	8.028	6.998	107421	54422	52.380	55.232m
18) L4 AR-1242-3	8.105	7.217	62634	27600	49.059	53.391m
19) L4 AR-1242-4	8.215	7.314	48383	27852	46.791	51.435m
20) L4 AR-1242-5	9.044	7.922	42807	34563	44.838	55.832

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020322\
Data File : P0084476.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2022 14:29
Operator : AJ\MA
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 01:23:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 04 01:22:53 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

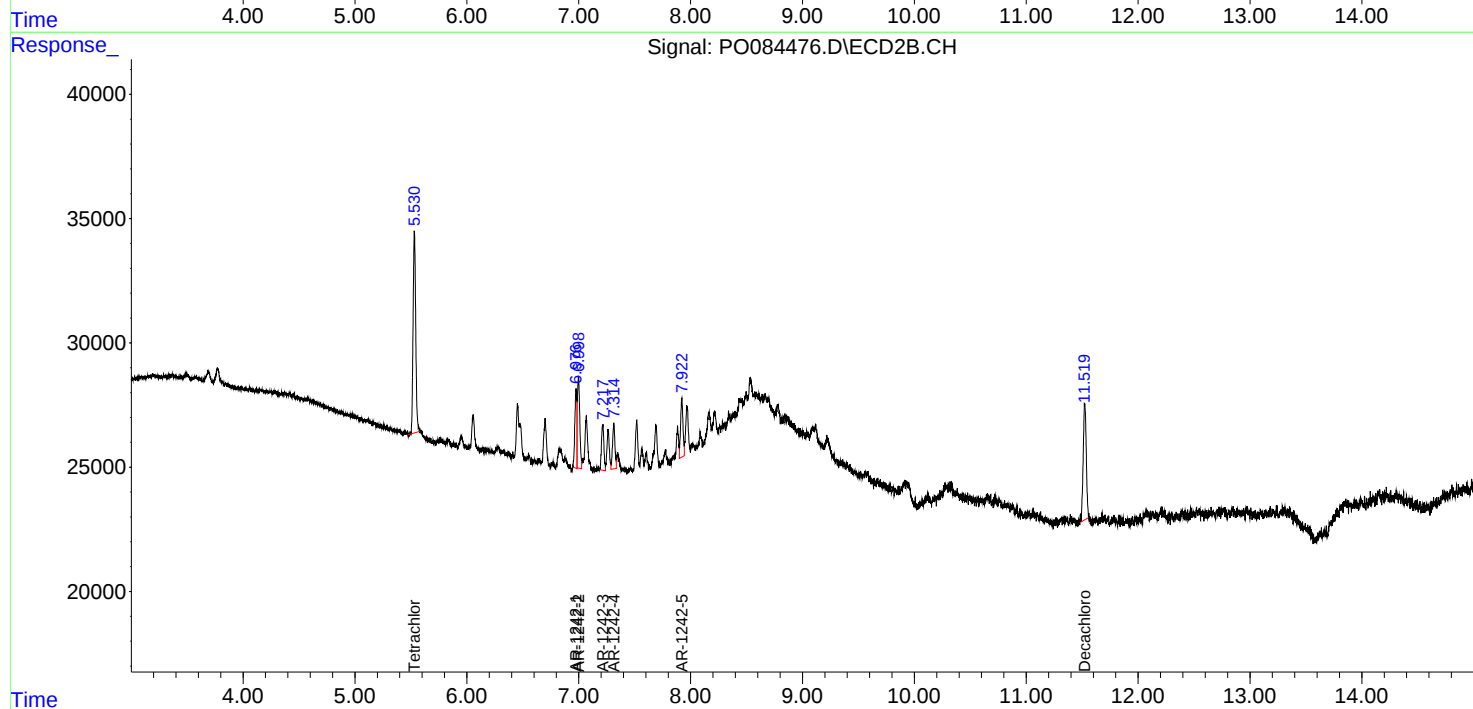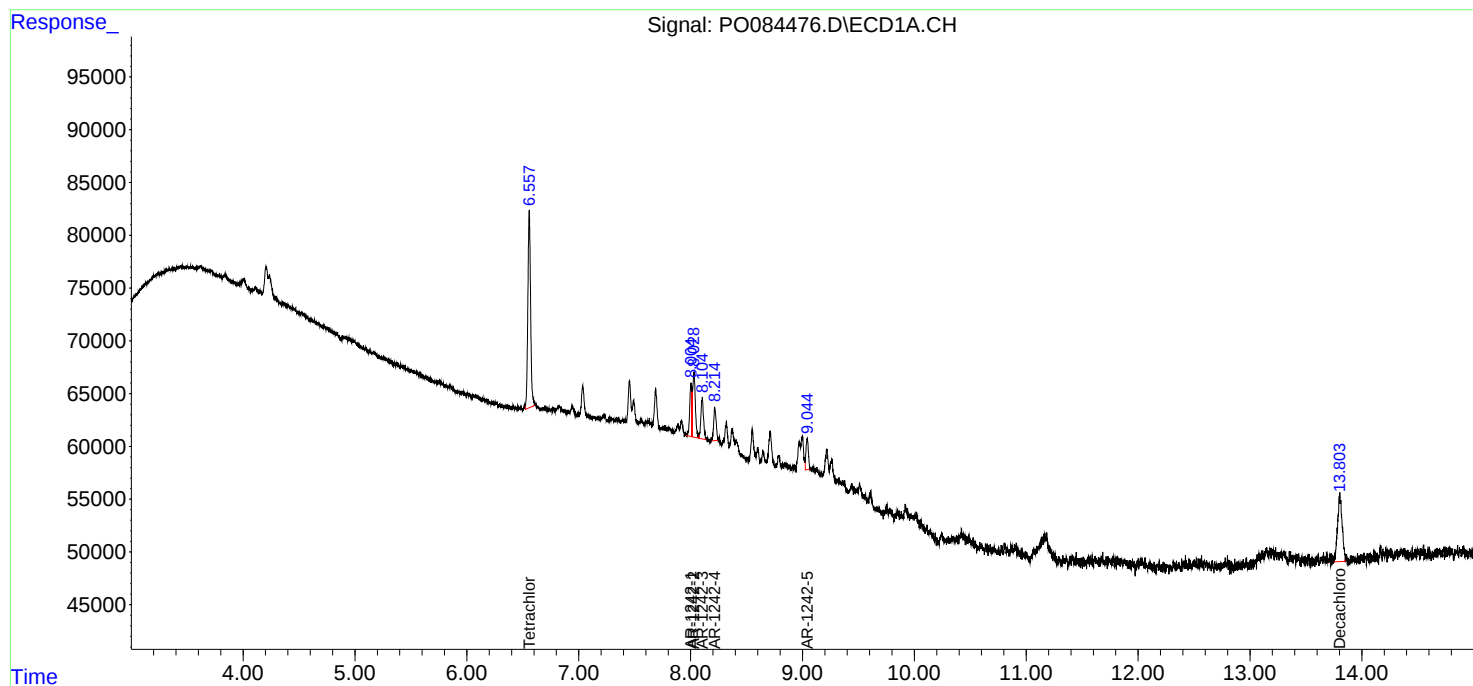

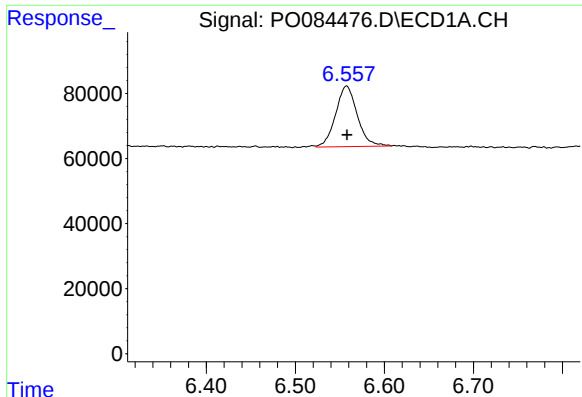


#1 Tetrachloro-m-xylene

R.T.: 6.558 min
Delta R.T.: 0.000 min
Response: 314615
Conc: 5.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

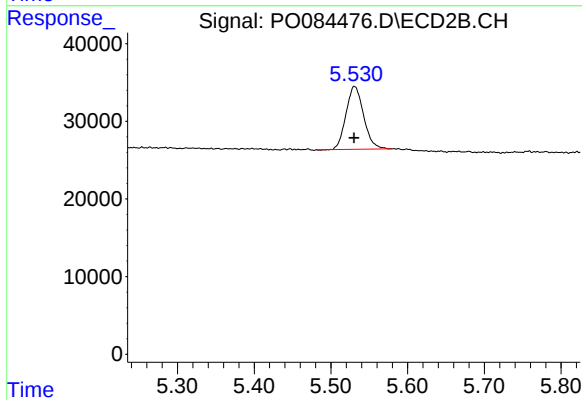


#1 Tetrachloro-m-xylene

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 130466
Conc: 5.24 ng/ml

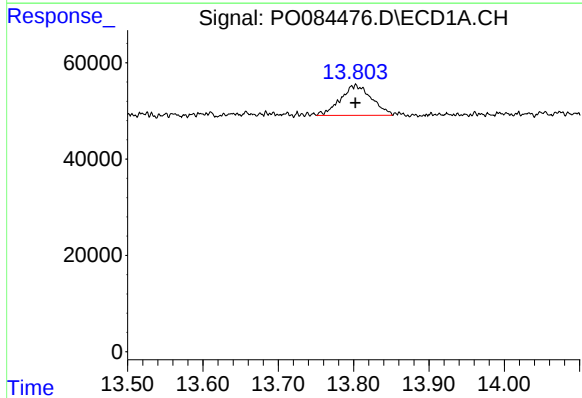


#2 Decachlorobiphenyl

R.T.: 13.803 min
Delta R.T.: 0.000 min
Response: 179108
Conc: 5.21 ng/ml m

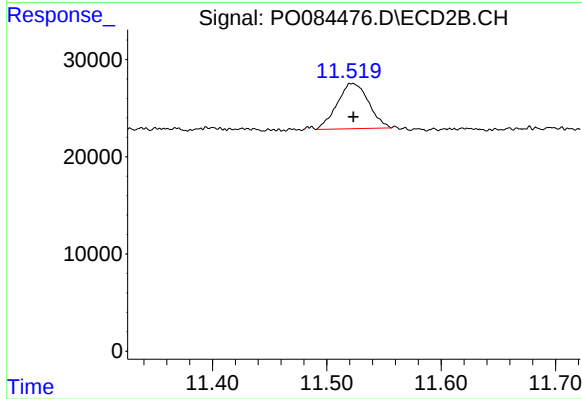

#2 Decachlorobiphenyl

R.T.: 11.523 min
Delta R.T.: 0.000 min
Response: 89181
Conc: 5.01 ng/ml

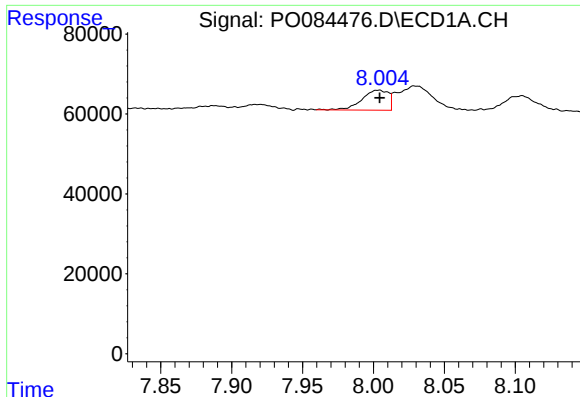


#16 AR-1242-1

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 65590
Conc: 50.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

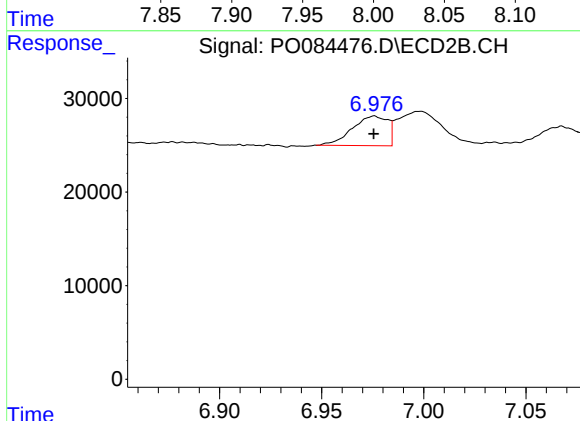


#16 AR-1242-1

R.T.: 6.976 min
Delta R.T.: 0.000 min
Response: 38926
Conc: 58.28 ng/ml m

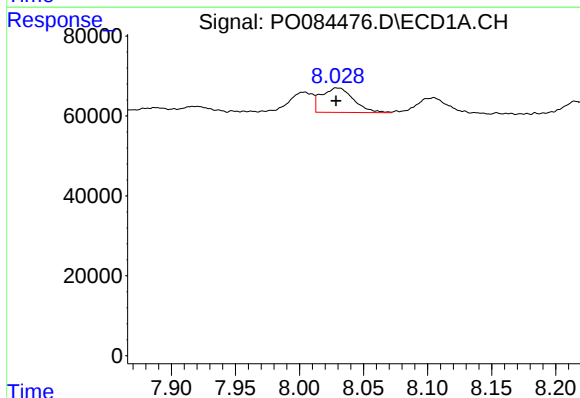


#17 AR-1242-2

R.T.: 8.028 min
Delta R.T.: 0.000 min
Response: 107421
Conc: 52.38 ng/ml

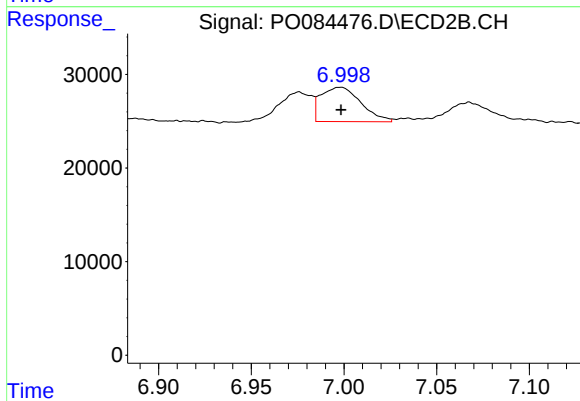

#17 AR-1242-2

R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 54422
Conc: 55.23 ng/ml m

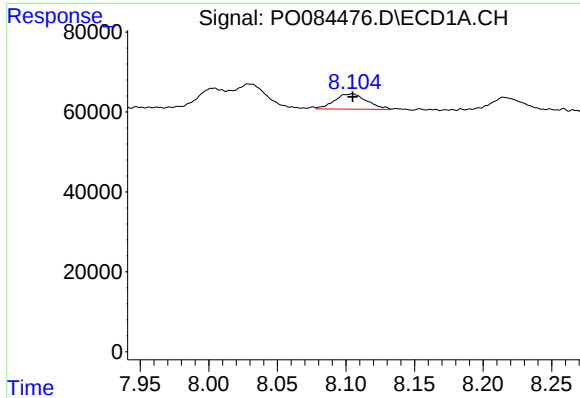


#18 AR-1242-3

R.T.: 8.105 min
Delta R.T.: 0.000 min
Response: 62634
Conc: 49.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

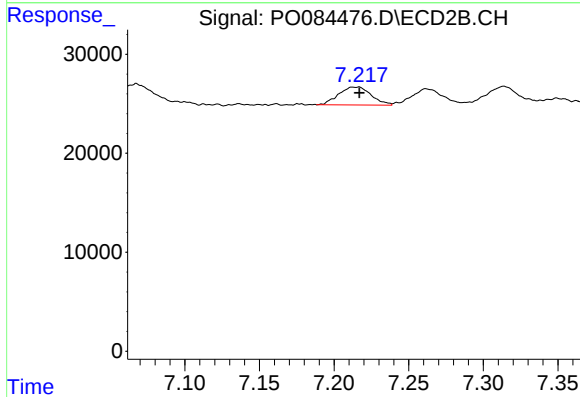


#18 AR-1242-3

R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 27600
Conc: 53.39 ng/ml m

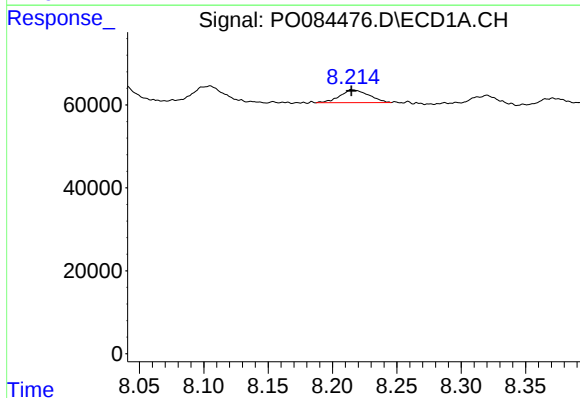


#19 AR-1242-4

R.T.: 8.215 min
Delta R.T.: 0.000 min
Response: 48383
Conc: 46.79 ng/ml

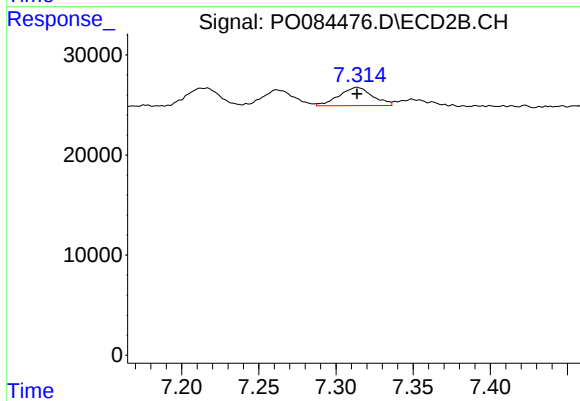

#19 AR-1242-4

R.T.: 7.314 min
Delta R.T.: 0.000 min
Response: 27852
Conc: 51.43 ng/ml m

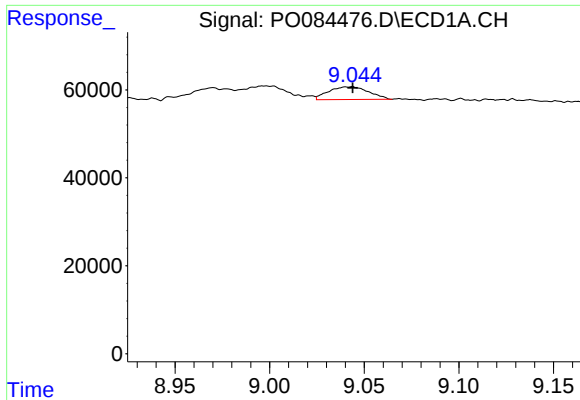


#20 AR-1242-5

R.T.: 9.044 min
Delta R.T.: 0.000 min
Response: 42807
Conc: 44.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

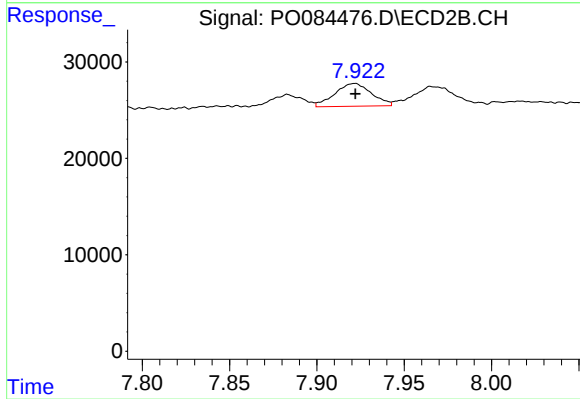

#20 AR-1242-5

R.T.: 7.922 min
Delta R.T.: 0.000 min
Response: 34563
Conc: 55.83 ng/ml