

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020322\
 Data File : P0084483.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Feb 2022 16:41
 Operator : AJ\MA
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/04/2022
 Supervised By :Ankita Jodhani 02/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:40:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0020322.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 04 03:40:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	6.569	5.546	4227764	1835094	75.951	76.027
2)	SA Decachlor...	13.813	11.532	2611641	1286016	76.646	74.236
Target Compounds							
26)	L6 AR-1254-1	8.980	7.932	1401068	966858	753.984m	766.974
27)	L6 AR-1254-2	9.216	8.097	2068157	823426	764.632	765.633
28)	L6 AR-1254-3	9.615	8.545	2126189	1272962	772.674	763.706
29)	L6 AR-1254-4	9.931	8.789	1473870	888859	765.751	772.619
30)	L6 AR-1254-5	10.431	9.236	1841203	1064718	758.965	774.523

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020322\
Data File : PO084483.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Feb 2022 16:41
Operator : AJ\MA
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:40:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO020322.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 04 03:40:46 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

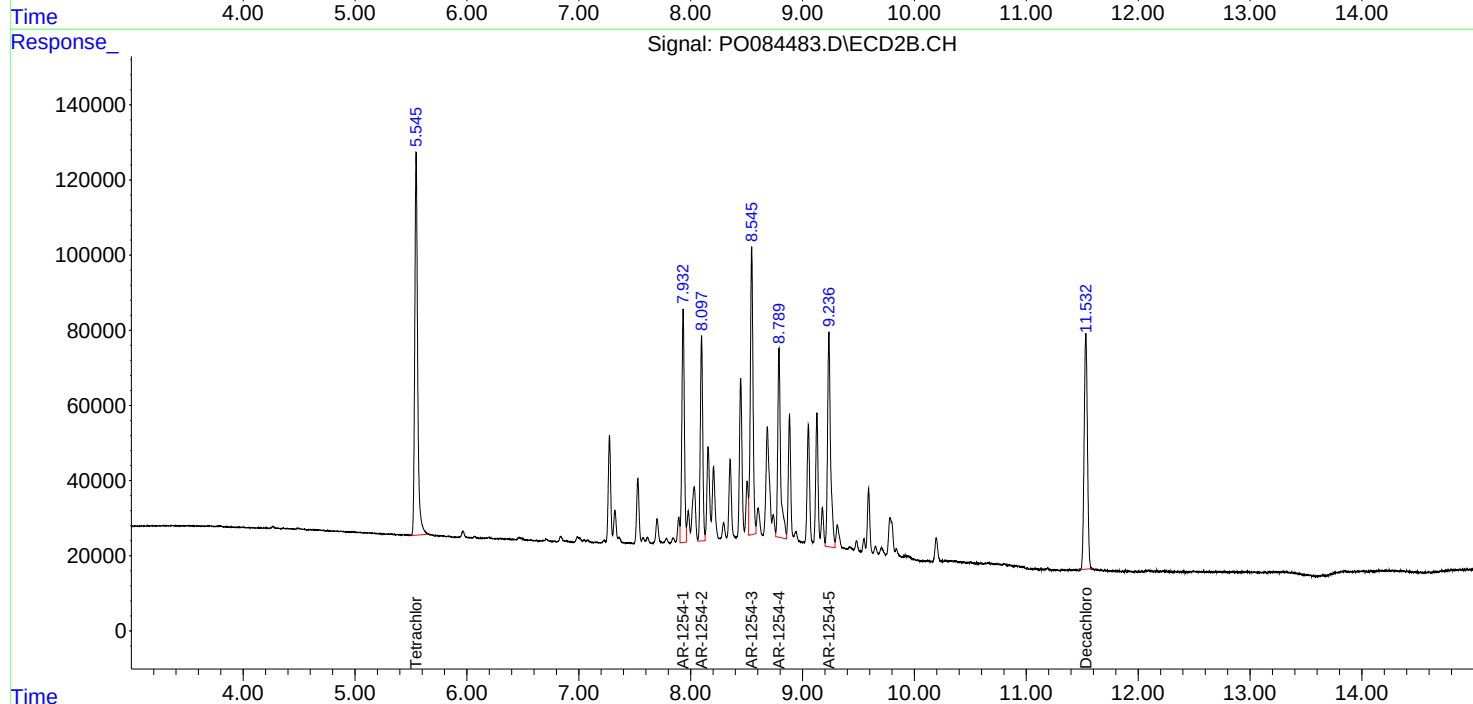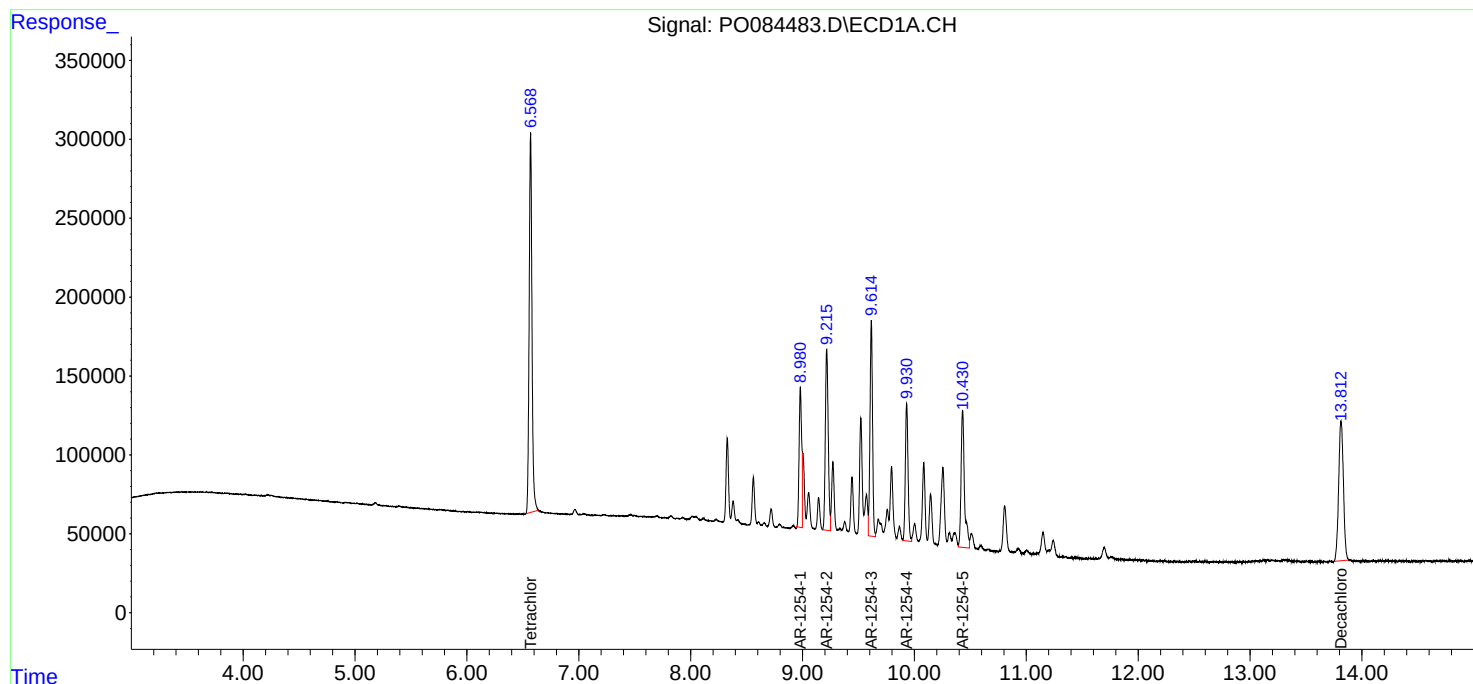

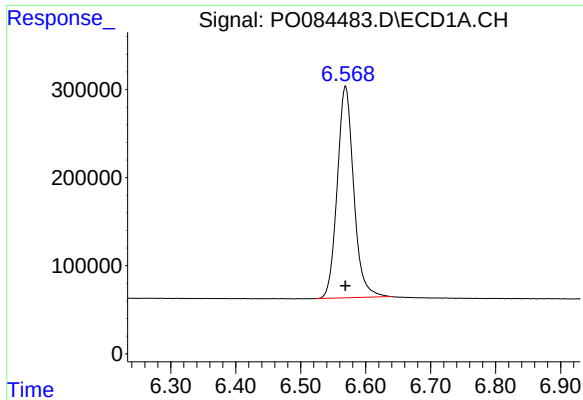


#1 Tetrachloro-m-xylene

R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 4227764
Conc: 75.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

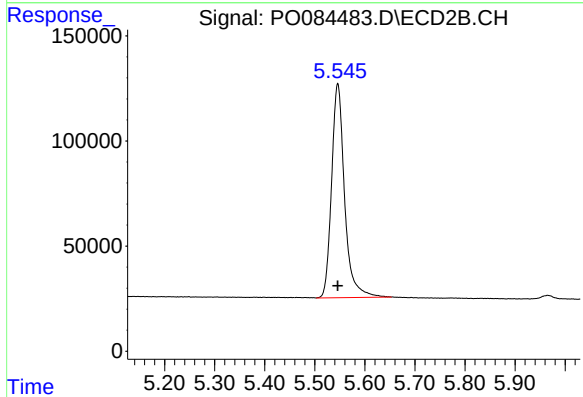


#1 Tetrachloro-m-xylene

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 1835094
Conc: 76.03 ng/ml

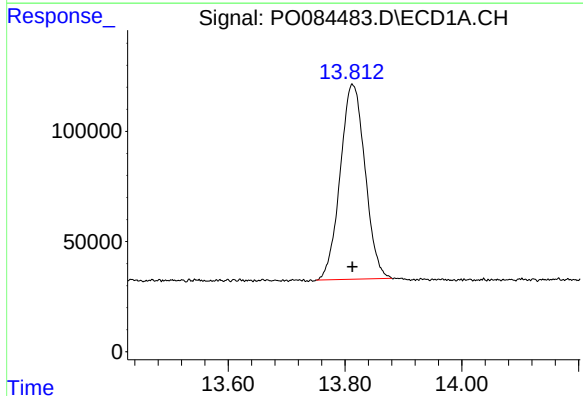


#2 Decachlorobiphenyl

R.T.: 13.813 min
Delta R.T.: 0.000 min
Response: 2611641
Conc: 76.65 ng/ml

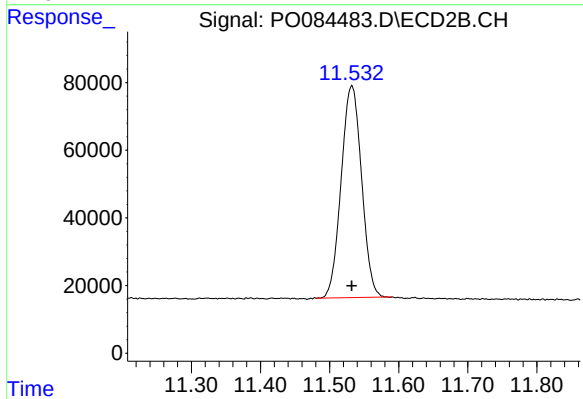

#2 Decachlorobiphenyl

R.T.: 11.532 min
Delta R.T.: 0.000 min
Response: 1286016
Conc: 74.24 ng/ml

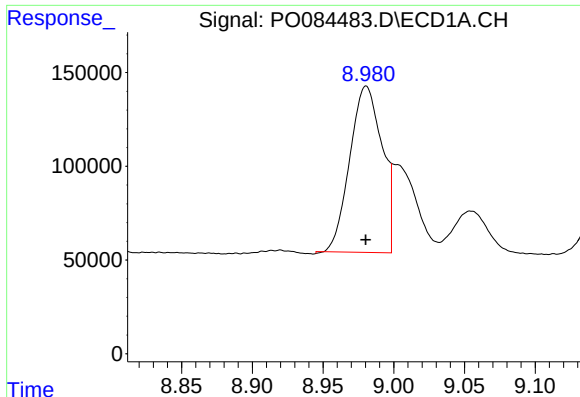


#26 AR-1254-1

R.T.: 8.980 min
Delta R.T.: 0.000 min
Response: 1401068
Conc: 753.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

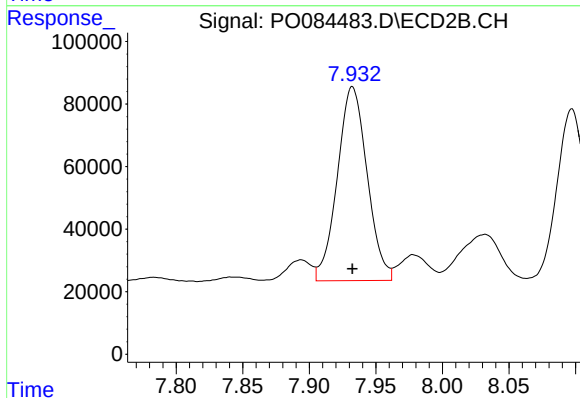


#26 AR-1254-1

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 966858
Conc: 766.97 ng/ml

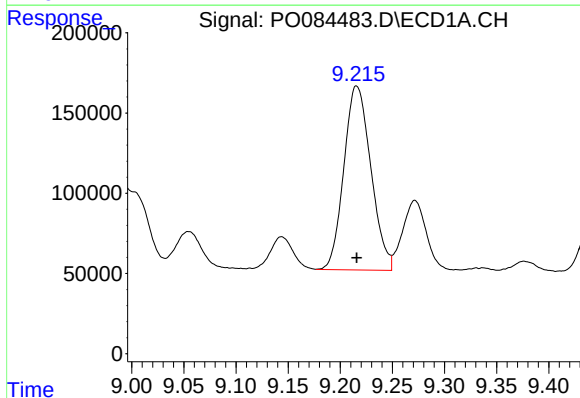


#27 AR-1254-2

R.T.: 9.216 min
Delta R.T.: 0.000 min
Response: 2068157
Conc: 764.63 ng/ml

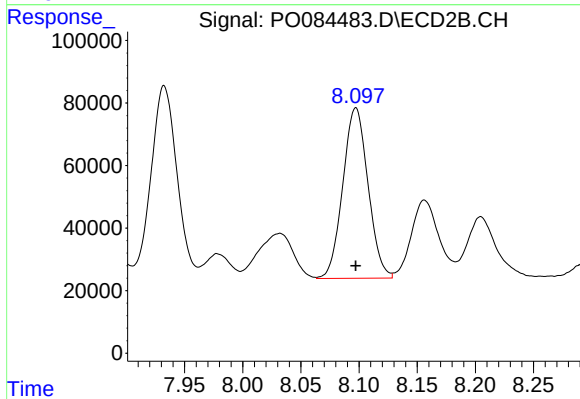

#27 AR-1254-2

R.T.: 8.097 min
Delta R.T.: 0.000 min
Response: 823426
Conc: 765.63 ng/ml

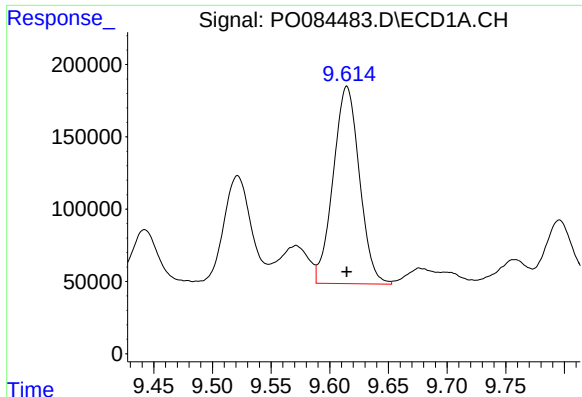


#28 AR-1254-3

R.T.: 9.615 min
Delta R.T.: 0.000 min
Response: 2126189
Conc: 772.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

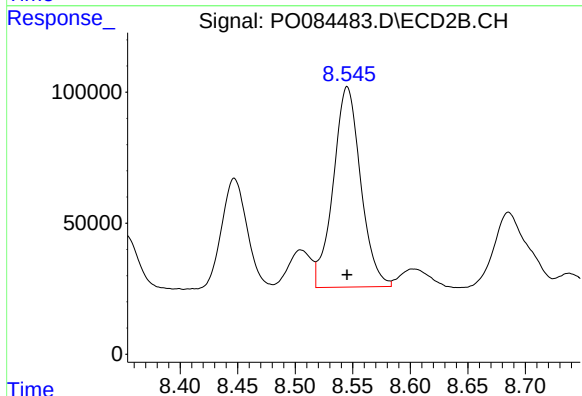


#28 AR-1254-3

R.T.: 8.545 min
Delta R.T.: 0.000 min
Response: 1272962
Conc: 763.71 ng/ml

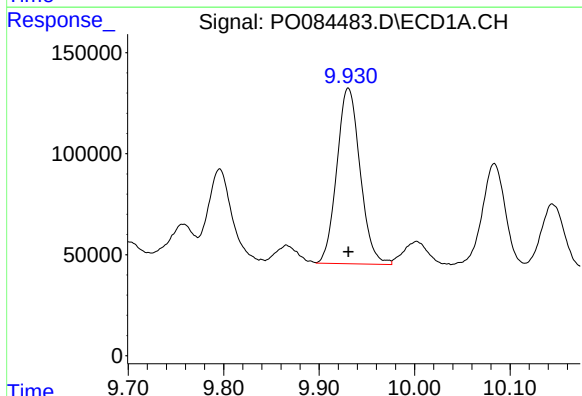


#29 AR-1254-4

R.T.: 9.931 min
Delta R.T.: 0.000 min
Response: 1473870
Conc: 765.75 ng/ml

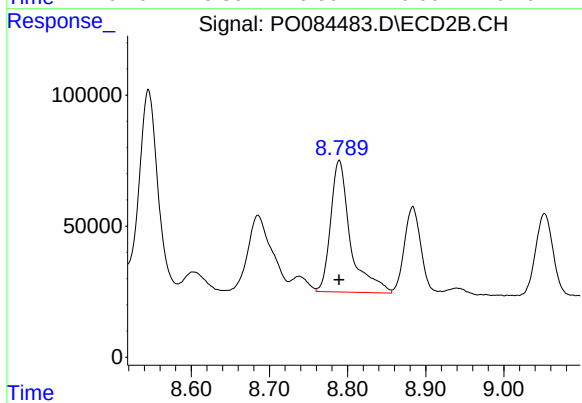

#29 AR-1254-4

R.T.: 8.789 min
Delta R.T.: 0.000 min
Response: 888859
Conc: 772.62 ng/ml

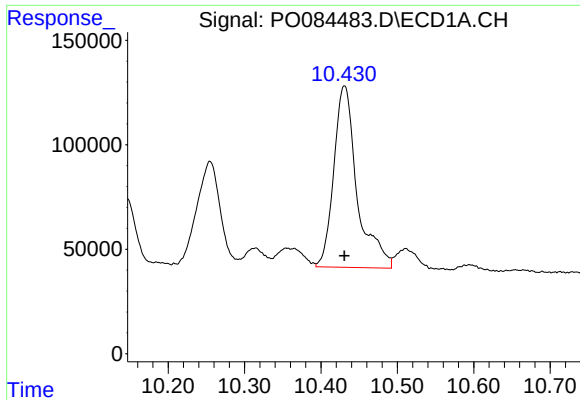


#30 AR-1254-5

R.T.: 10.431 min
Delta R.T.: 0.000 min
Response: 1841203
Conc: 758.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/04/2022
Supervised By :Ankita Jodhani 02/04/2022

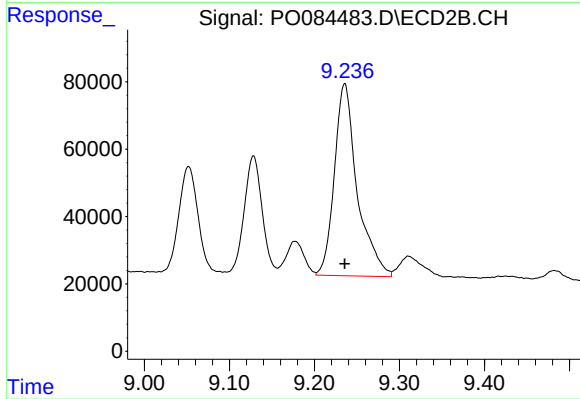

#30 AR-1254-5

R.T.: 9.236 min
Delta R.T.: 0.000 min
Response: 1064718
Conc: 774.52 ng/ml