

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020420\
 Data File : P0066241.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2020 15:35
 Operator : DD\AJ
 Sample : L1380-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M030-13C

Manual Integrations
 APPROVED

mohammad
 2/6/2020 12:45:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 05:53:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.430	916460	1227829	31.460	30.017
2) SA Decachlor...	9.647	8.327	678795	1200883	17.225m	20.489

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020420\
Data File : PO066241.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2020 15:35
Operator : DD\AJ
Sample : L1380-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
M030-13C


Manual Integrations
APPROVED

mohammad
2/6/2020 12:45:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 05:53:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

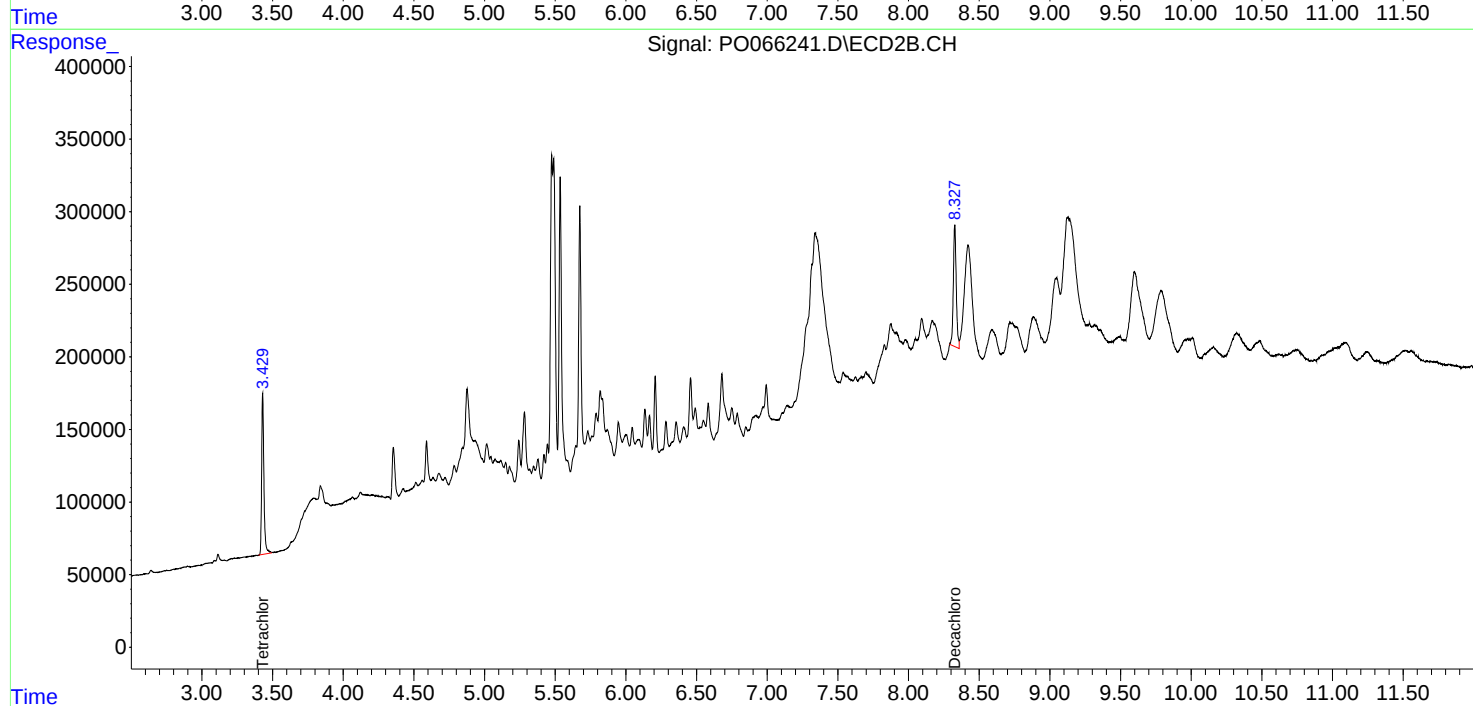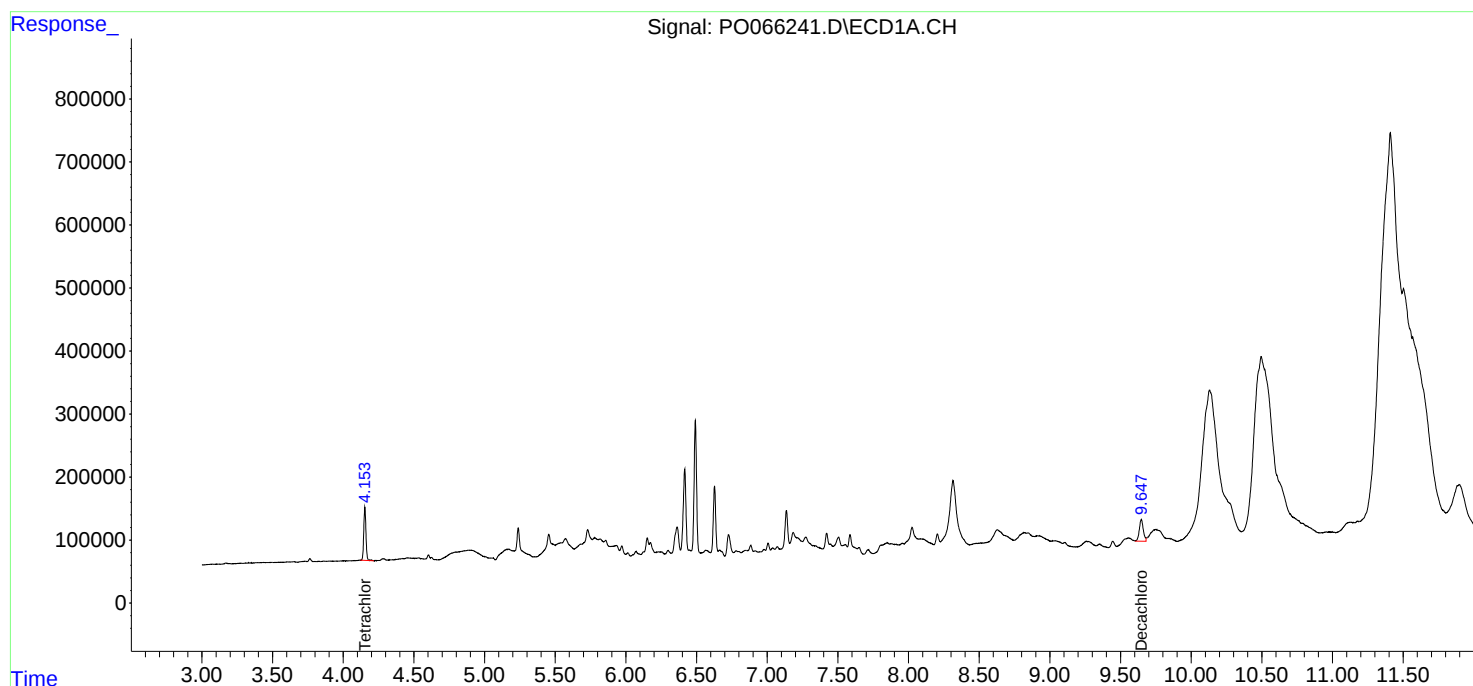

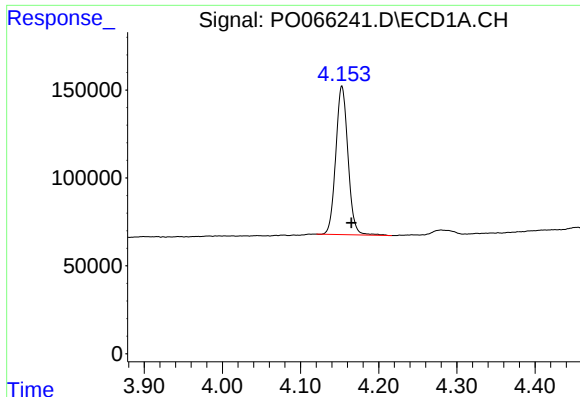


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: -0.012 min
Response: 916460
Conc: 31.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-13C


Manual Integrations
APPROVED

mohammad
2/6/2020 12:45:00 PM

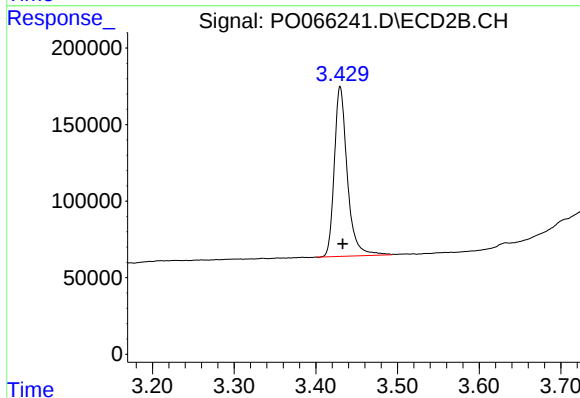


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 1227829
Conc: 30.02 ng/ml

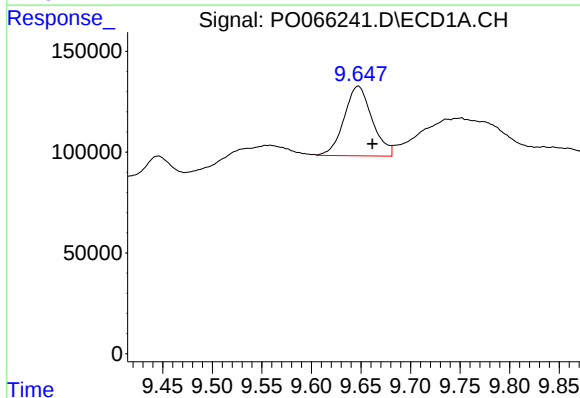

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.014 min
Response: 678795
Conc: 17.22 ng/ml m

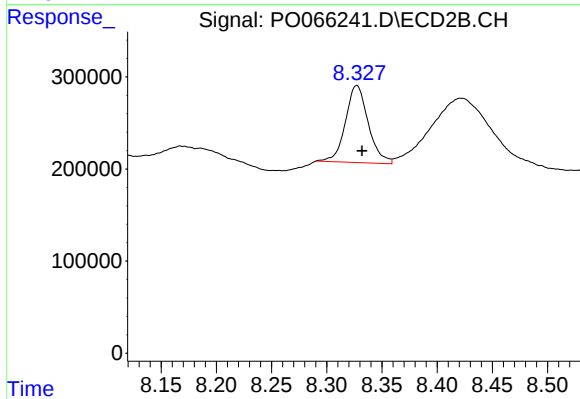

#2 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.005 min
Response: 1200883
Conc: 20.49 ng/ml