

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
 Data File : P0075511.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 14:15
 Operator : AJ/MA
 Sample : M1291-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-007-0510

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:40:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:06:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.996	2154196	1154705	21.286	24.021
2) SA Decachlor...	10.938	9.244	1993075	921995	20.657	18.994
Target Compounds						
36) L8 AR-1262-1	8.574	7.339	210737	24210	24.149m	11.099m#
37) L8 AR-1262-2	9.130	7.889	315285	150056	20.849m	19.567m
38) L8 AR-1262-3	9.441	8.173	526158	181005	50.365	54.695
39) L8 AR-1262-4	9.536	8.238	474812	211914	64.241	36.907 #
40) L8 AR-1262-5	10.199	8.731	219355	121434	42.298	44.144m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020421\
Data File : PO075511.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 14:15
Operator : AJ/MA
Sample : M1291-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
OU421-007-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:40:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:06:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

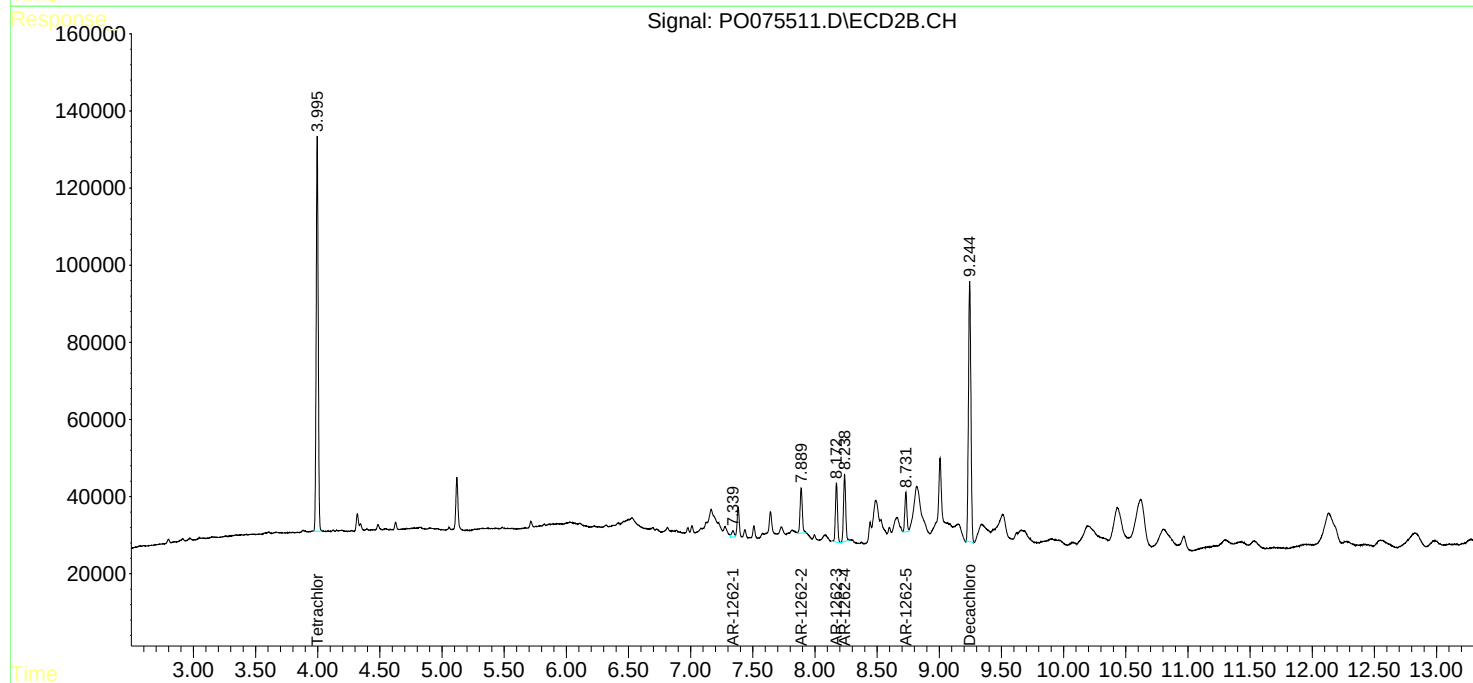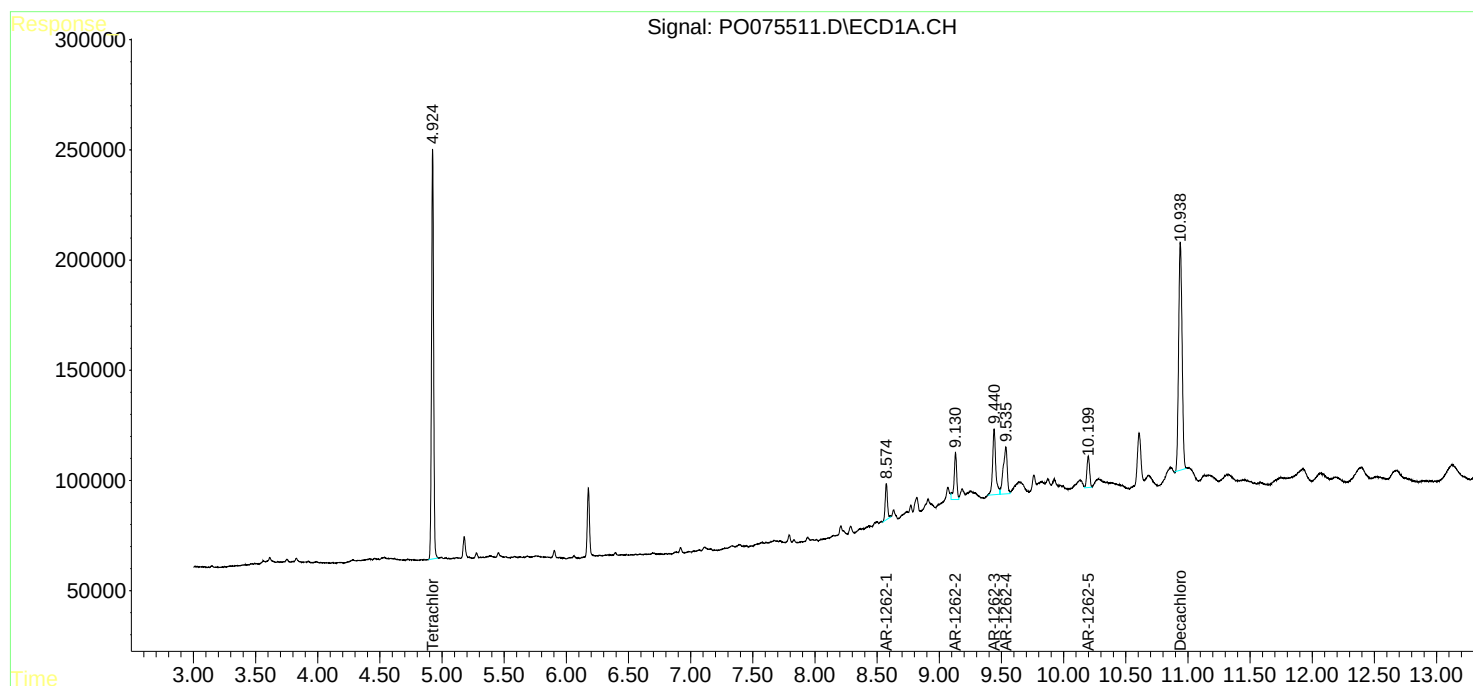

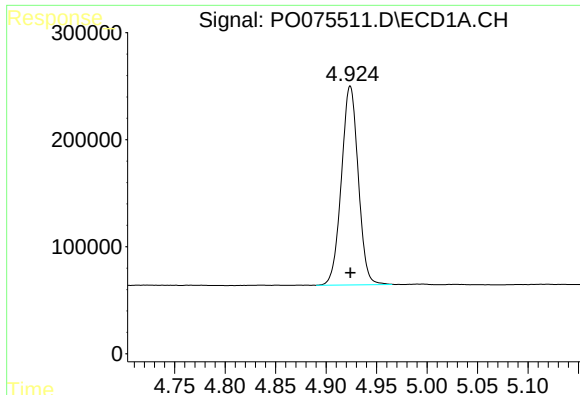


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 2154196
Conc: 21.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-007-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:40:44 AM

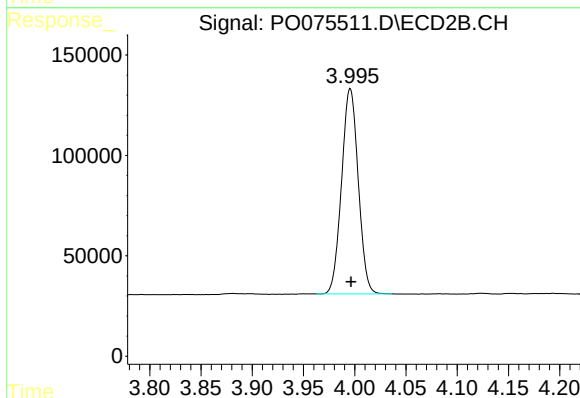


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: 0.000 min
Response: 1154705
Conc: 24.02 ng/ml

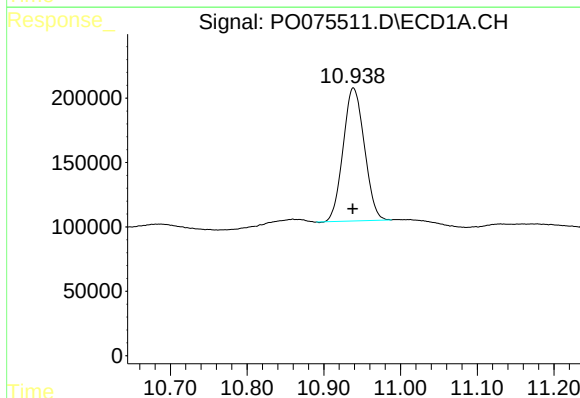


#2 Decachlorobiphenyl

R.T.: 10.938 min
Delta R.T.: 0.000 min
Response: 1993075
Conc: 20.66 ng/ml

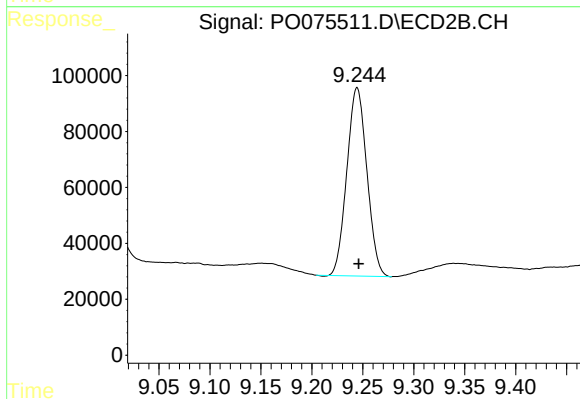

#2 Decachlorobiphenyl

R.T.: 9.244 min
Delta R.T.: -0.002 min
Response: 921995
Conc: 18.99 ng/ml

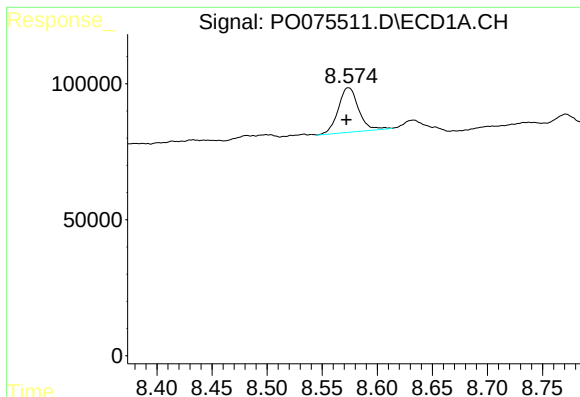


#36 AR-1262-1

R.T.: 8.574 min
Delta R.T.: 0.002 min
Response: 210737
Conc: 24.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-007-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:40:44 AM

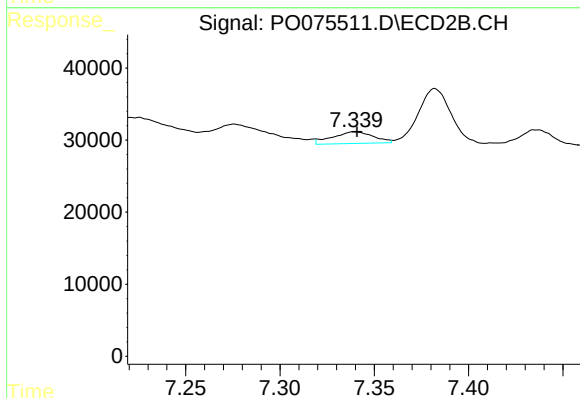


#36 AR-1262-1

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 24210
Conc: 11.10 ng/ml m

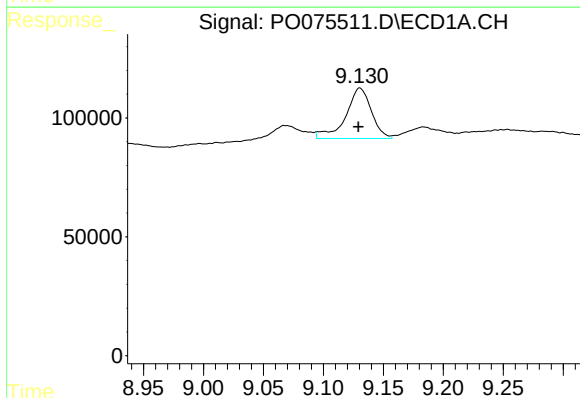


#37 AR-1262-2

R.T.: 9.130 min
Delta R.T.: 0.000 min
Response: 315285
Conc: 20.85 ng/ml m

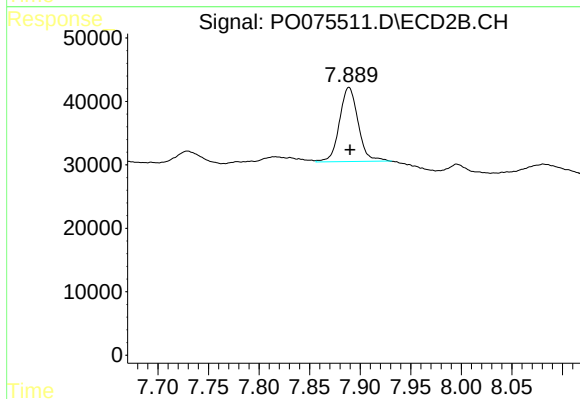

#37 AR-1262-2

R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 150056
Conc: 19.57 ng/ml m

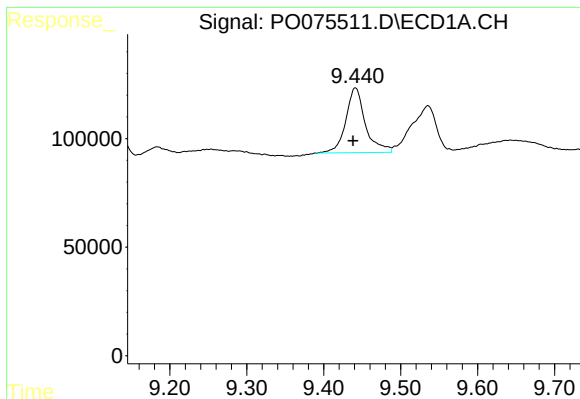


#38 AR-1262-3

R.T.: 9.441 min
Delta R.T.: 0.003 min
Response: 526158
Conc: 50.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-007-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:40:44 AM

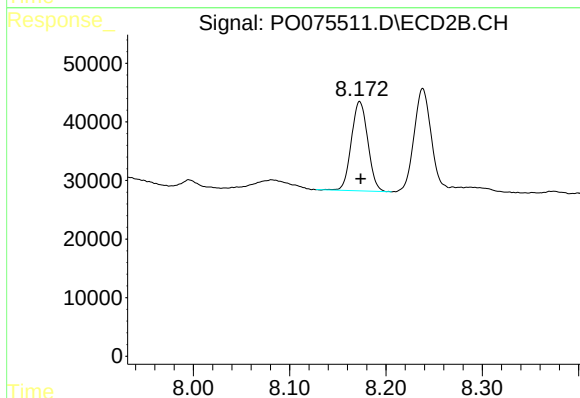


#38 AR-1262-3

R.T.: 8.173 min
Delta R.T.: 0.000 min
Response: 181005
Conc: 54.70 ng/ml

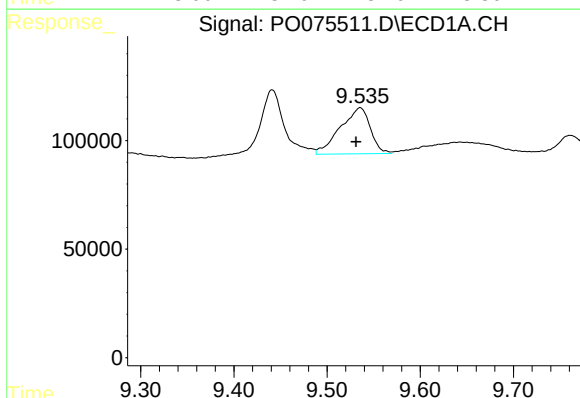


#39 AR-1262-4

R.T.: 9.536 min
Delta R.T.: 0.004 min
Response: 474812
Conc: 64.24 ng/ml

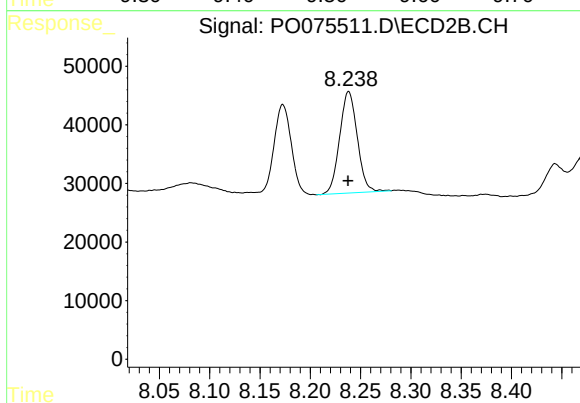

#39 AR-1262-4

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 211914
Conc: 36.91 ng/ml

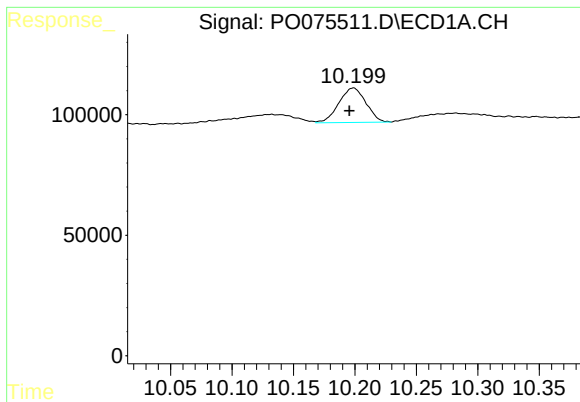


#40 AR-1262-5

R.T.: 10.199 min
Delta R.T.: 0.003 min
Response: 219355
Conc: 42.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-007-0510

Manual Integrations
APPROVED

Ankita
2/8/2021 8:40:44 AM

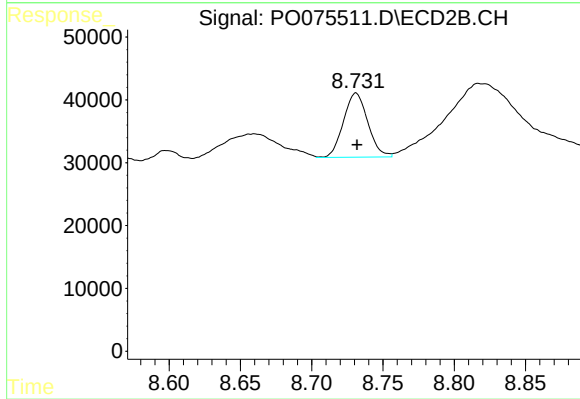

#40 AR-1262-5

R.T.: 8.731 min
Delta R.T.: -0.001 min
Response: 121434
Conc: 44.14 ng/ml m