

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
Data File : P0075517.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 15:57
Operator : AJ/MA
Sample : M1291-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2021-01-27-FD03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:09:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.994	2329104	1156315	23.014	24.054
2) SA Decachlor...	10.936	9.243	2184493	1058269	22.641	21.801

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
Data File : P0075517.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 15:57
Operator : AJ/MA
Sample : M1291-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2021-01-27-FD03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:09:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

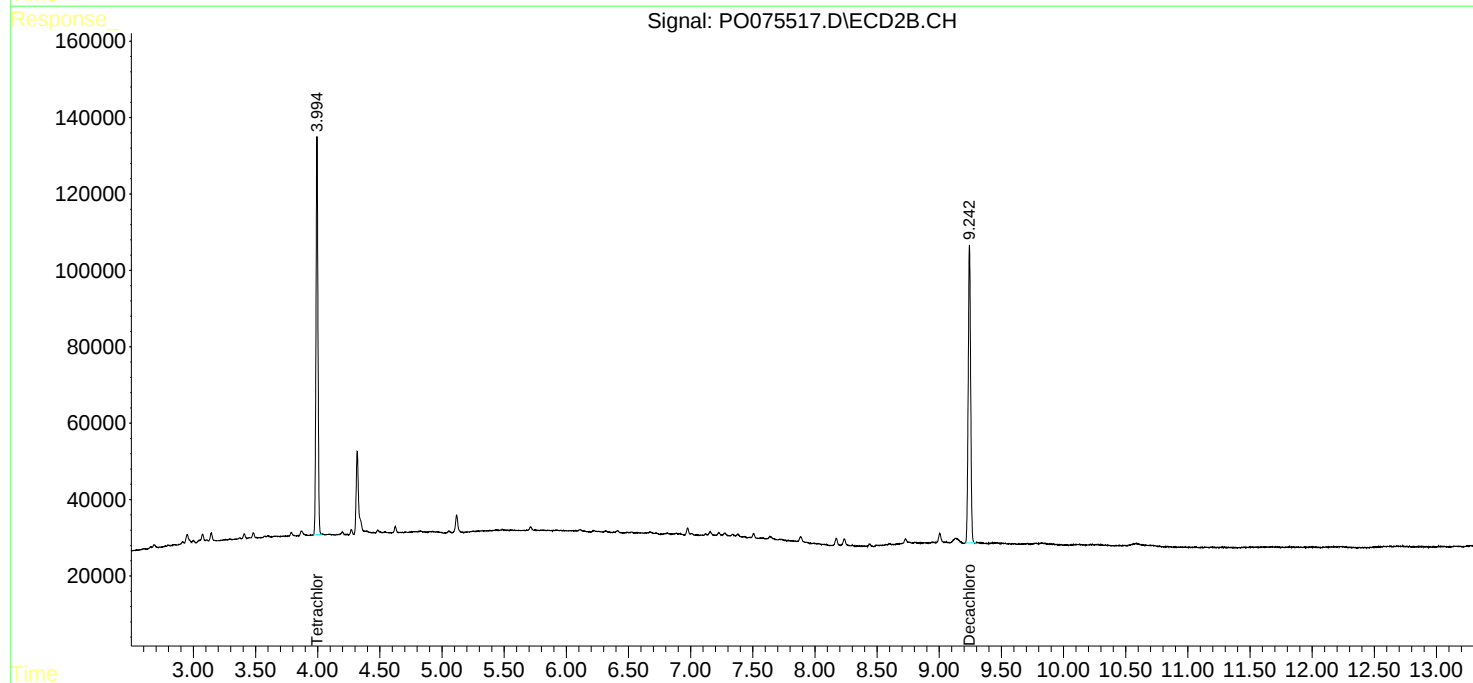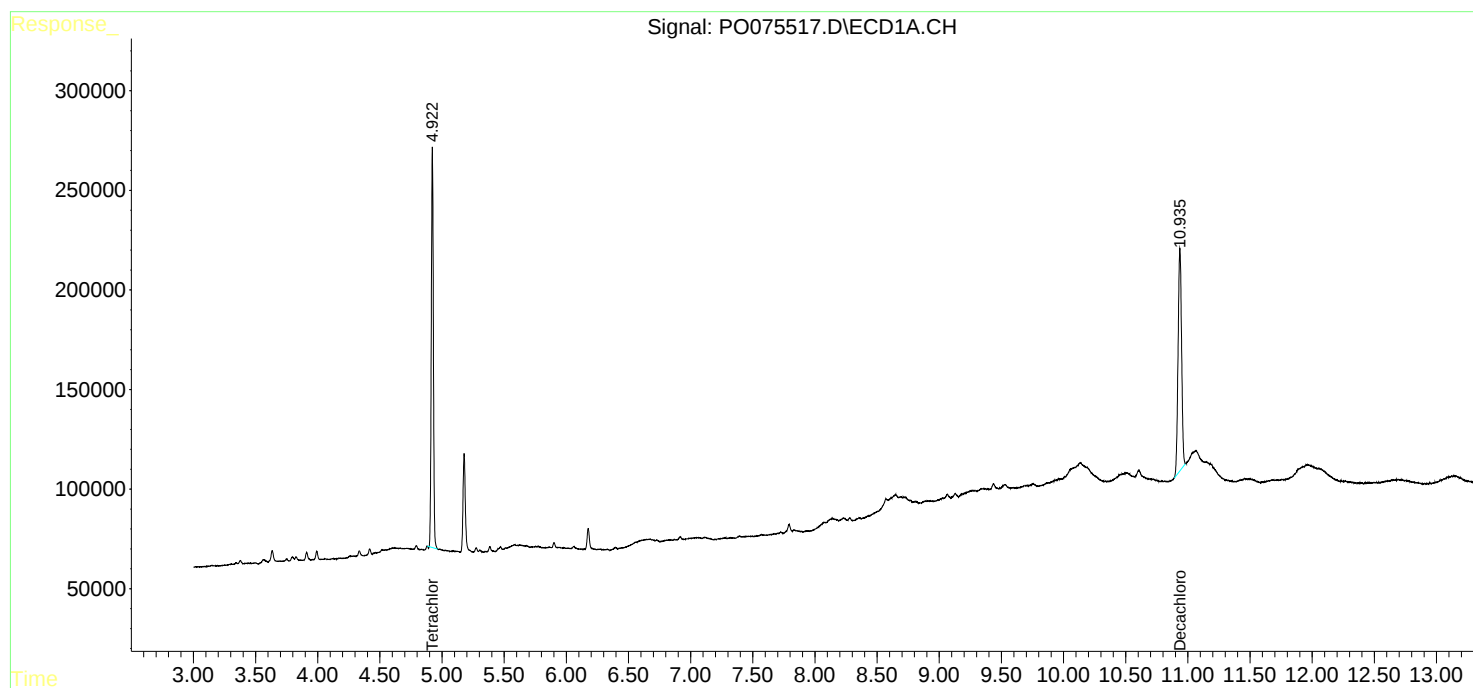


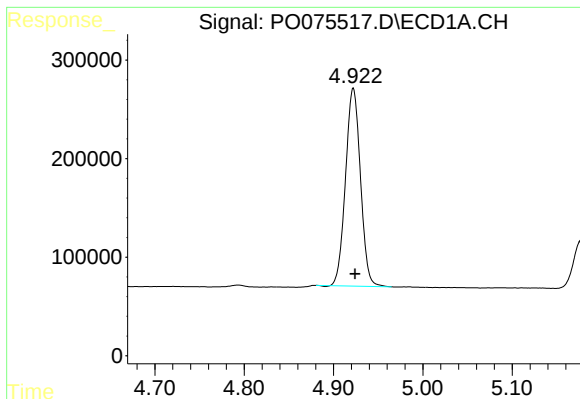

#1 Tetrachloro-m-xylene


R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 2329104
Conc: 23.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
2021-01-27-FD03

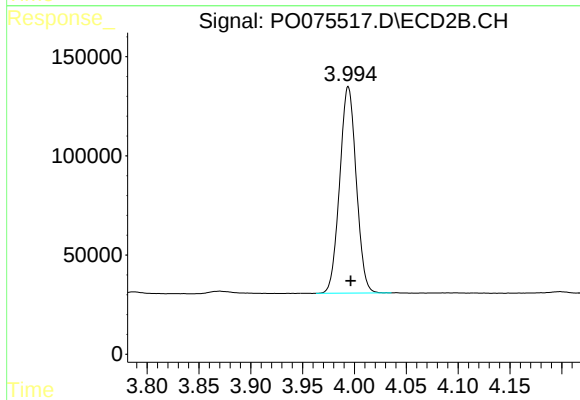


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1156315
Conc: 24.05 ng/ml

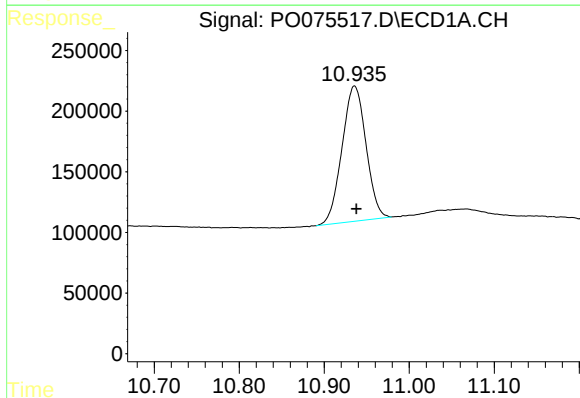

#2 Decachlorobiphenyl

R.T.: 10.936 min
Delta R.T.: -0.002 min
Response: 2184493
Conc: 22.64 ng/ml

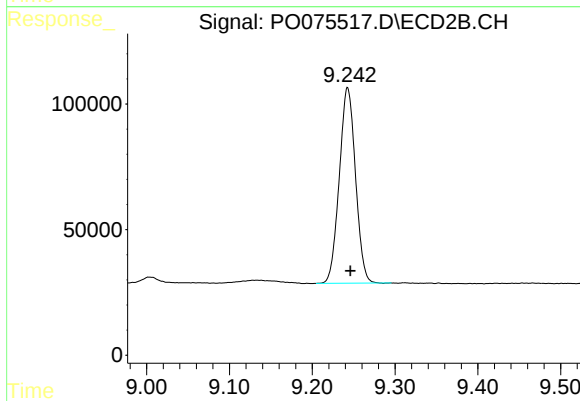

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 1058269
Conc: 21.80 ng/ml