

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
 Data File : P0075529.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 19:40
 Operator : AJ/MA
 Sample : M1291-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-004-0205

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:41:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:14:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.994	1997776	979963	19.740	20.386
2) SA Decachlor...	10.934	9.241	2010264	989433	20.836	20.383
Target Compounds						
36) L8 AR-1262-1	8.570	7.337	478776	11618	54.865m	5.326m#
37) L8 AR-1262-2	9.127	7.886	296901	180137	19.634m	23.489
38) L8 AR-1262-3	9.436	8.169	565232	294824	54.106	89.089m#
39) L8 AR-1262-4	9.532	8.235	584270	312883	79.050	54.492 #
40) L8 AR-1262-5	10.193	8.728	353403	182506	68.147	66.345

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020421\
Data File : PO075529.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 19:40
Operator : AJ/MA
Sample : M1291-17
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
OU421-004-0205


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:14:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

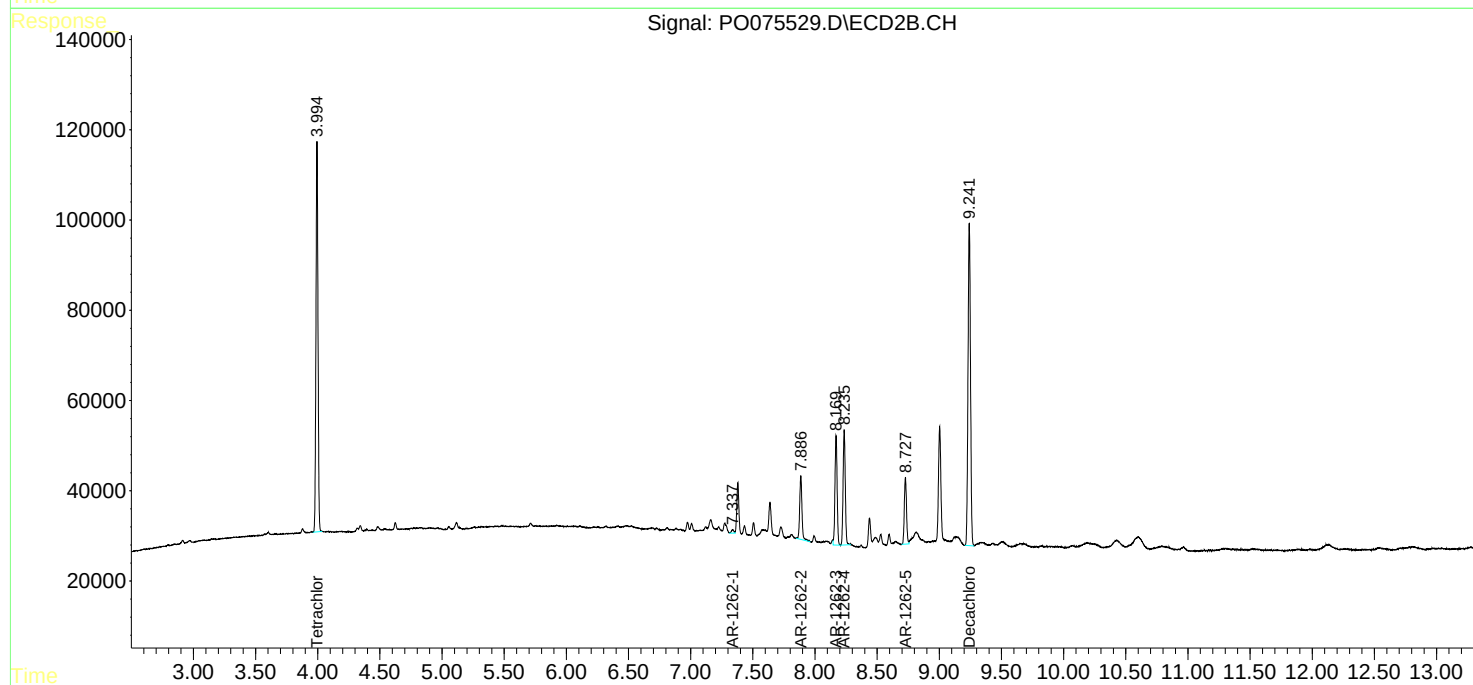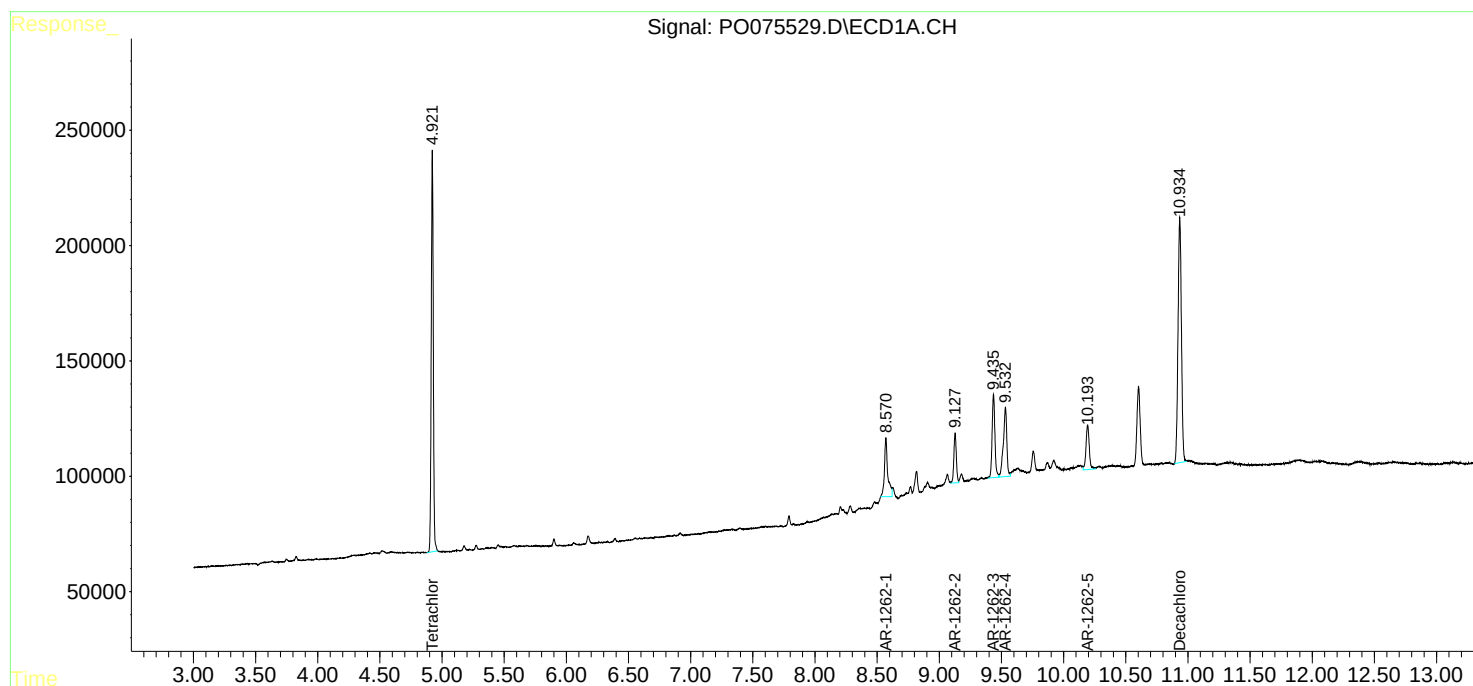

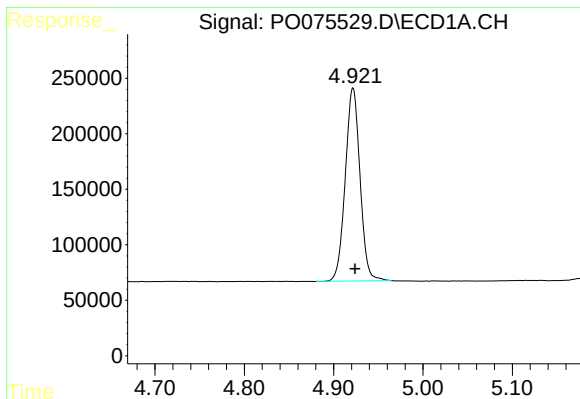


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 1997776
Conc: 19.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0205


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:27 AM

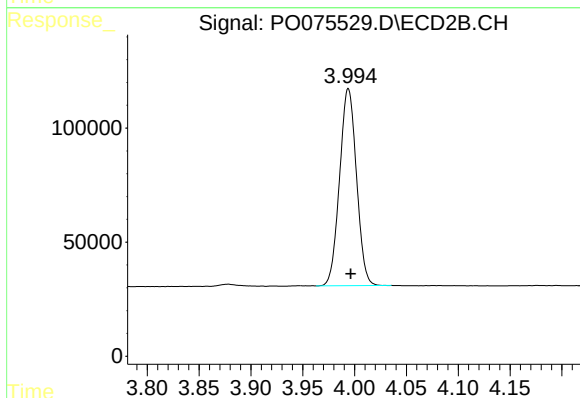


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 979963
Conc: 20.39 ng/ml

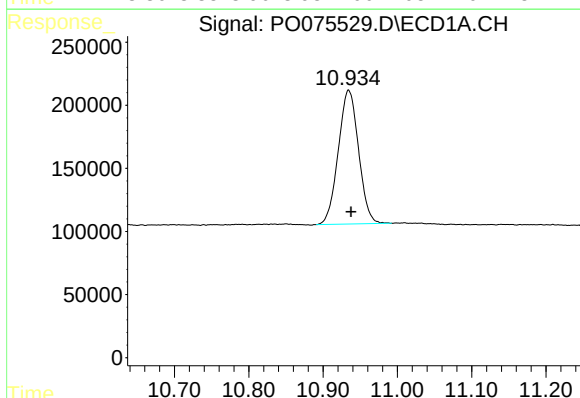


#2 Decachlorobiphenyl

R.T.: 10.934 min
Delta R.T.: -0.003 min
Response: 2010264
Conc: 20.84 ng/ml

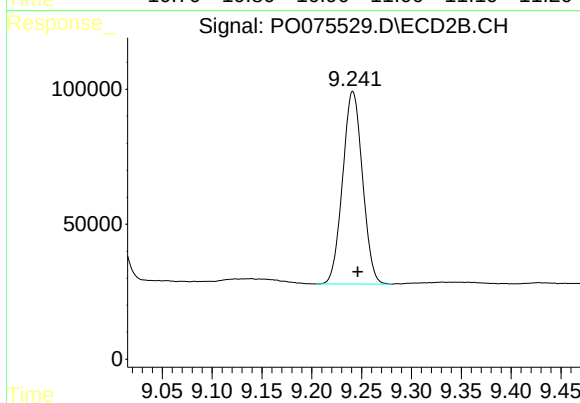

#2 Decachlorobiphenyl

R.T.: 9.241 min
Delta R.T.: -0.005 min
Response: 989433
Conc: 20.38 ng/ml

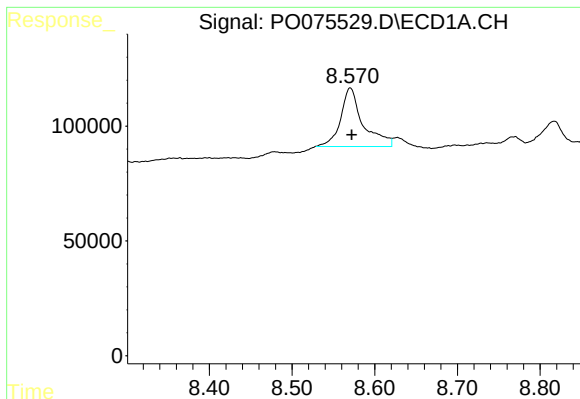


#36 AR-1262-1

R.T.: 8.570 min
Delta R.T.: -0.002 min
Response: 478776
Conc: 54.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OU421-004-0205


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:27 AM

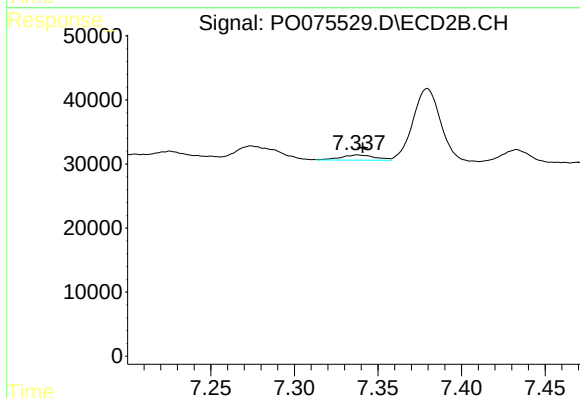


#36 AR-1262-1

R.T.: 7.337 min
Delta R.T.: -0.004 min
Response: 11618
Conc: 5.33 ng/ml m

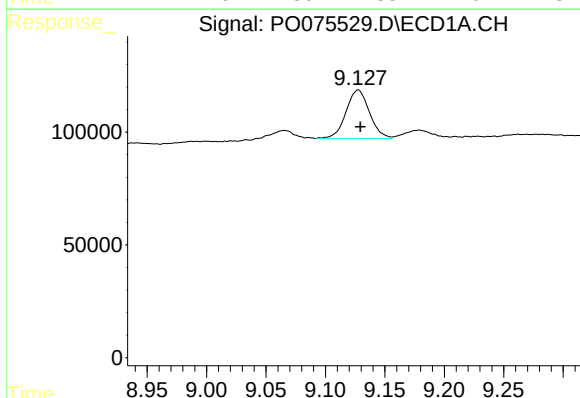


#37 AR-1262-2

R.T.: 9.127 min
Delta R.T.: -0.002 min
Response: 296901
Conc: 19.63 ng/ml m

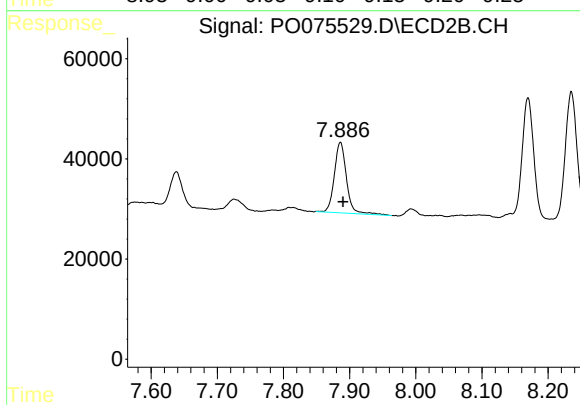

#37 AR-1262-2

R.T.: 7.886 min
Delta R.T.: -0.004 min
Response: 180137
Conc: 23.49 ng/ml

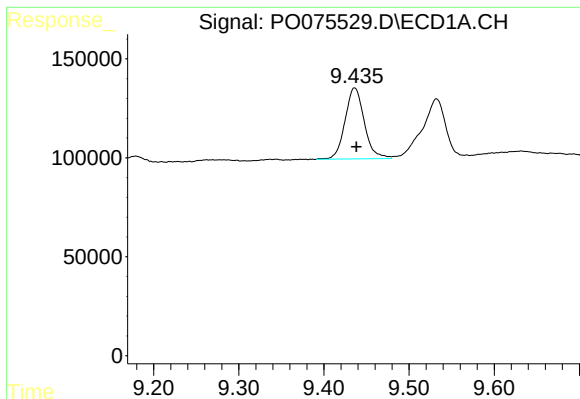


#38 AR-1262-3

R.T.: 9.436 min
Delta R.T.: -0.002 min
Response: 565232
Conc: 54.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0205


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:27 AM

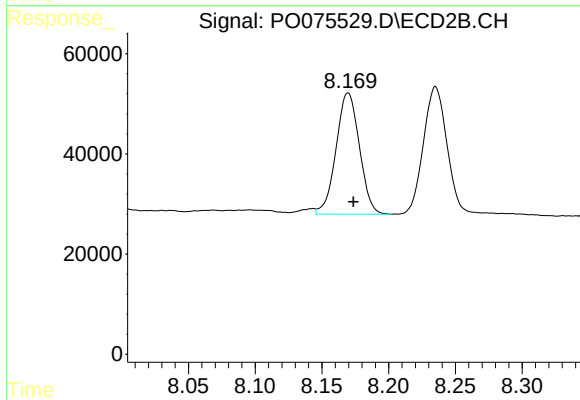


#38 AR-1262-3

R.T.: 8.169 min
Delta R.T.: -0.004 min
Response: 294824
Conc: 89.09 ng/ml m

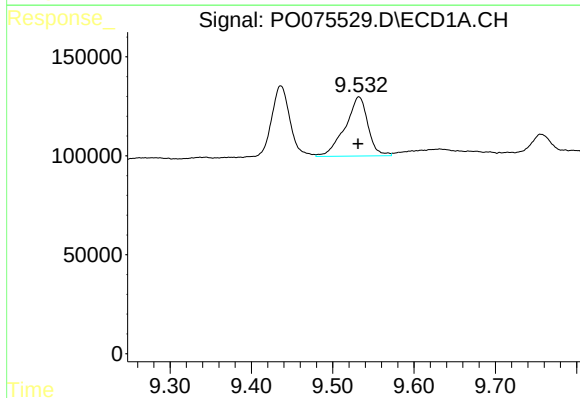


#39 AR-1262-4

R.T.: 9.532 min
Delta R.T.: 0.001 min
Response: 584270
Conc: 79.05 ng/ml

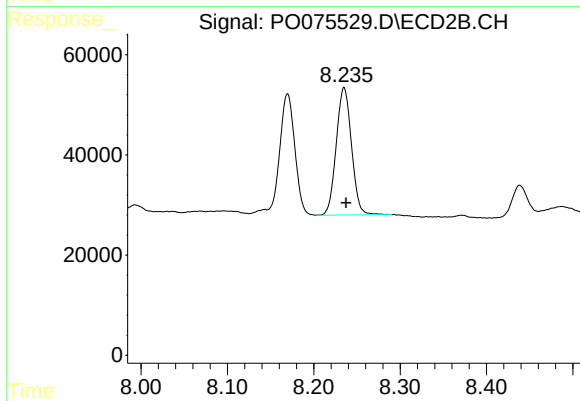

#39 AR-1262-4

R.T.: 8.235 min
Delta R.T.: -0.002 min
Response: 312883
Conc: 54.49 ng/ml

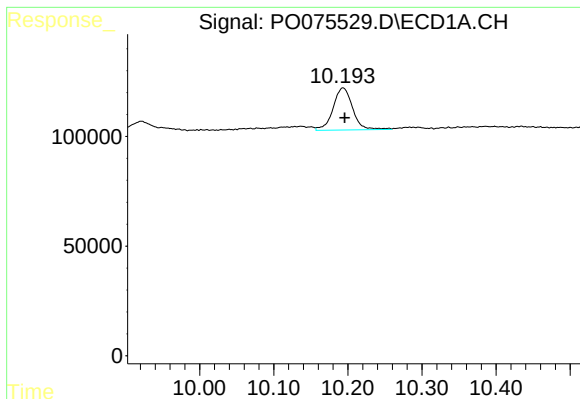


#40 AR-1262-5

R.T.: 10.193 min
Delta R.T.: -0.002 min
Response: 353403
Conc: 68.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0205

Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:27 AM

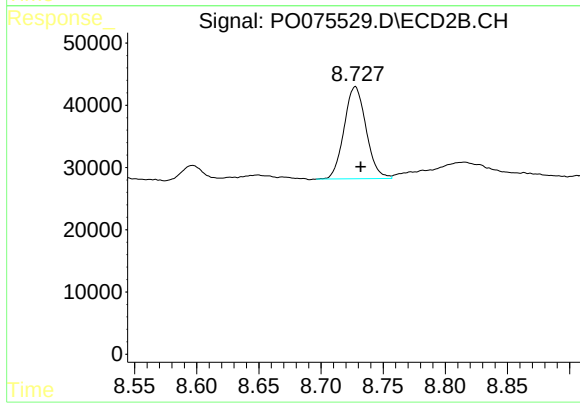

#40 AR-1262-5

R.T.: 8.728 min
Delta R.T.: -0.004 min
Response: 182506
Conc: 66.35 ng/ml