

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
 Data File : P0075530.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2021 19:57
 Operator : AJ/MA
 Sample : M1291-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU421-004-0510

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:41:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:15:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.994	2226956	1096493	22.005	22.810
2) SA Decachlor...	10.936	9.243	2157847	1015956	22.365	20.930
Target Compounds						
36) L8 AR-1262-1	8.572	7.339	211974	45711	24.291	20.957
37) L8 AR-1262-2	9.128	7.886	241101	140435	15.944	18.312
38) L8 AR-1262-3	9.438	8.171	410696	216590	39.313	65.448m#
39) L8 AR-1262-4	9.533	8.237	428656	231800	57.996	40.370 #
40) L8 AR-1262-5	10.195	8.729	299095	136740	57.675	49.708

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020421\
Data File : PO075530.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2021 19:57
Operator : AJ/MA
Sample : M1291-18
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OU421-004-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:15:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

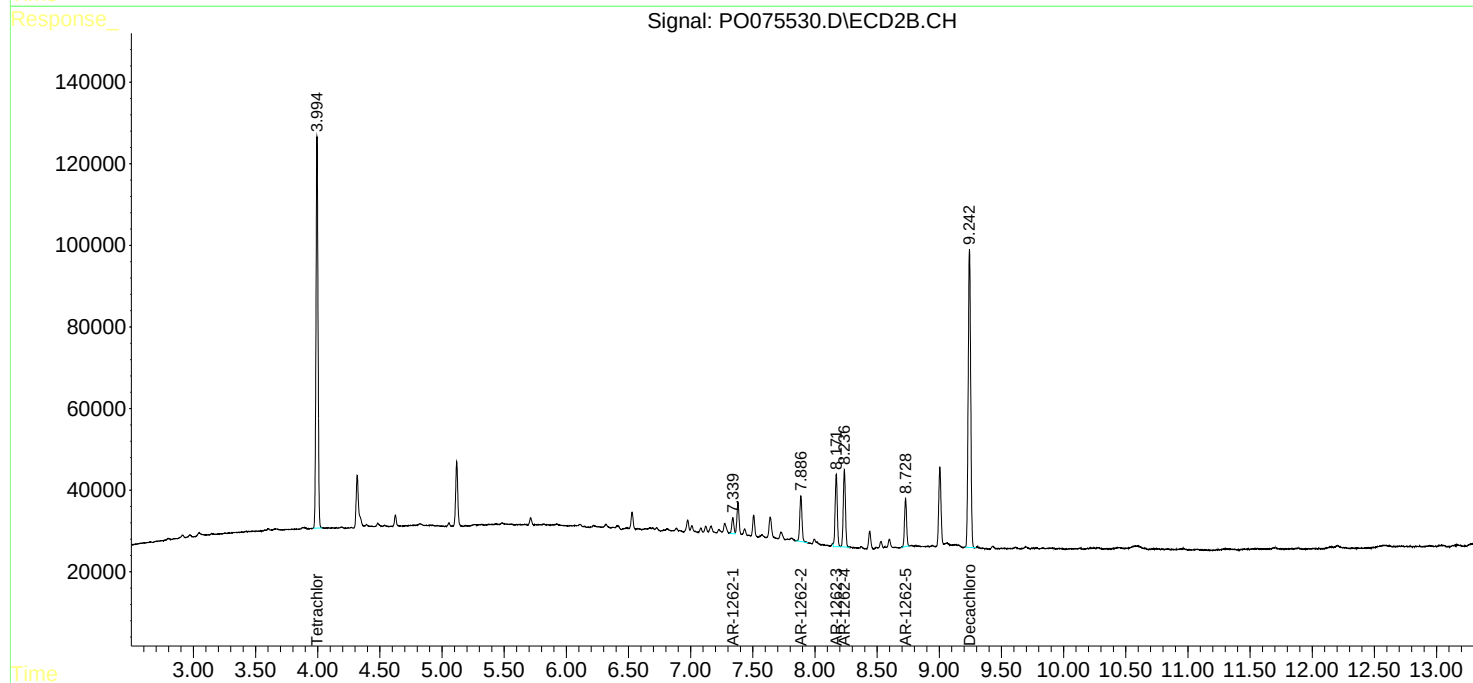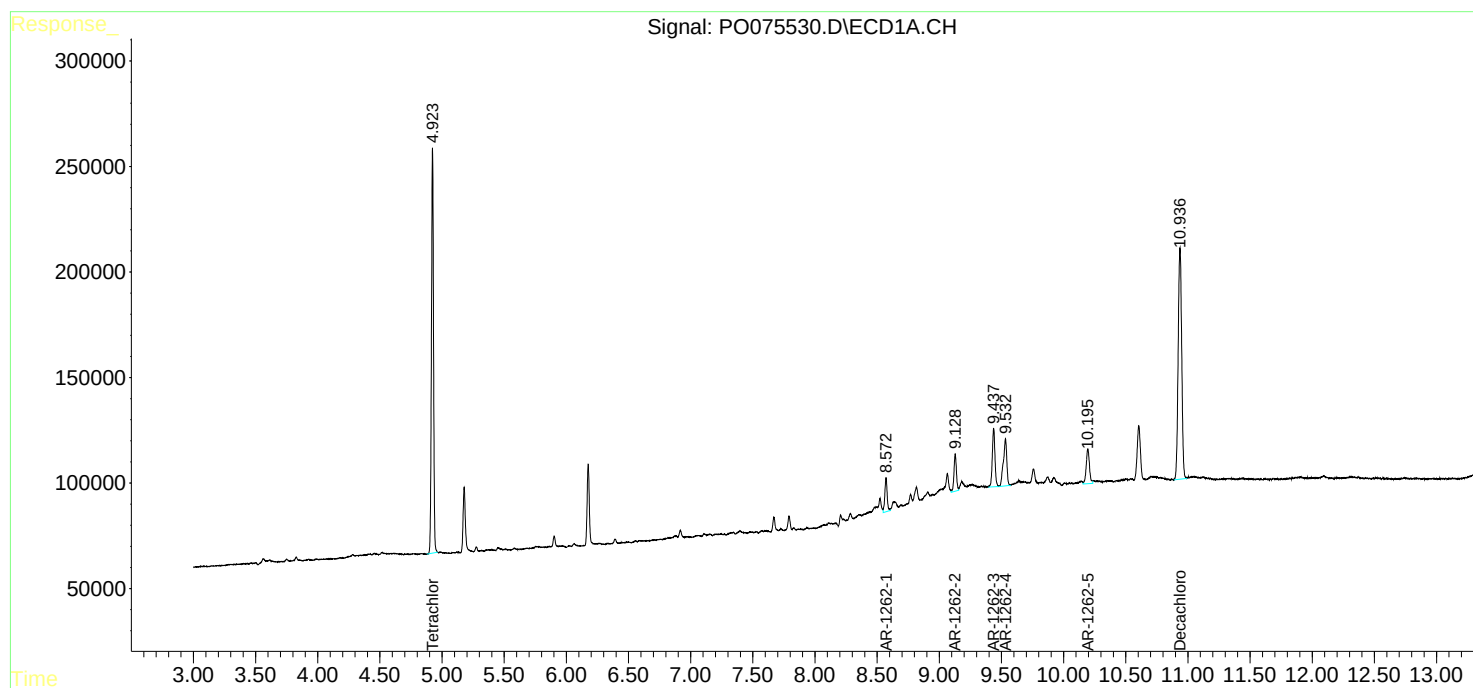

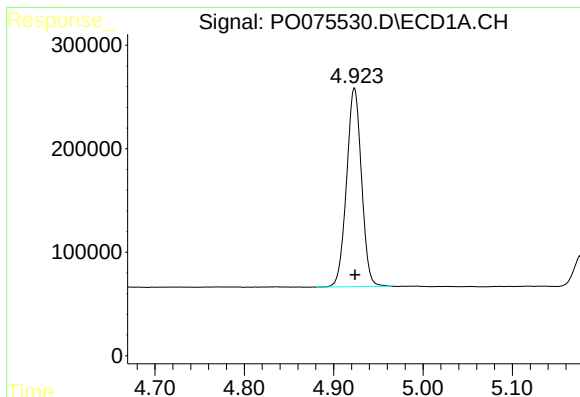


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 2226956
Conc: 22.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:29 AM

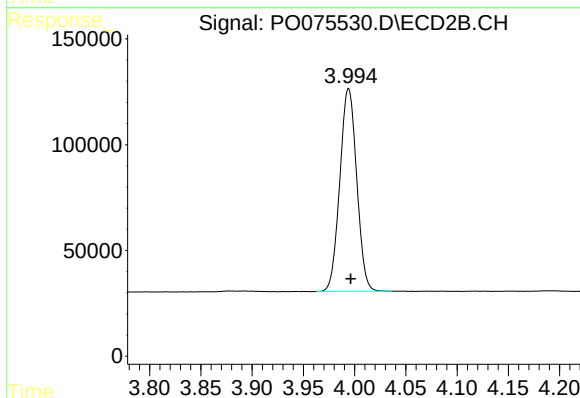


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1096493
Conc: 22.81 ng/ml

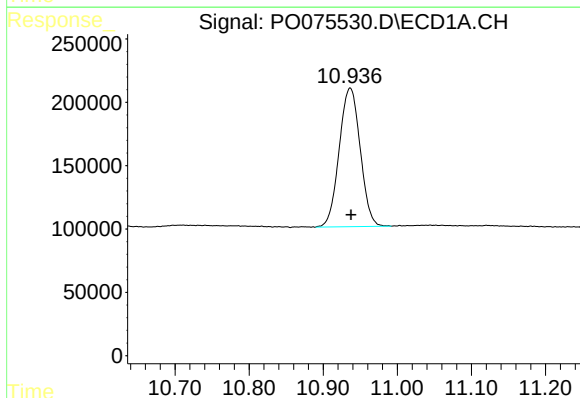


#2 Decachlorobiphenyl

R.T.: 10.936 min
Delta R.T.: -0.001 min
Response: 2157847
Conc: 22.37 ng/ml

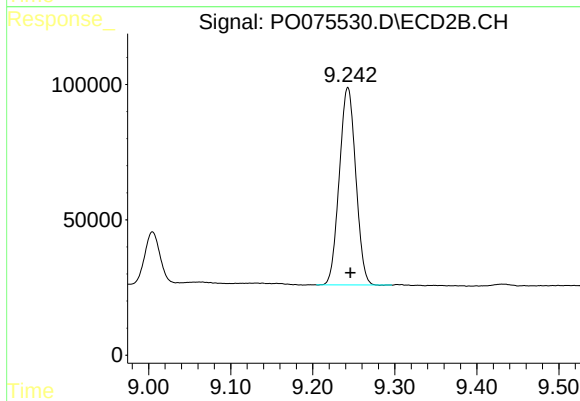

#2 Decachlorobiphenyl

R.T.: 9.243 min
Delta R.T.: -0.003 min
Response: 1015956
Conc: 20.93 ng/ml

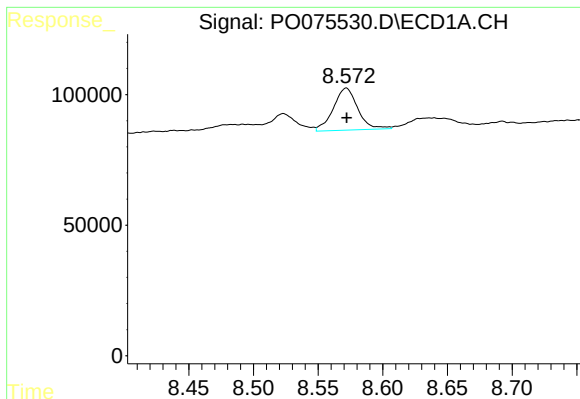


#36 AR-1262-1

R.T.: 8.572 min
Delta R.T.: 0.000 min
Response: 211974
Conc: 24.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:29 AM

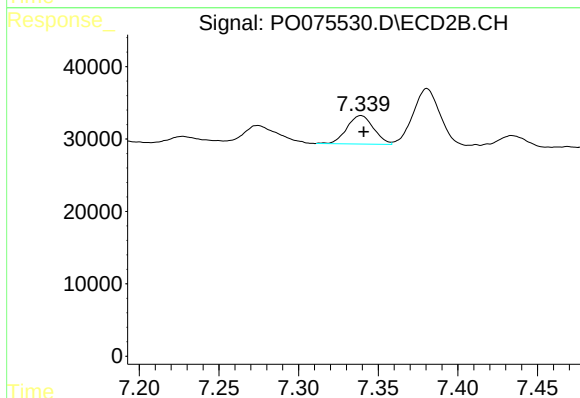


#36 AR-1262-1

R.T.: 7.339 min
Delta R.T.: -0.002 min
Response: 45711
Conc: 20.96 ng/ml

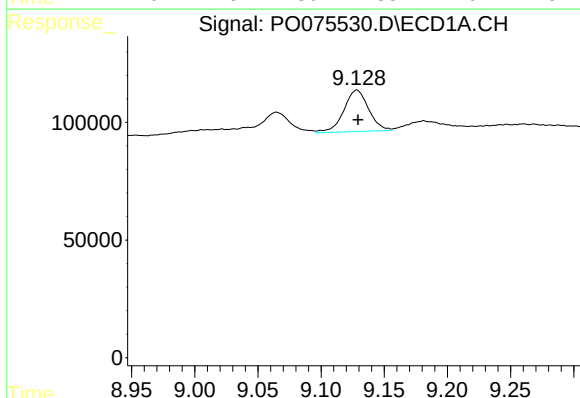


#37 AR-1262-2

R.T.: 9.128 min
Delta R.T.: 0.000 min
Response: 241101
Conc: 15.94 ng/ml

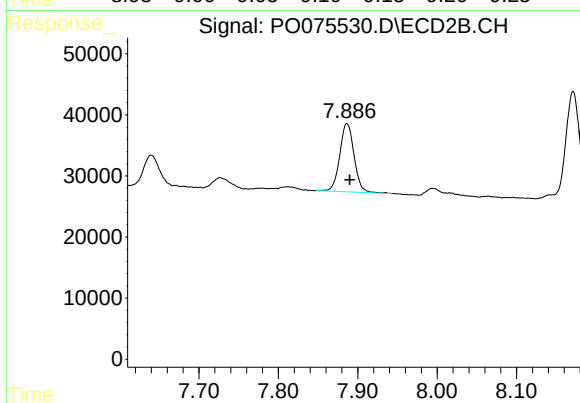

#37 AR-1262-2

R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 140435
Conc: 18.31 ng/ml

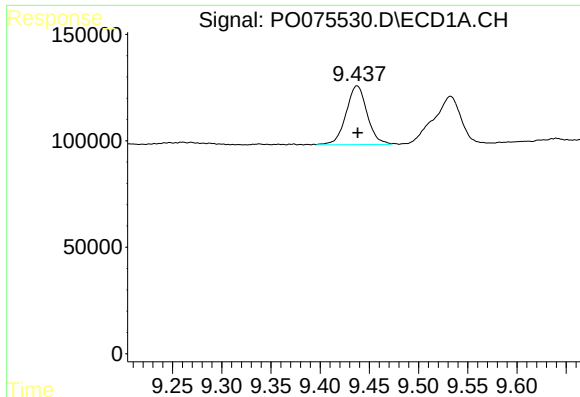


#38 AR-1262-3

R.T.: 9.438 min
Delta R.T.: 0.000 min
Response: 410696
Conc: 39.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0510


Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:29 AM

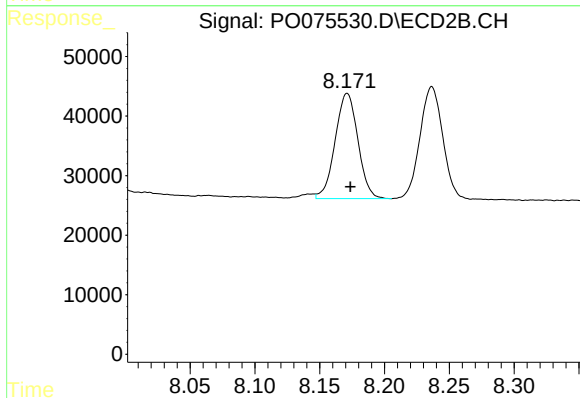


#38 AR-1262-3

R.T.: 8.171 min
Delta R.T.: -0.003 min
Response: 216590
Conc: 65.45 ng/ml m

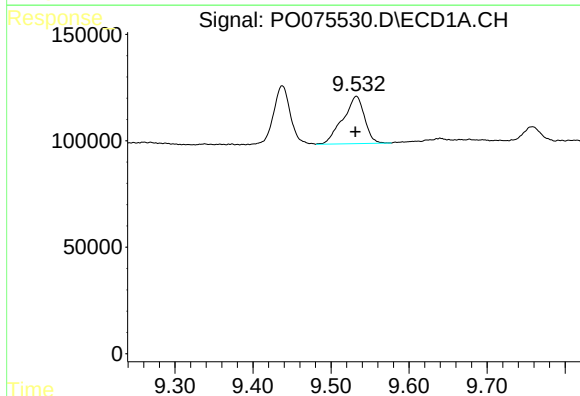


#39 AR-1262-4

R.T.: 9.533 min
Delta R.T.: 0.001 min
Response: 428656
Conc: 58.00 ng/ml

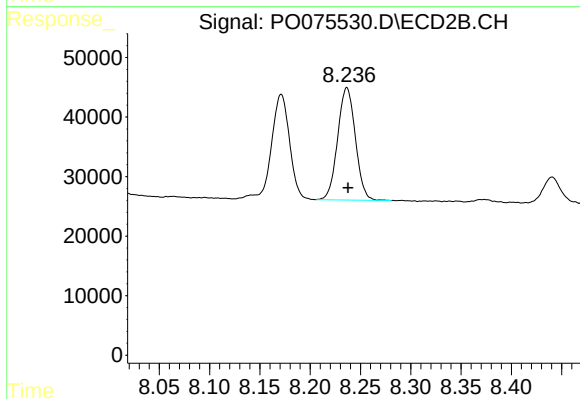

#39 AR-1262-4

R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 231800
Conc: 40.37 ng/ml

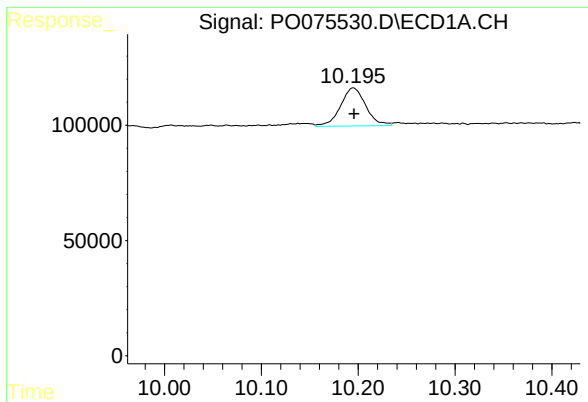


#40 AR-1262-5

R.T.: 10.195 min
Delta R.T.: 0.000 min
Response: 299095
Conc: 57.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU421-004-0510

Manual Integrations
APPROVED

Ankita
2/8/2021 8:41:29 AM

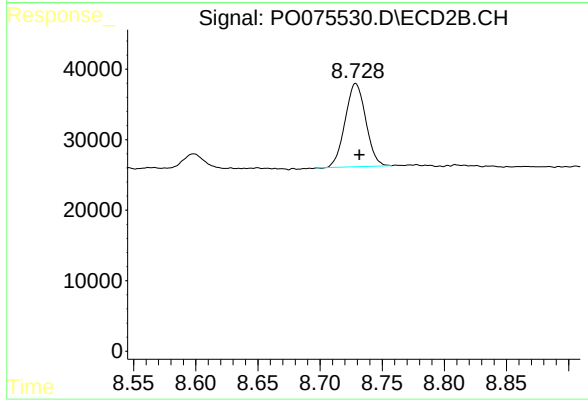

#40 AR-1262-5

R.T.: 8.729 min
Delta R.T.: -0.003 min
Response: 136740
Conc: 49.71 ng/ml