

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
 Data File : P0075544.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 00:31
 Operator : AJ/MA
 Sample : M1293-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT-4

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:42:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:21:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.995	1668481	759034	16.487m	15.790m
2) SA Decachlor...	10.937	9.242	1891850	853246	19.608	17.578m
Target Compounds						
31) L7 AR-1260-1	7.939	6.814	424801	261199	92.078	96.215
32) L7 AR-1260-2	8.206	7.011	985082	287917	152.619	86.791 #
33) L7 AR-1260-3	8.571	7.160	432870	272834	79.327	91.801m
34) L7 AR-1260-4	8.801	7.641	559562	174661	108.854m	67.140 #
35) L7 AR-1260-5	9.130	7.888	955510	447292	80.967	70.681

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020421\
Data File : PO075544.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 00:31
Operator : AJ/MA
Sample : M1293-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:21:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

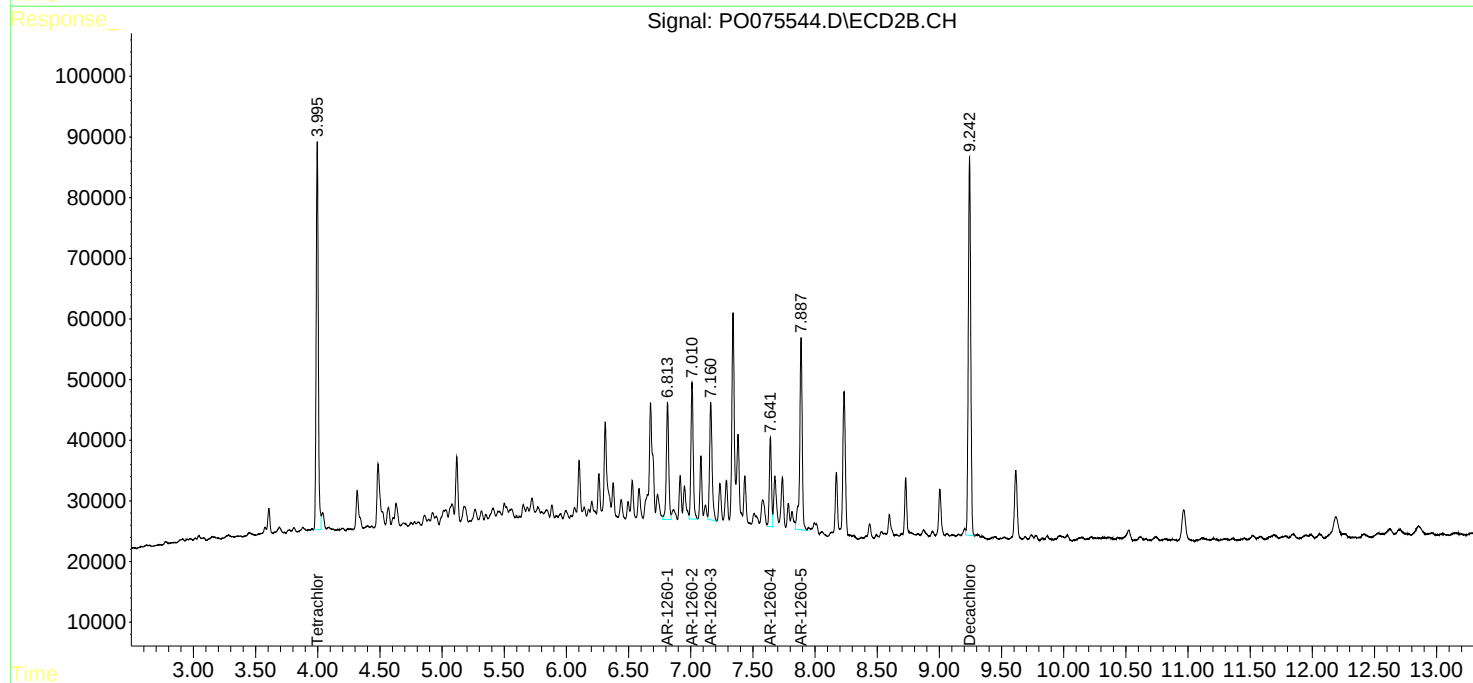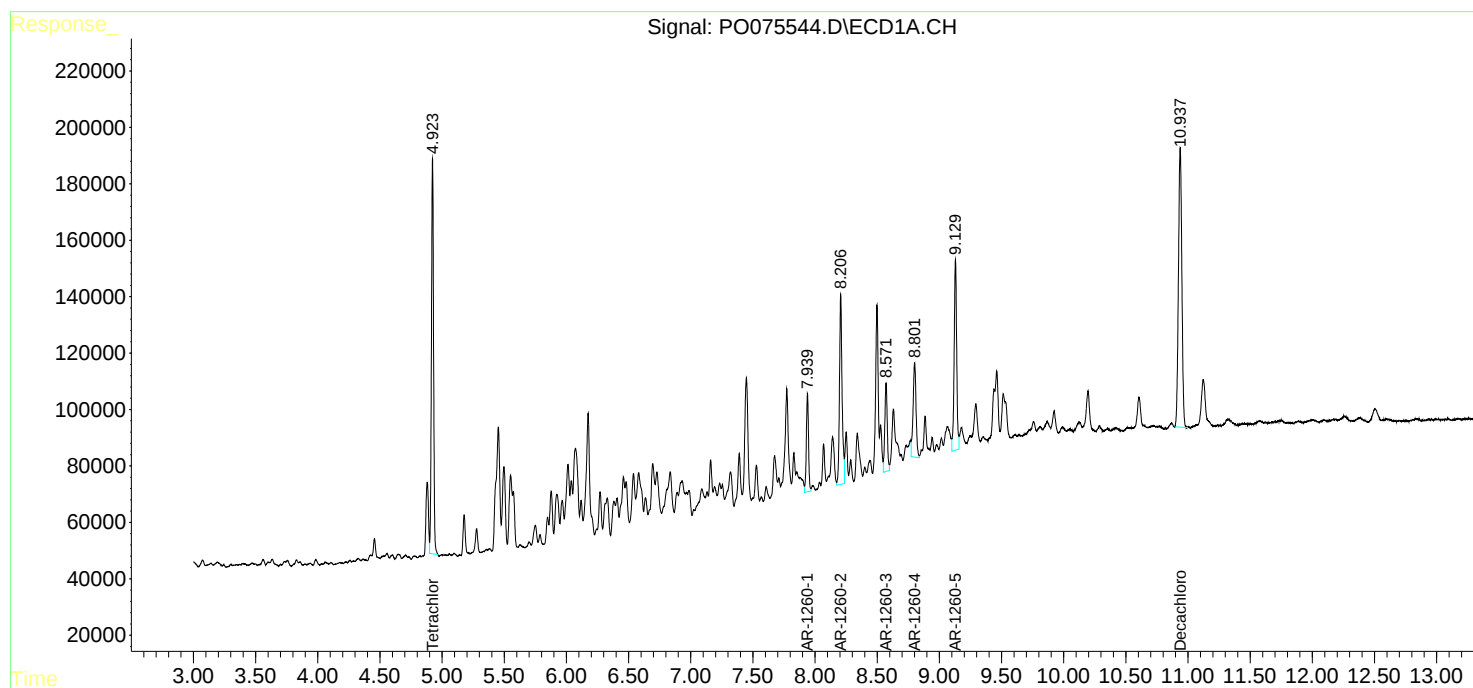

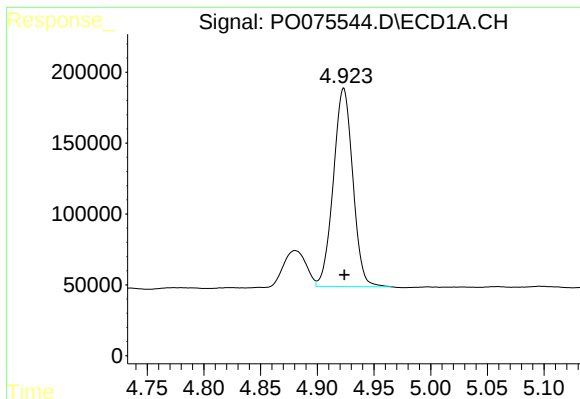


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 1668481
Conc: 16.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:08 AM

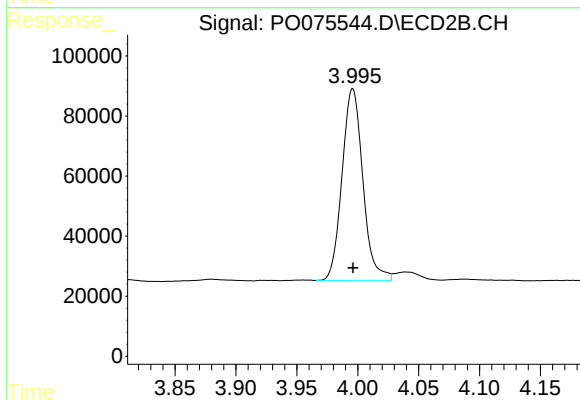


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 759034
Conc: 15.79 ng/ml m

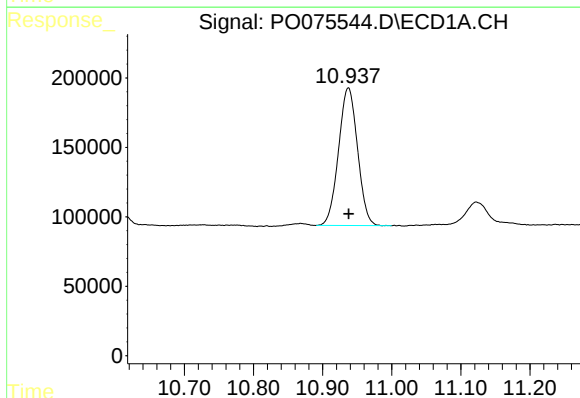


#2 Decachlorobiphenyl

R.T.: 10.937 min
Delta R.T.: 0.000 min
Response: 1891850
Conc: 19.61 ng/ml

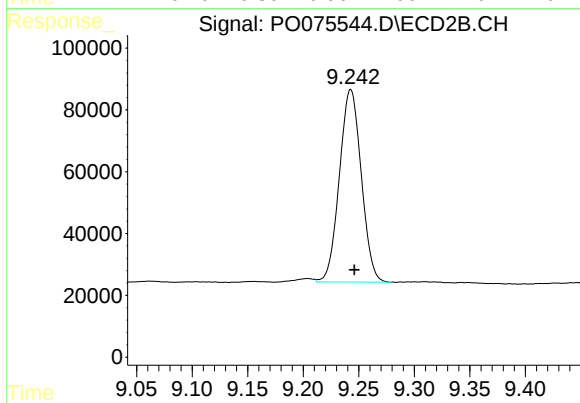

#2 Decachlorobiphenyl

R.T.: 9.242 min
Delta R.T.: -0.004 min
Response: 853246
Conc: 17.58 ng/ml m

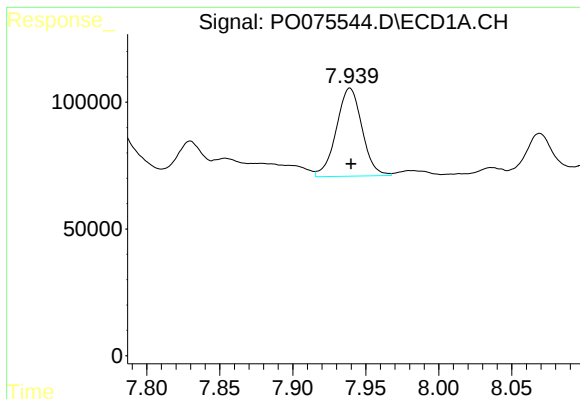


#31 AR-1260-1

R.T.: 7.939 min
Delta R.T.: 0.000 min
Response: 424801
Conc: 92.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:08 AM

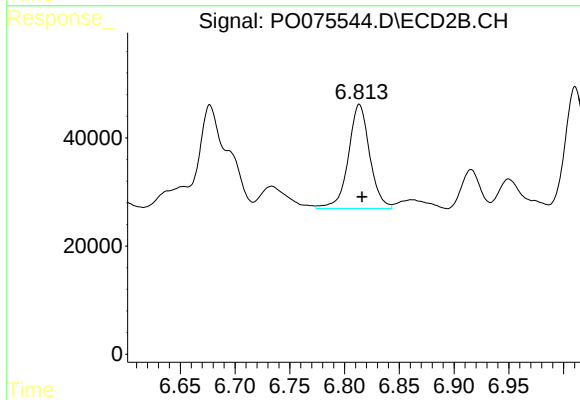


#31 AR-1260-1

R.T.: 6.814 min
Delta R.T.: -0.003 min
Response: 261199
Conc: 96.22 ng/ml

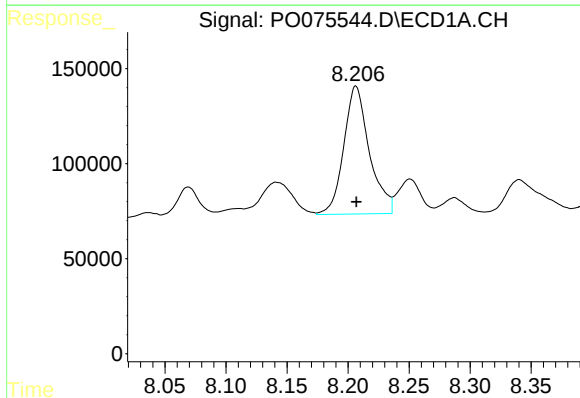


#32 AR-1260-2

R.T.: 8.206 min
Delta R.T.: 0.000 min
Response: 985082
Conc: 152.62 ng/ml

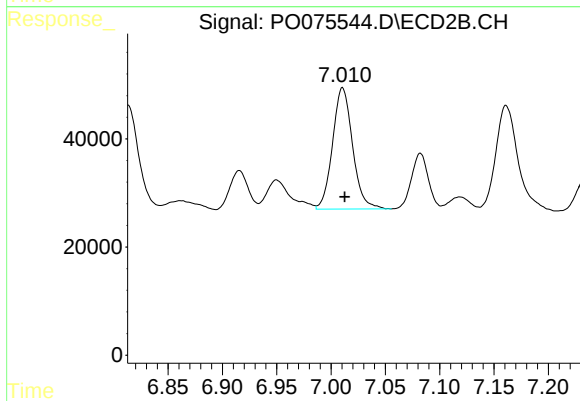

#32 AR-1260-2

R.T.: 7.011 min
Delta R.T.: -0.002 min
Response: 287917
Conc: 86.79 ng/ml

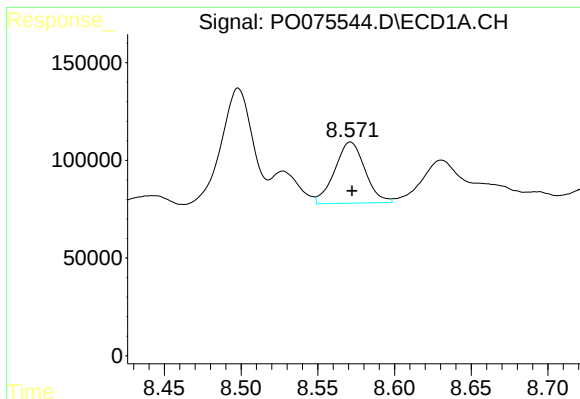


#33 AR-1260-3

R.T.: 8.571 min
Delta R.T.: -0.001 min
Response: 432870
Conc: 79.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4


Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:08 AM

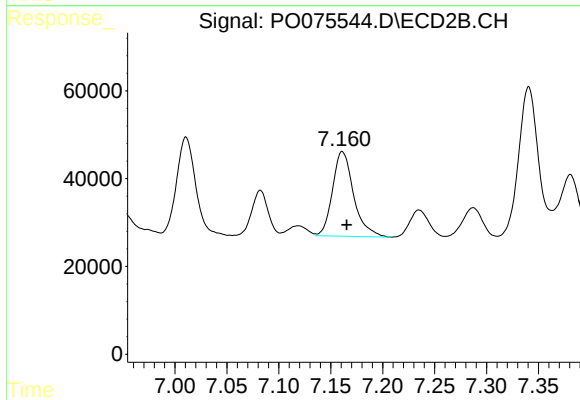


#33 AR-1260-3

R.T.: 7.160 min
Delta R.T.: -0.005 min
Response: 272834
Conc: 91.80 ng/ml m

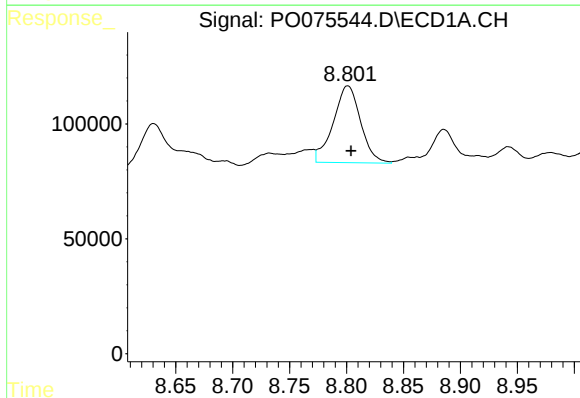


#34 AR-1260-4

R.T.: 8.801 min
Delta R.T.: -0.003 min
Response: 559562
Conc: 108.85 ng/ml m

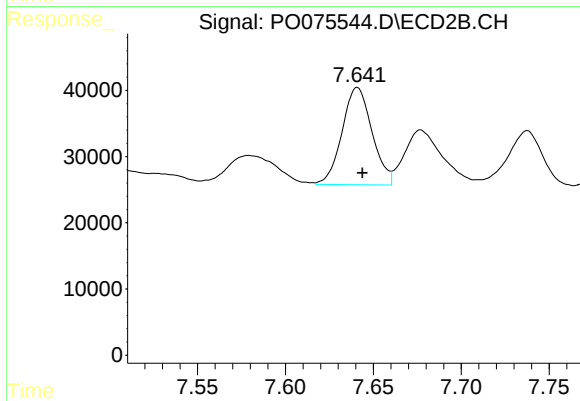

#34 AR-1260-4

R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 174661
Conc: 67.14 ng/ml

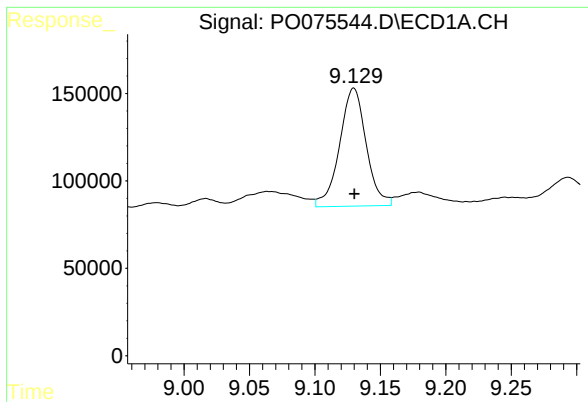


#35 AR-1260-5

R.T.: 9.130 min
Delta R.T.: 0.000 min
Response: 955510
Conc: 80.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT-4

Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:08 AM

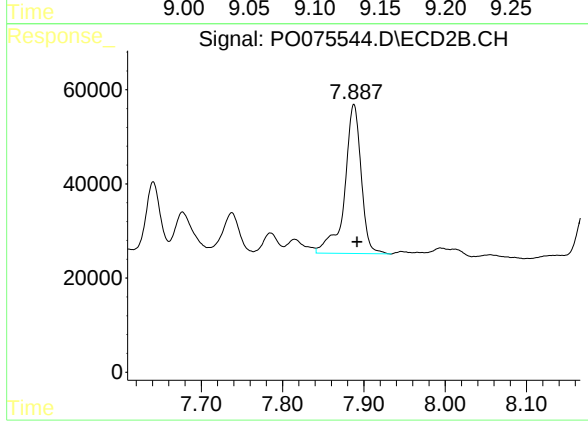

#35 AR-1260-5

R.T.: 7.888 min
Delta R.T.: -0.004 min
Response: 447292
Conc: 70.68 ng/ml