

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020421\
 Data File : P0075546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2021 1:06
 Operator : AJ/MA
 Sample : M1290-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WOOSPK-063-0002

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:42:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 05:11:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.921	3.994	1654862	907878	16.352m	18.886
2) SA Decachlor...	10.936	9.242	2008265	876270	20.815	18.052

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020421\
Data File : PO075546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2021 1:06
Operator : AJ/MA
Sample : M1290-09
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WOOSPK-063-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 05:11:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

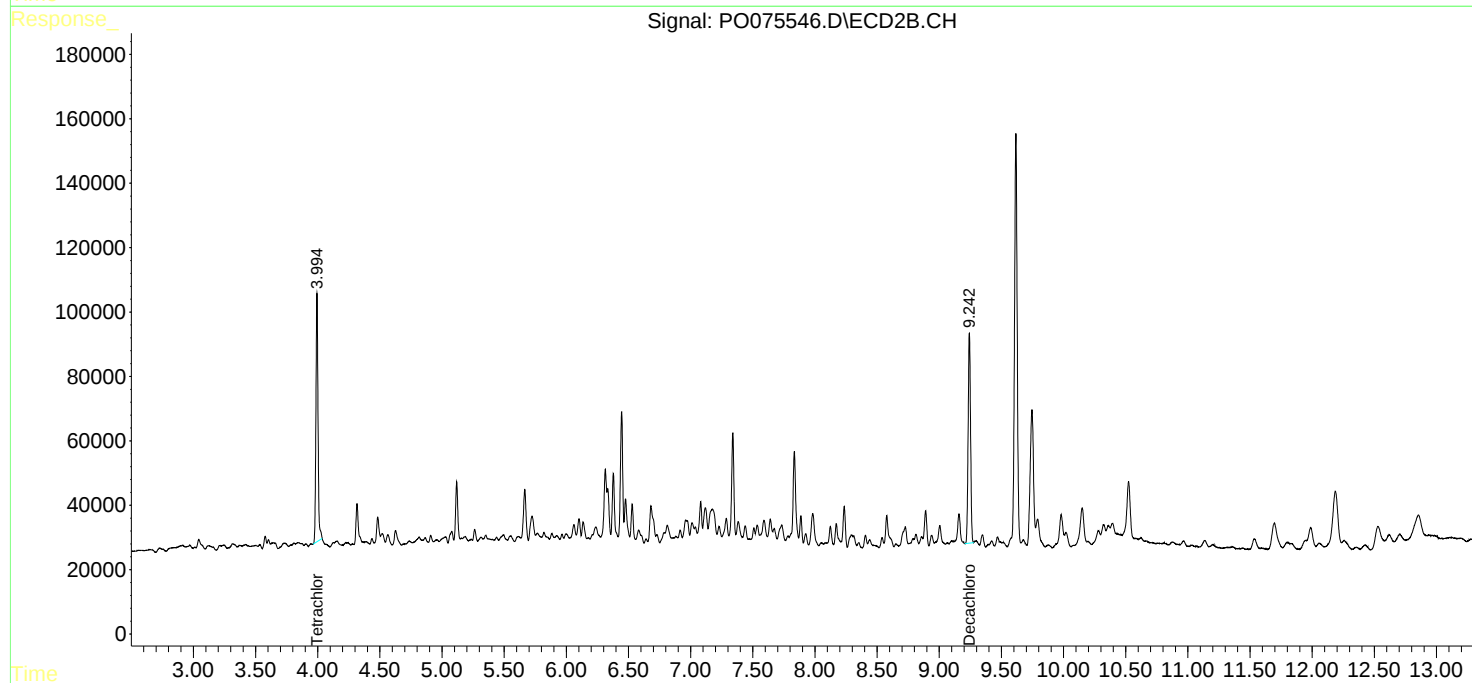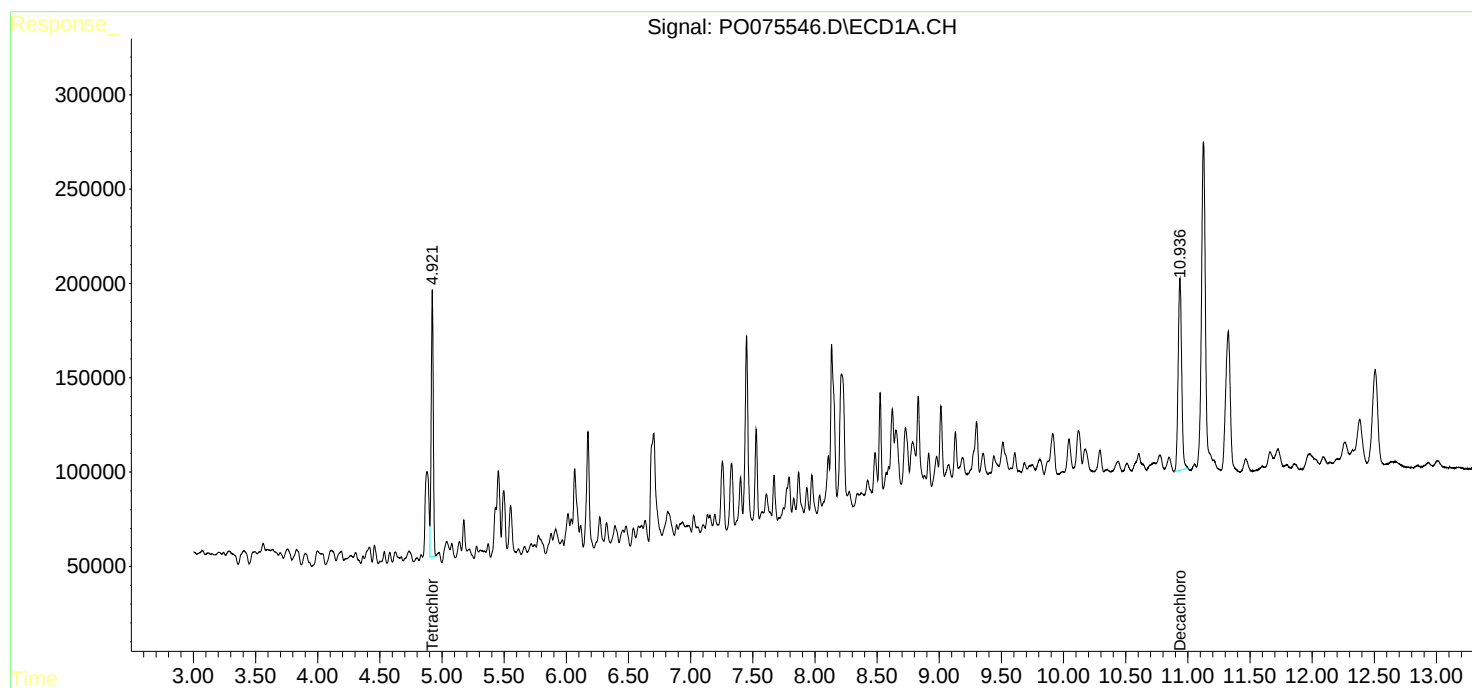

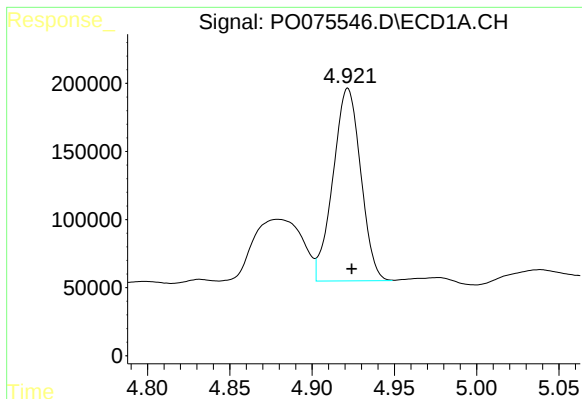


#1 Tetrachloro-m-xylene

R.T.: 4.921 min
Delta R.T.: -0.003 min
Response: 1654862
Conc: 16.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
WOOSPK-063-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 8:42:14 AM

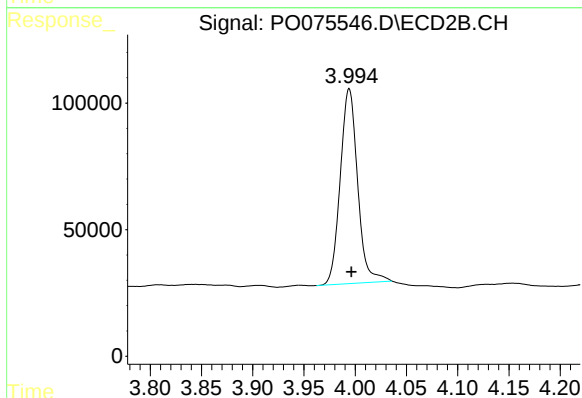


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 907878
Conc: 18.89 ng/ml

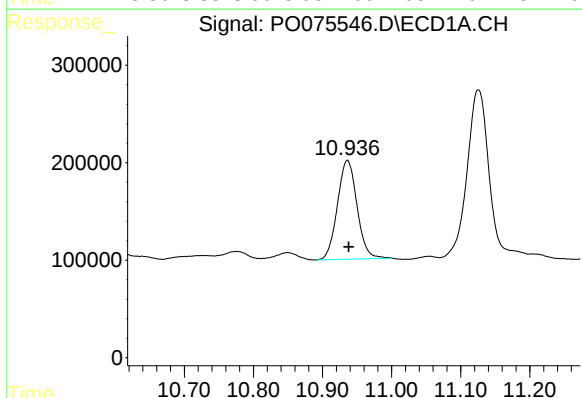

#2 Decachlorobiphenyl

R.T.: 10.936 min
Delta R.T.: -0.002 min
Response: 2008265
Conc: 20.81 ng/ml

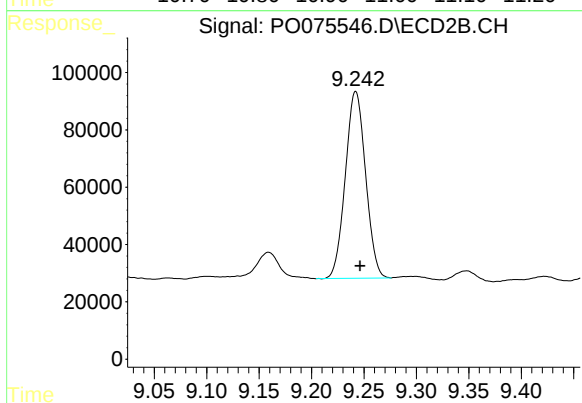

#2 Decachlorobiphenyl

R.T.: 9.242 min
Delta R.T.: -0.004 min
Response: 876270
Conc: 18.05 ng/ml