

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
 Data File : P0066272.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2020 10:46
 Operator : DD\AJ
 Sample : L1377-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BW-2

Manual Integrations
 APPROVED

mohammad
 2/7/2020 5:02:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 04:50:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.431	866617	1119546	29.749m	27.370
2) SA Decachlor...	9.643	8.323	763437	1041925	19.373	17.777

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020520\
Data File : PO066272.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 10:46
Operator : DD\AJ
Sample : L1377-01
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampled :
BW-2


Manual Integrations
APPROVED

mohammad
2/7/2020 5:02:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 04:50:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

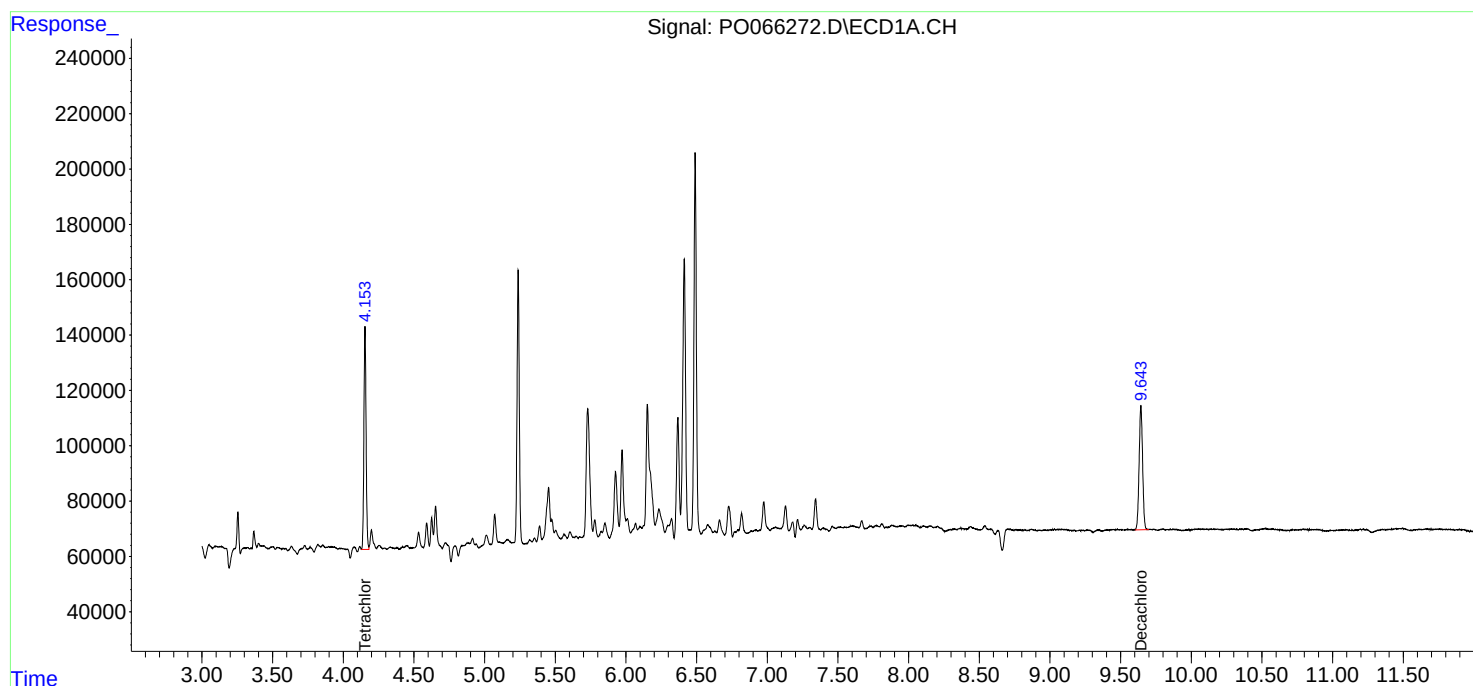

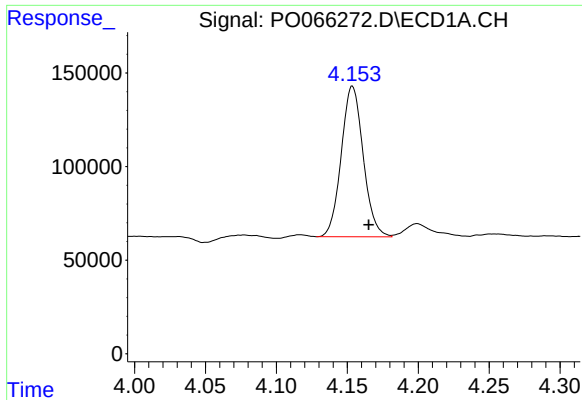


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: -0.012 min
Response: 866617
Conc: 29.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BW-2


Manual Integrations
APPROVED

mohammad
2/7/2020 5:02:36 PM

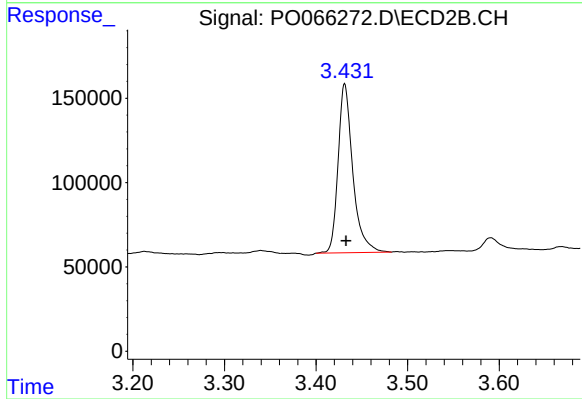


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.001 min
Response: 1119546
Conc: 27.37 ng/ml

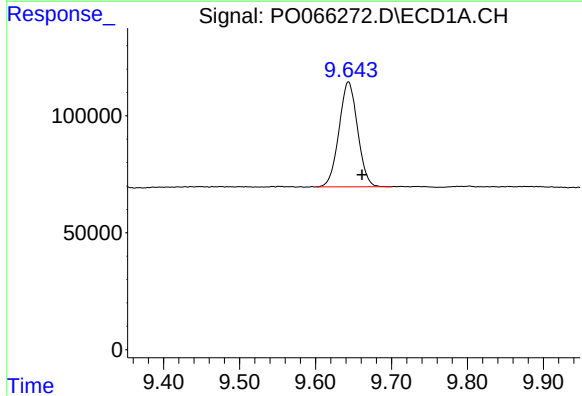

#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.018 min
Response: 763437
Conc: 19.37 ng/ml

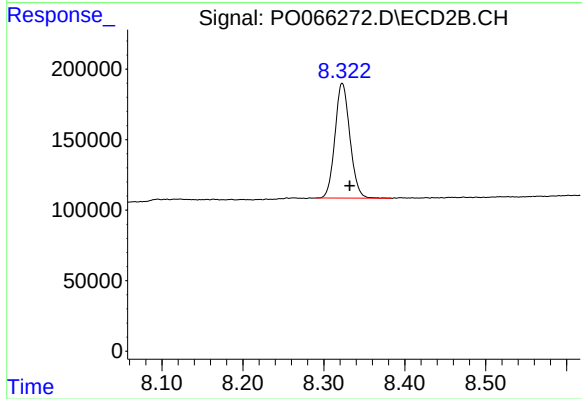

#2 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.009 min
Response: 1041925
Conc: 17.78 ng/ml