

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
 Data File : P0066298.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2020 18:02
 Operator : DD\AJ
 Sample : L1379-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M030-3A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 05:01:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.153	3.430	826663	1052062	28.378m	25.720
2)	SA Decachlor...	9.645	8.325	362405	523740	9.196	8.936
Target Compounds							
26)	L6 AR-1254-1	6.143	5.274	541567	860419	348.564	270.308
27)	L6 AR-1254-2	6.359	5.420	1037880	1077752	417.683	367.235
28)	L6 AR-1254-3	6.721	5.817	1250423	1897547	467.954	413.204
29)	L6 AR-1254-4	7.005	6.043	1108140	1374781	479.901	436.315
30)	L6 AR-1254-5	7.419	6.456	1613036	3057691	706.927	721.928



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
Data File : P0066298.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 18:02
Operator : DD\AJ
Sample : L1379-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
M030-3A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:01:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

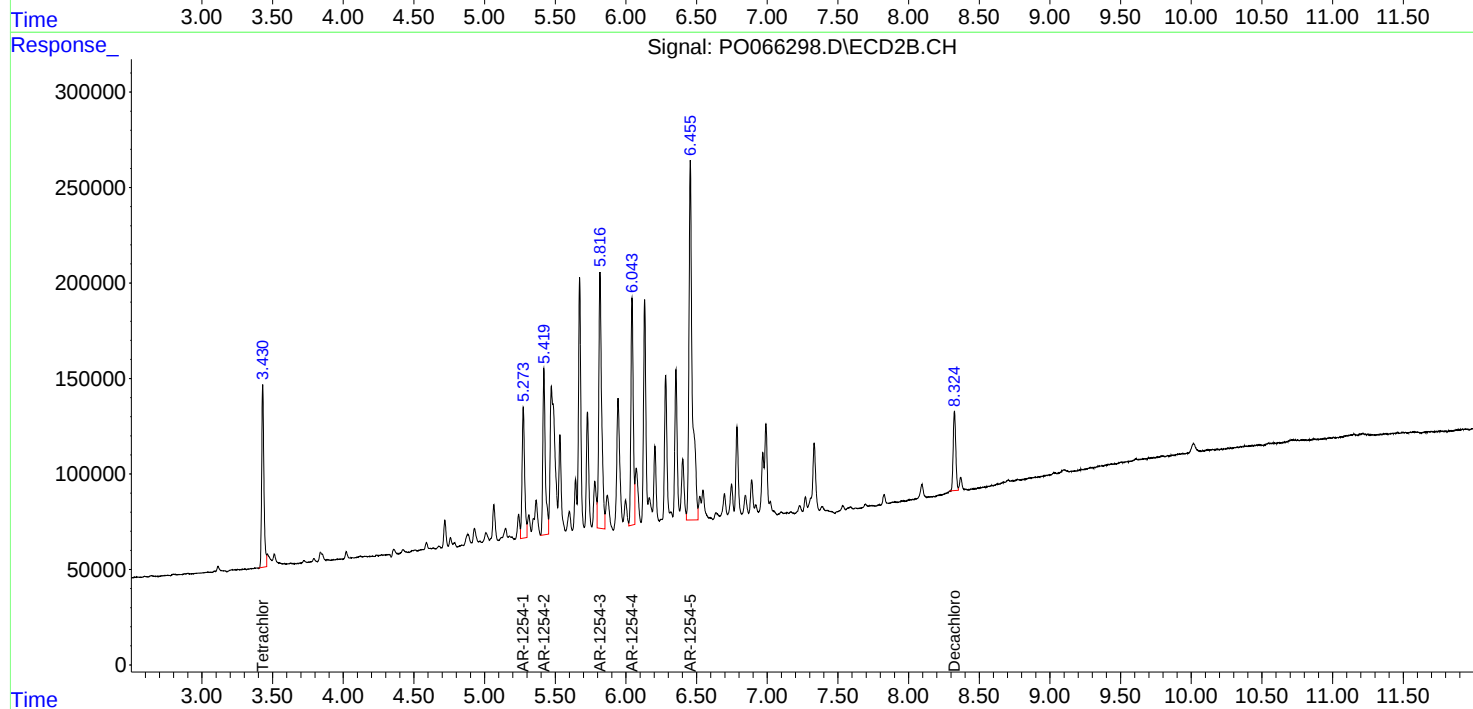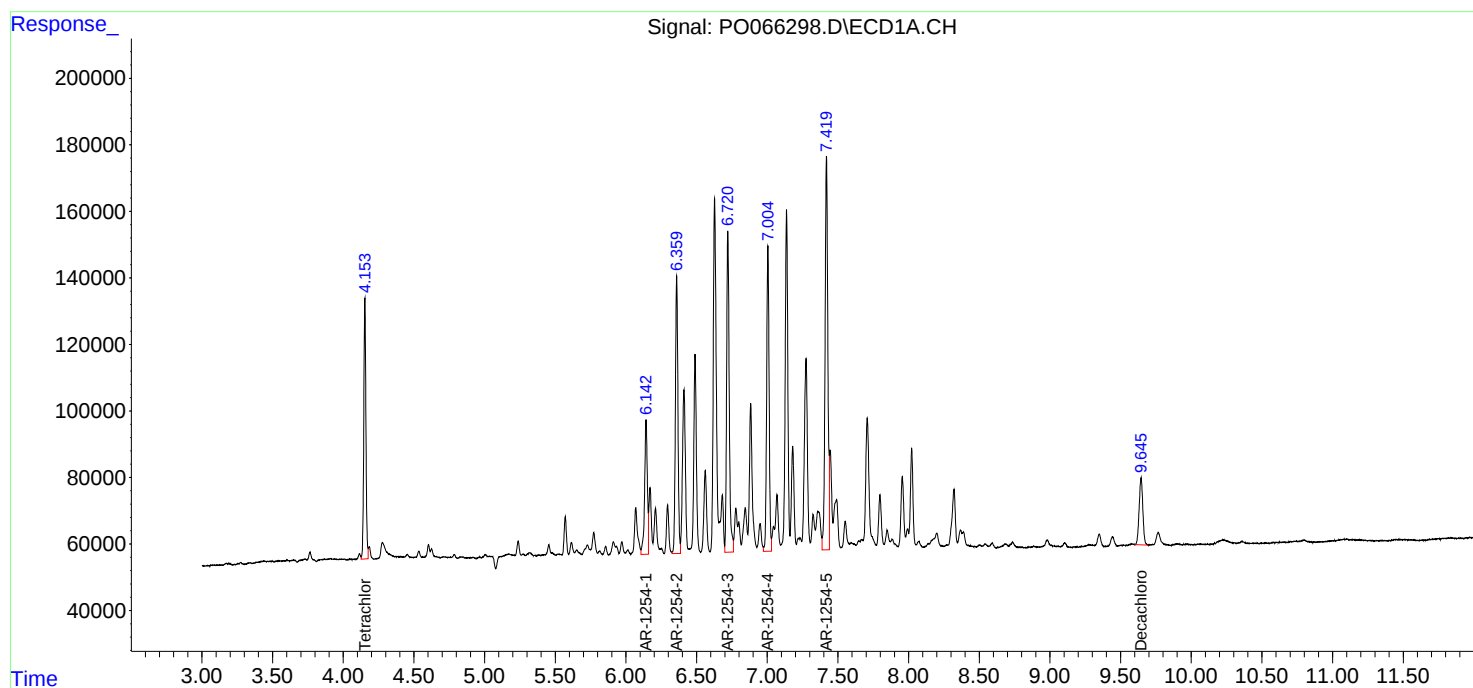


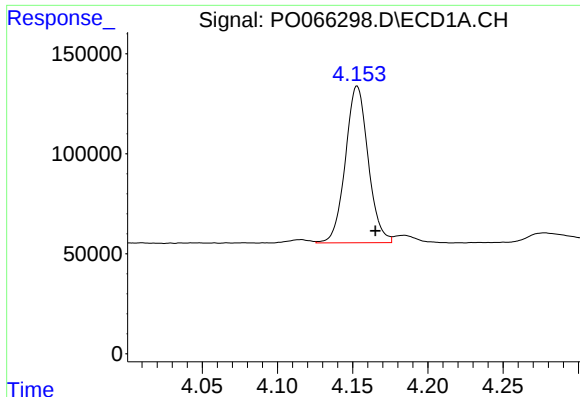

#1 Tetrachloro-m-xylene


R.T.: 4.153 min
Delta R.T.: -0.012 min
Response: 826663
Conc: 28.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
M030-3A

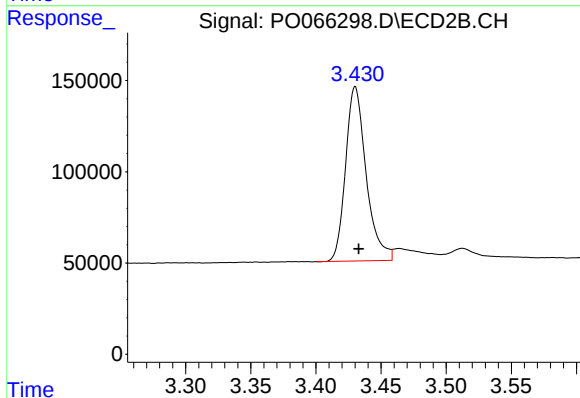


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 1052062
Conc: 25.72 ng/ml

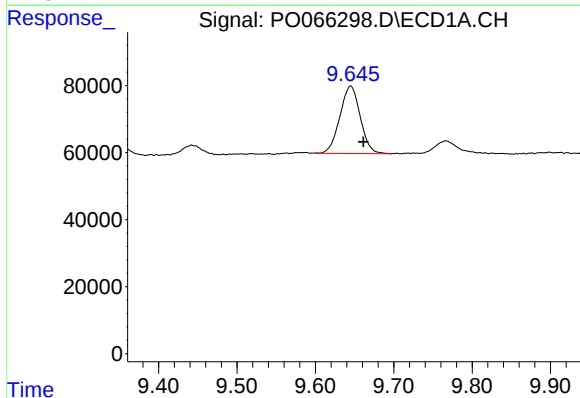


#2 Decachlorobiphenyl

R.T.: 9.645 min
Delta R.T.: -0.016 min
Response: 362405
Conc: 9.20 ng/ml

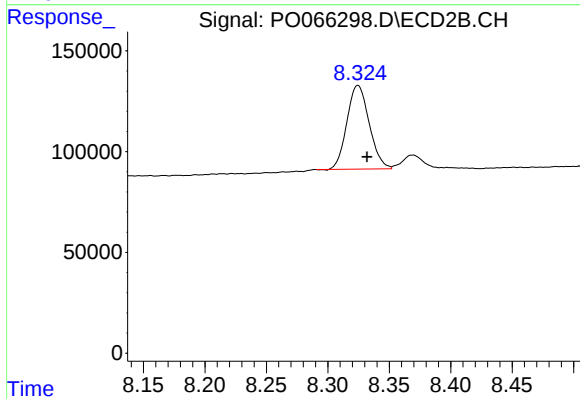

#2 Decachlorobiphenyl


R.T.: 8.325 min
Delta R.T.: -0.007 min
Response: 523740
Conc: 8.94 ng/ml

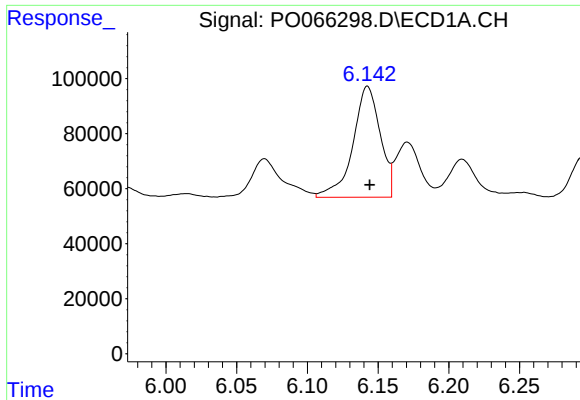

#26 AR-1254-1


R.T.: 6.143 min
Delta R.T.: -0.002 min
Response: 541567
Conc: 348.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-3A

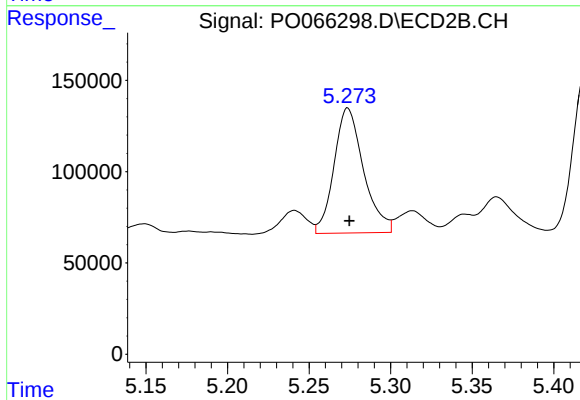


#26 AR-1254-1

R.T.: 5.274 min
Delta R.T.: -0.001 min
Response: 860419
Conc: 270.31 ng/ml

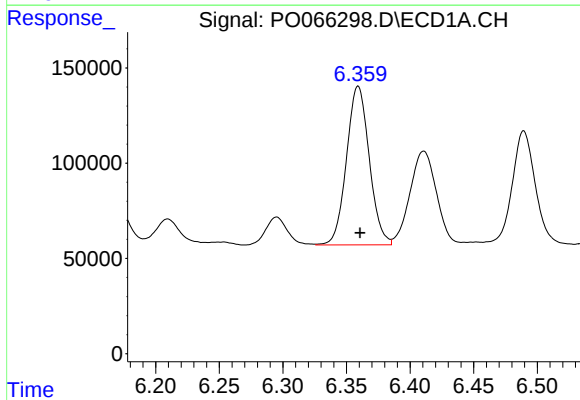


#27 AR-1254-2

R.T.: 6.359 min
Delta R.T.: -0.001 min
Response: 1037880
Conc: 417.68 ng/ml

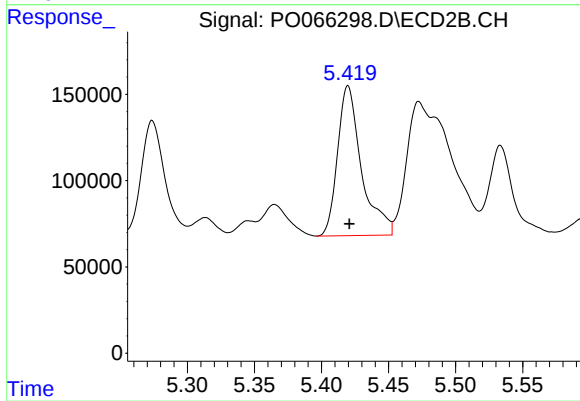

#27 AR-1254-2


R.T.: 5.420 min
Delta R.T.: 0.000 min
Response: 1077752
Conc: 367.24 ng/ml

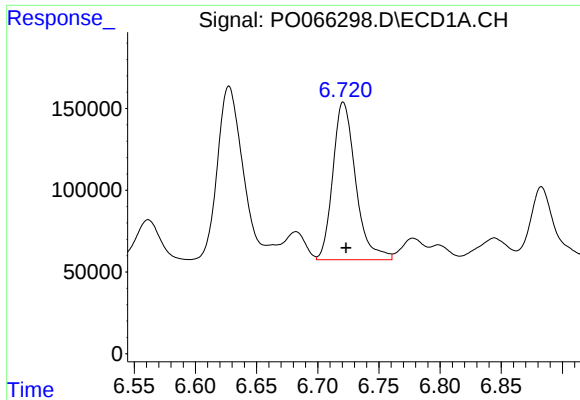

#28 AR-1254-3


R.T.: 6.721 min
Delta R.T.: -0.002 min
Response: 1250423
Conc: 467.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-3A

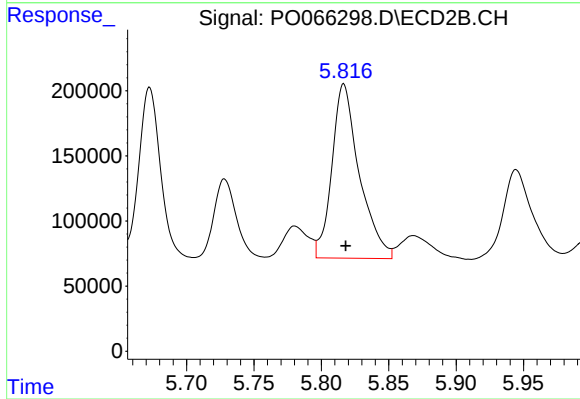


#28 AR-1254-3

R.T.: 5.817 min
Delta R.T.: -0.002 min
Response: 1897547
Conc: 413.20 ng/ml

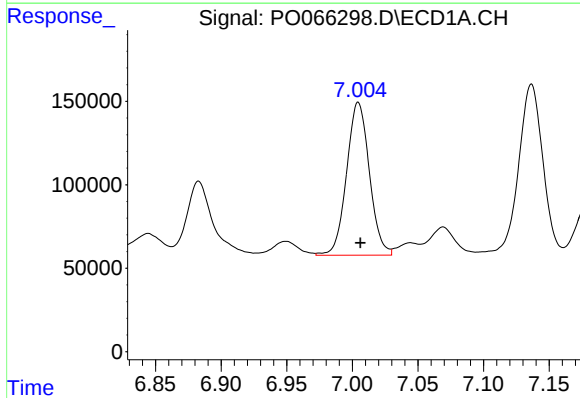


#29 AR-1254-4

R.T.: 7.005 min
Delta R.T.: -0.002 min
Response: 1108140
Conc: 479.90 ng/ml

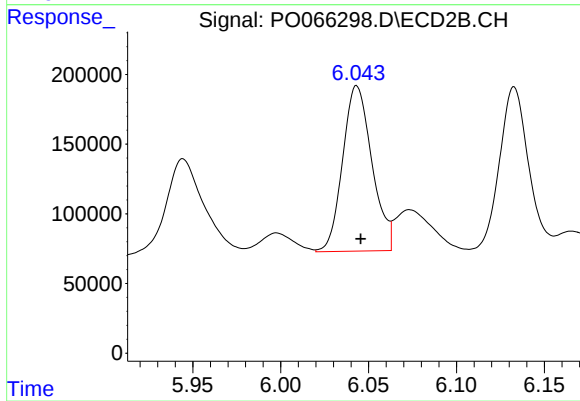

#29 AR-1254-4


R.T.: 6.043 min
Delta R.T.: -0.002 min
Response: 1374781
Conc: 436.32 ng/ml

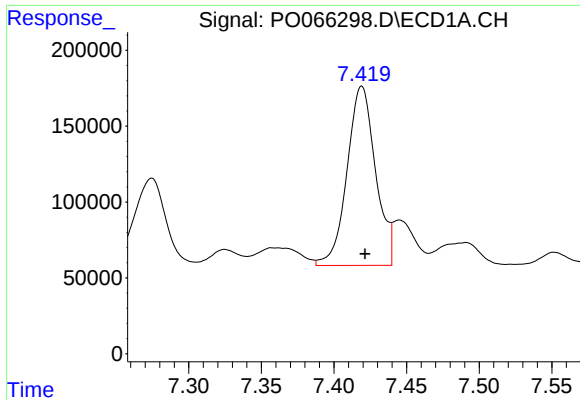

#30 AR-1254-5

R.T.: 7.419 min
Delta R.T.: -0.002 min
Response: 1613036
Conc: 706.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-3A

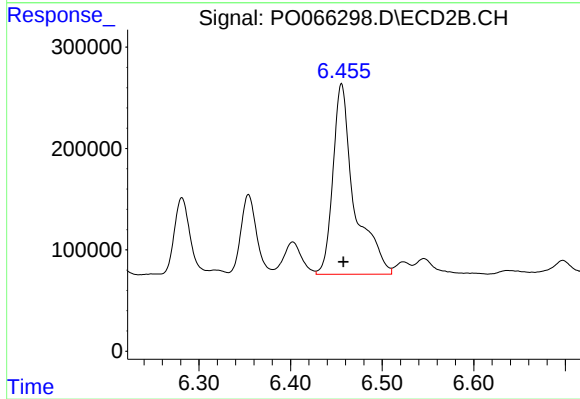

#30 AR-1254-5

R.T.: 6.456 min
Delta R.T.: -0.002 min
Response: 3057691
Conc: 721.93 ng/ml