

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
 Data File : P0066305.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2020 19:59
 Operator : DD\AJ
 Sample : L1379-14
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M030-6A

Manual Integrations
 APPROVED

mohammad
 2/7/2020 5:03:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 05:04:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.152	3.430	577272	722299	19.817	17.658
2)	SA Decachlor...	9.643	8.323	203187	277719	5.156	4.738
Target Compounds							
26)	L6 AR-1254-1	6.147	5.277	50498	79912	32.502	25.105
27)	L6 AR-1254-2	6.360	5.420	69545	41739	27.988	14.222 #
28)	L6 AR-1254-3	6.722	5.815	90708	145542	33.946	31.693
29)	L6 AR-1254-4	7.004	6.042	60169	83333	26.057m	26.447
30)	L6 AR-1254-5	7.418	6.454	95640	145917	41.915m	34.451

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020520\
Data File : PO066305.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 19:59
Operator : DD\AJ
Sample : L1379-14
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
M030-6A


Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:04:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

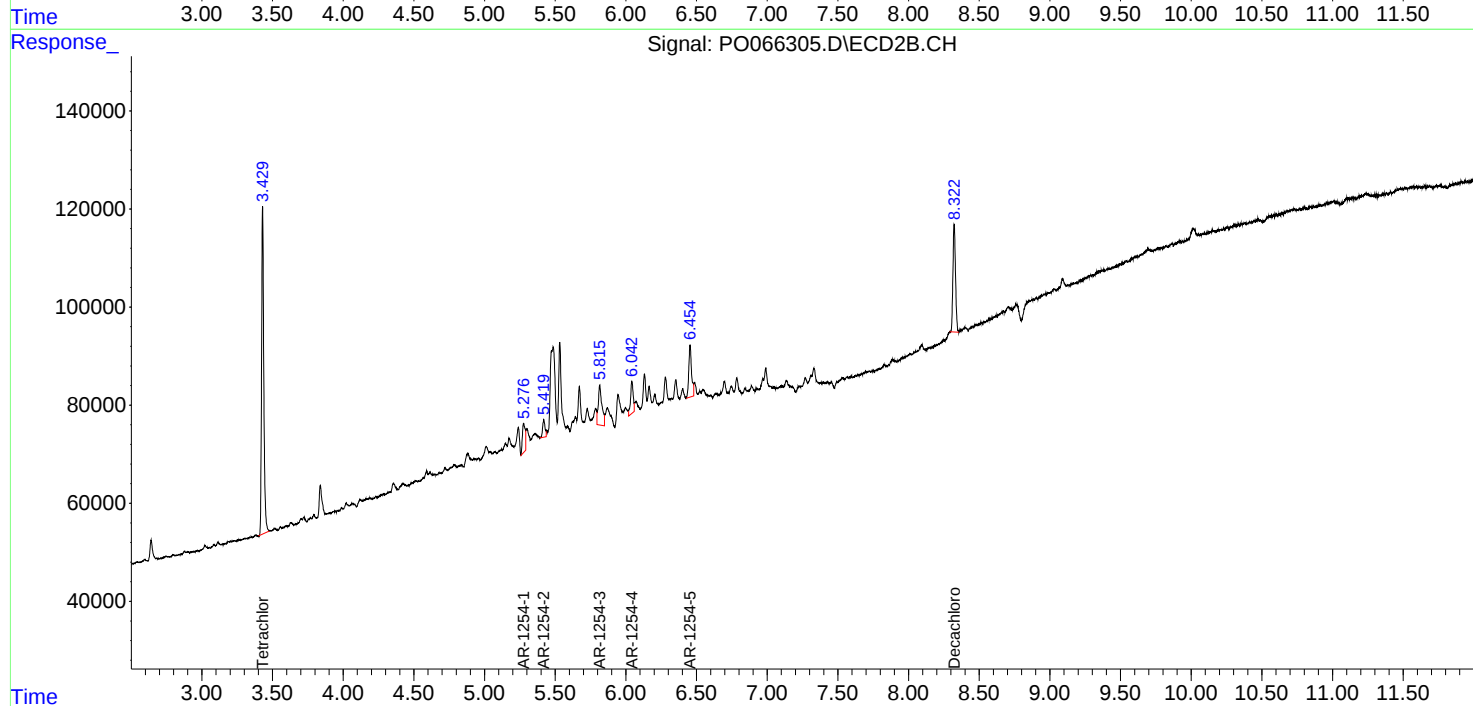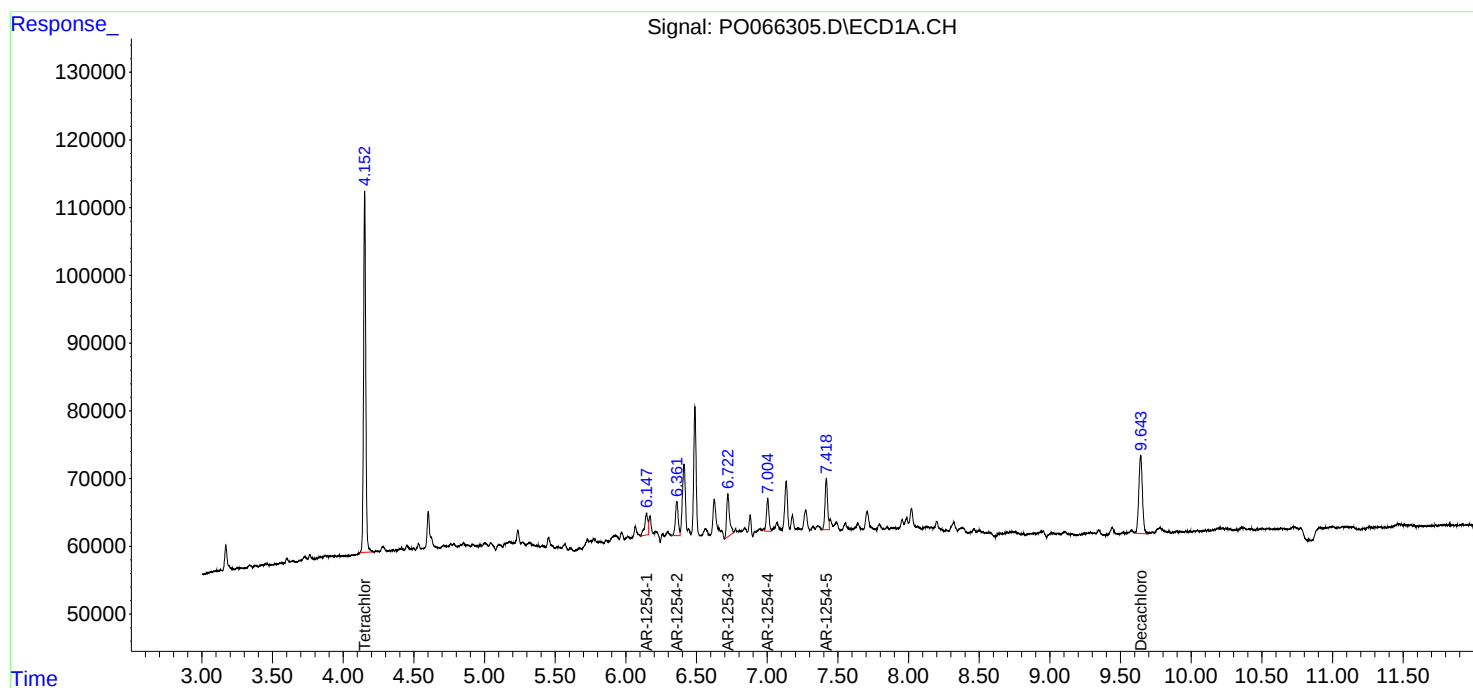

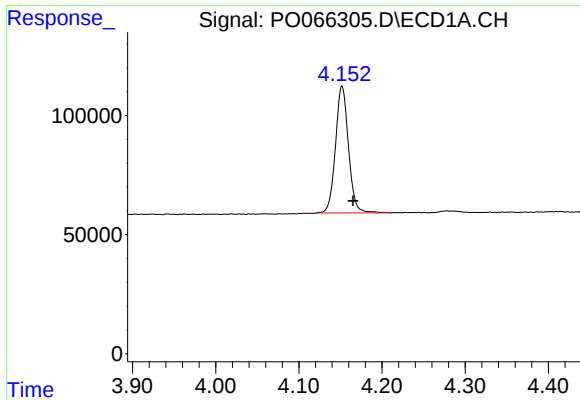


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: -0.013 min
Response: 577272
Conc: 19.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-6A


Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:32 PM

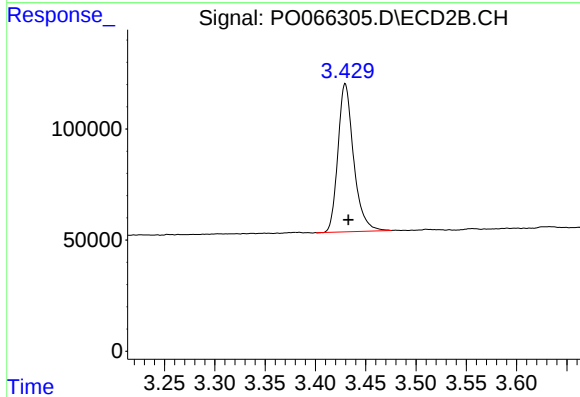


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 722299
Conc: 17.66 ng/ml

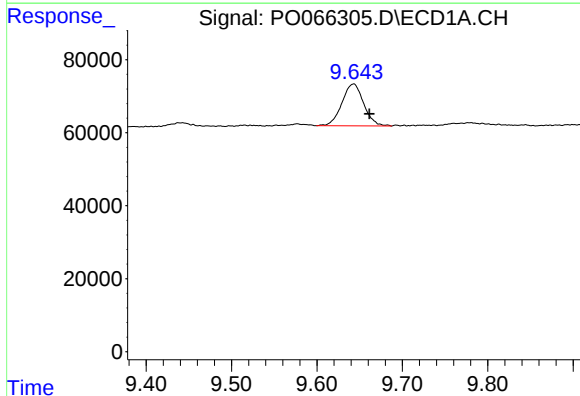


#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.018 min
Response: 203187
Conc: 5.16 ng/ml

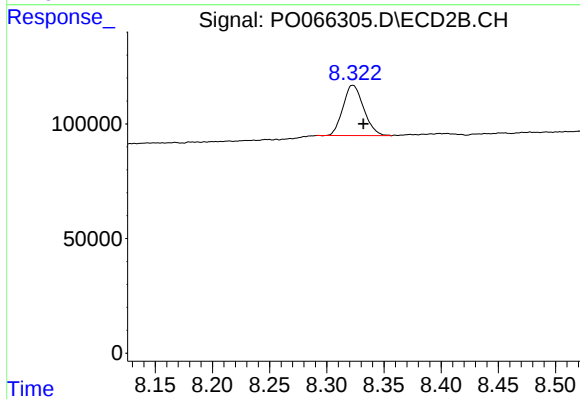

#2 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.009 min
Response: 277719
Conc: 4.74 ng/ml

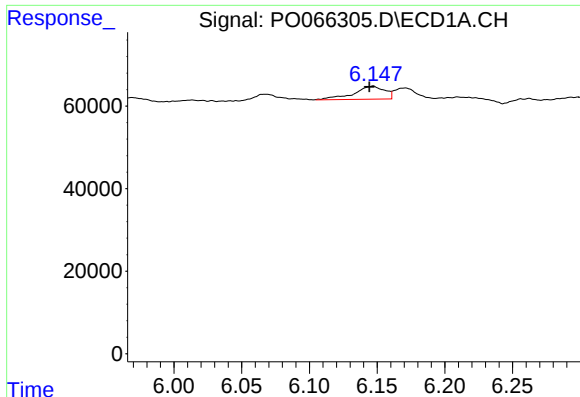


#26 AR-1254-1

R.T.: 6.147 min
Delta R.T.: 0.003 min
Response: 50498
Conc: 32.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-6A


Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:32 PM

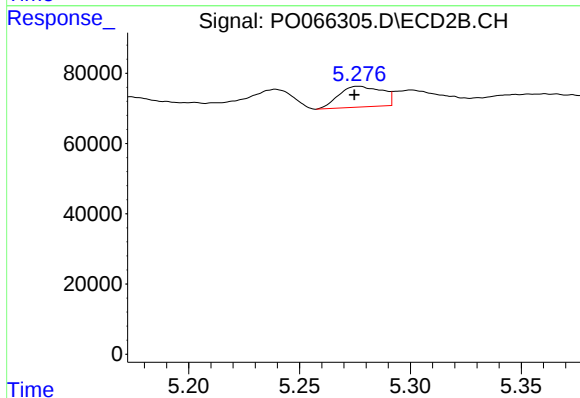


#26 AR-1254-1

R.T.: 5.277 min
Delta R.T.: 0.002 min
Response: 79912
Conc: 25.11 ng/ml

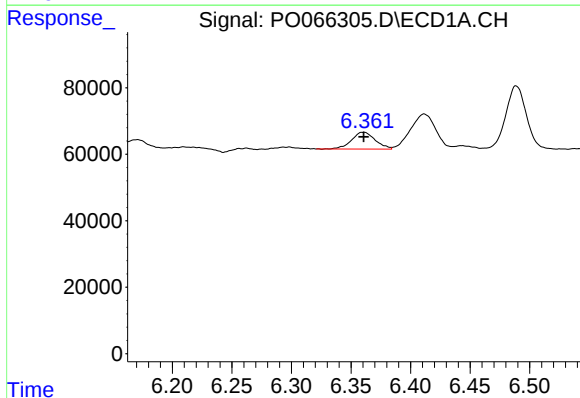


#27 AR-1254-2

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 69545
Conc: 27.99 ng/ml

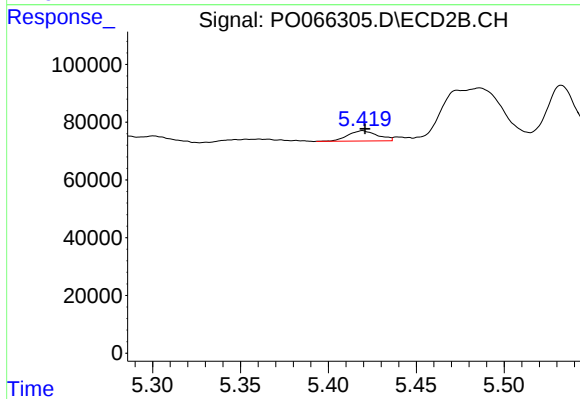

#27 AR-1254-2

R.T.: 5.420 min
Delta R.T.: -0.001 min
Response: 41739
Conc: 14.22 ng/ml

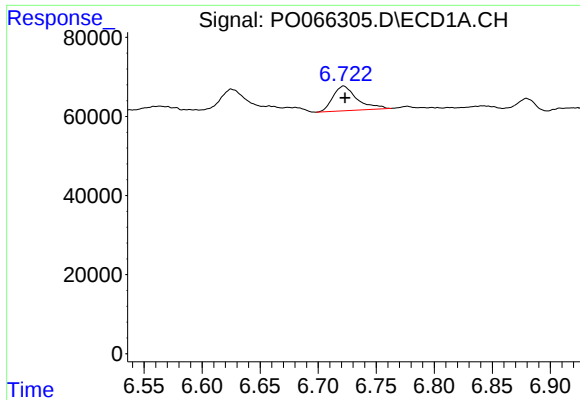


#28 AR-1254-3

R.T.: 6.722 min
Delta R.T.: -0.001 min
Response: 90708
Conc: 33.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-6A


Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:32 PM

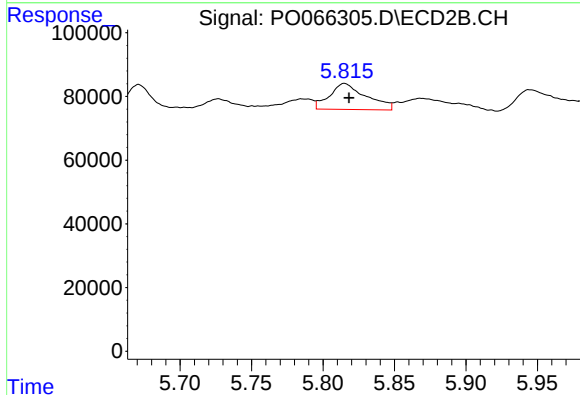


#28 AR-1254-3

R.T.: 5.815 min
Delta R.T.: -0.003 min
Response: 145542
Conc: 31.69 ng/ml

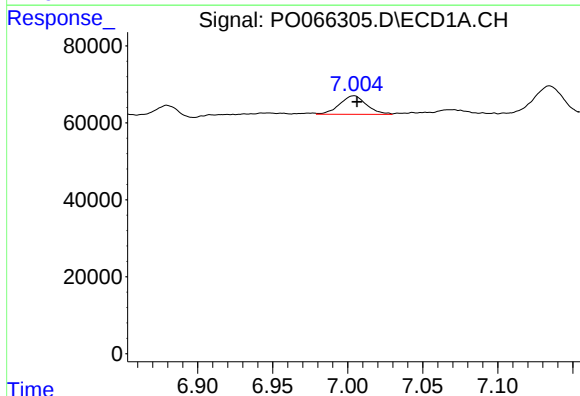


#29 AR-1254-4

R.T.: 7.004 min
Delta R.T.: -0.002 min
Response: 60169
Conc: 26.06 ng/ml m

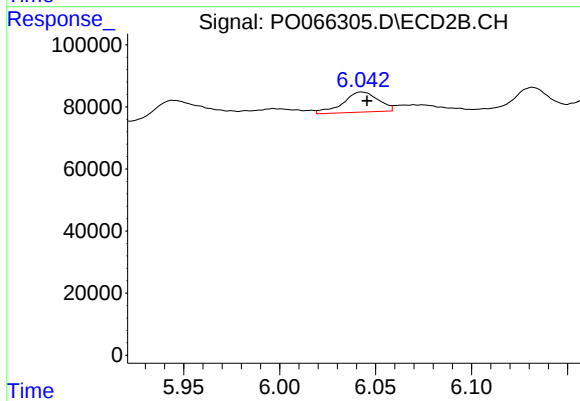

#29 AR-1254-4

R.T.: 6.042 min
Delta R.T.: -0.003 min
Response: 83333
Conc: 26.45 ng/ml

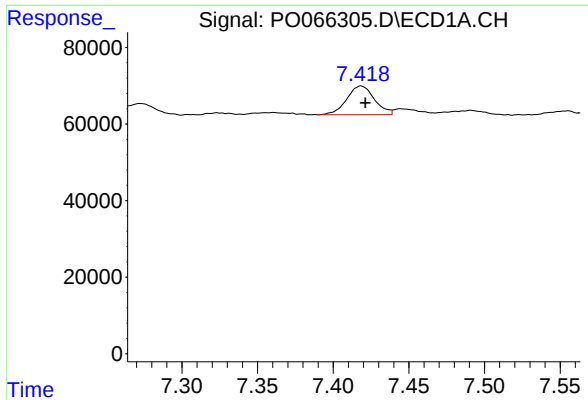


#30 AR-1254-5

R.T.: 7.418 min
Delta R.T.: -0.003 min
Response: 95640
Conc: 41.92 ng/ml m

Instrument :
ECD_O
ClientSampleId :
M030-6A

Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:32 PM

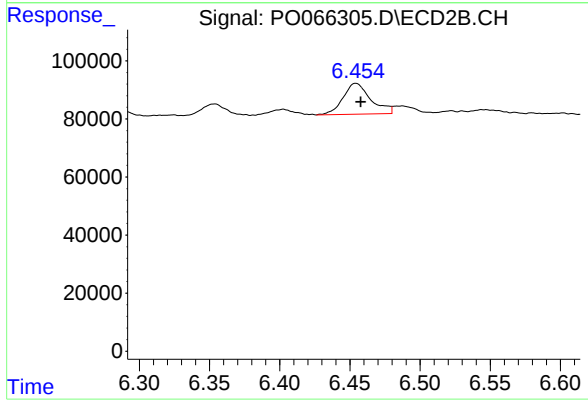

#30 AR-1254-5

R.T.: 6.454 min
Delta R.T.: -0.003 min
Response: 145917
Conc: 34.45 ng/ml