

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
 Data File : P0066307.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2020 20:33
 Operator : DD\AJ
 Sample : L1379-16
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M030-8A

Manual Integrations
 APPROVED

mohammad
 2/7/2020 5:03:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 05:05:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.430	665616	832472	22.849	20.352
2) SA Decachlor...	9.644	8.324	264366	367073	6.708	6.263

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
Data File : P0066307.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 20:33
Operator : DD\AJ
Sample : L1379-16
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
M030-8A


Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:05:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

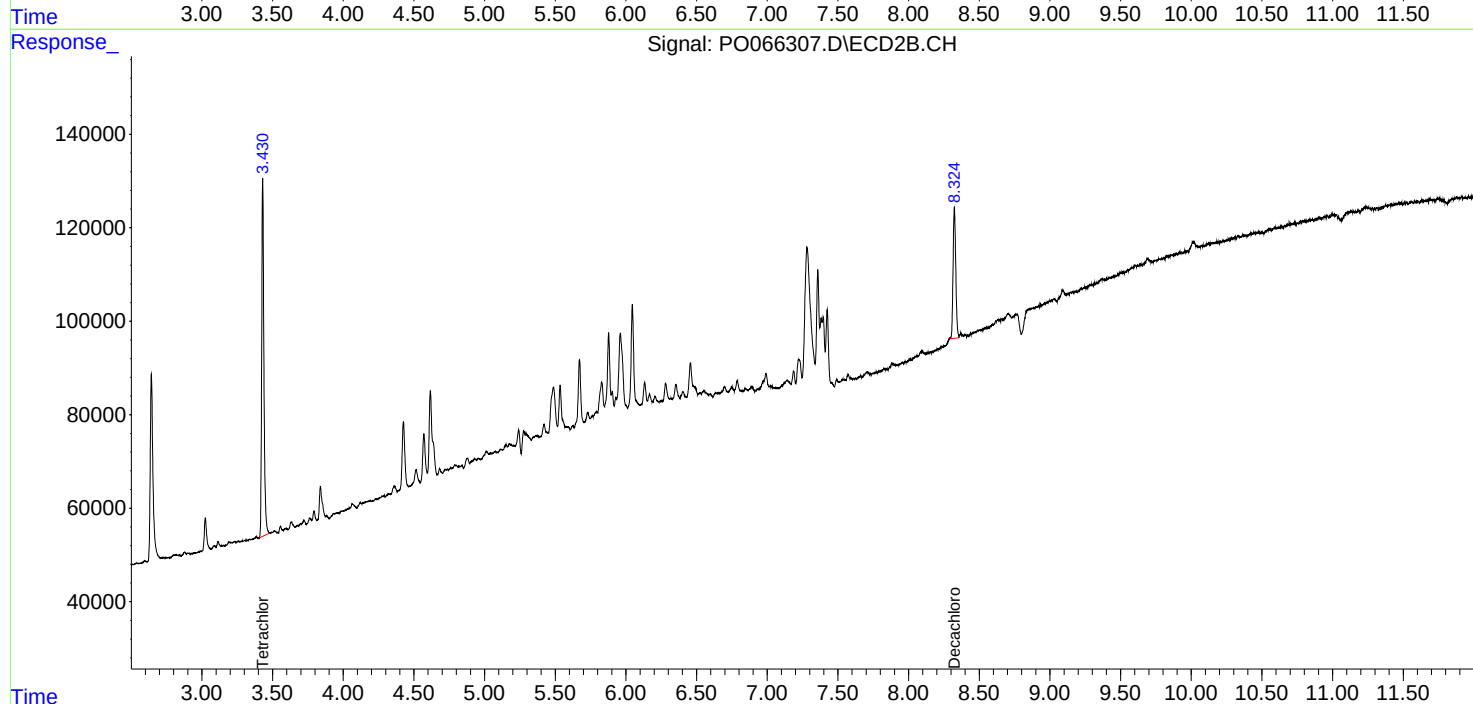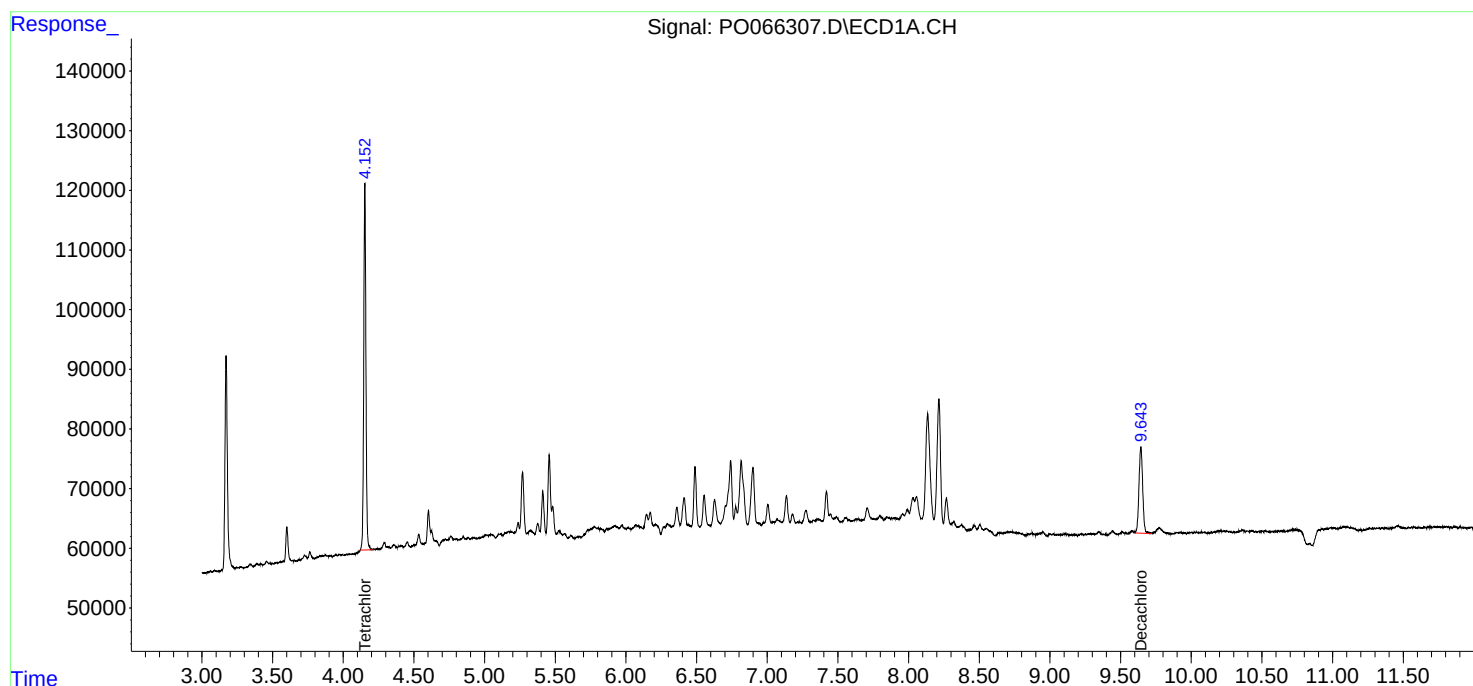

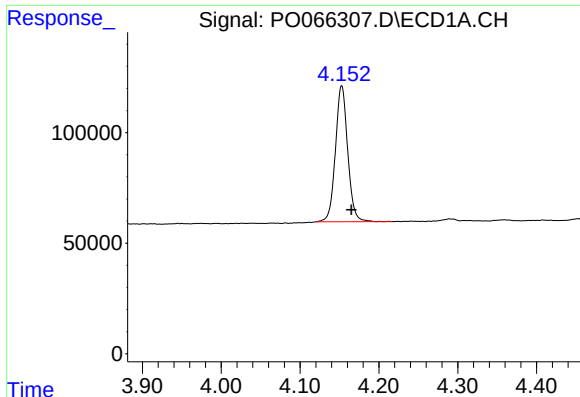


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: -0.012 min
Response: 665616
Conc: 22.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-8A


Manual Integrations
APPROVED

mohammad
2/7/2020 5:03:37 PM

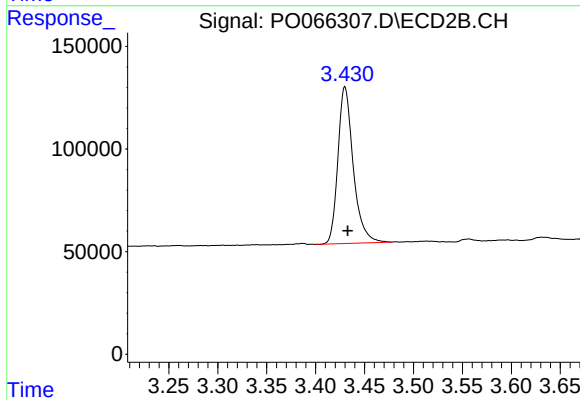


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 832472
Conc: 20.35 ng/ml

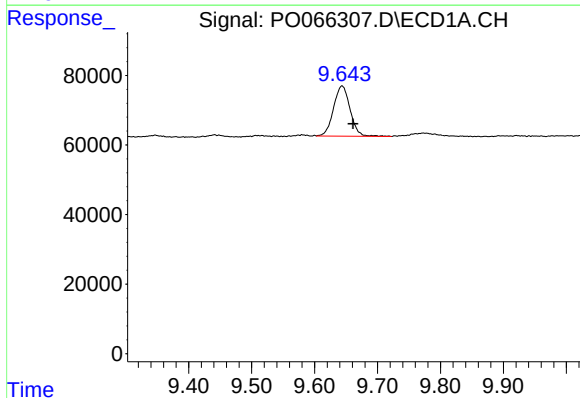

#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.018 min
Response: 264366
Conc: 6.71 ng/ml

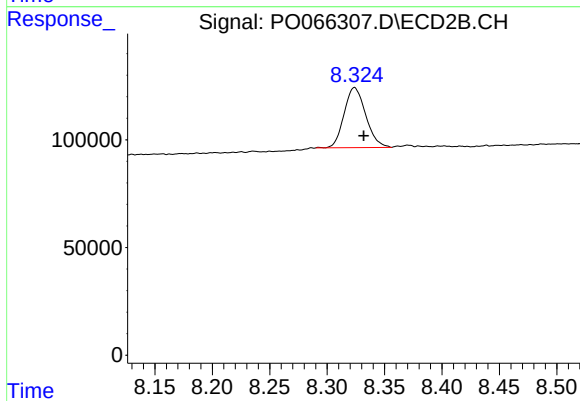

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.008 min
Response: 367073
Conc: 6.26 ng/ml