

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
 Data File : P0066308.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Feb 2020 20:49
 Operator : DD\AJ
 Sample : L1379-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M030-9A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 05:06:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.152	3.430	730249	920374	25.068	22.501
2) SA Decachlor...	9.644	8.324	224463	331812	5.696	5.661

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
Data File : P0066308.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 20:49
Operator : DD\AJ
Sample : L1379-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
M030-9A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:06:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

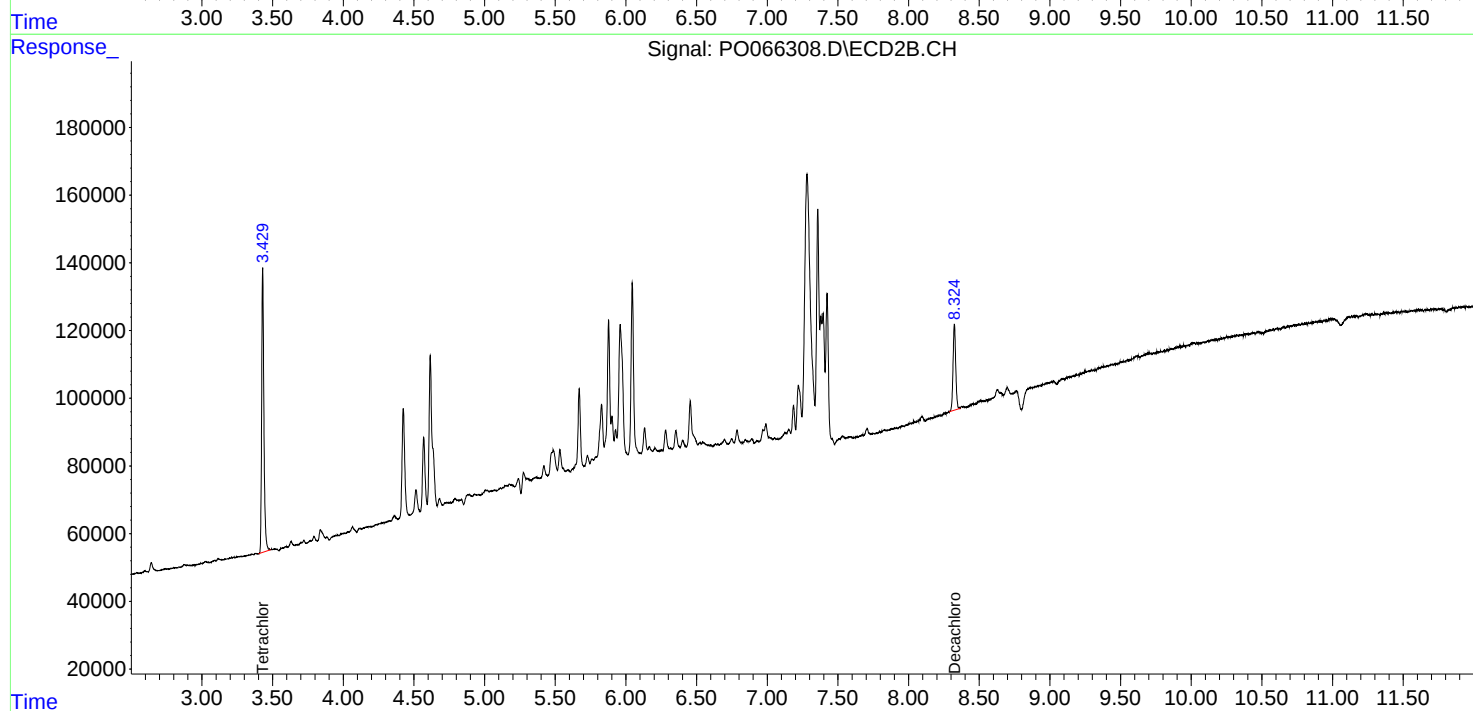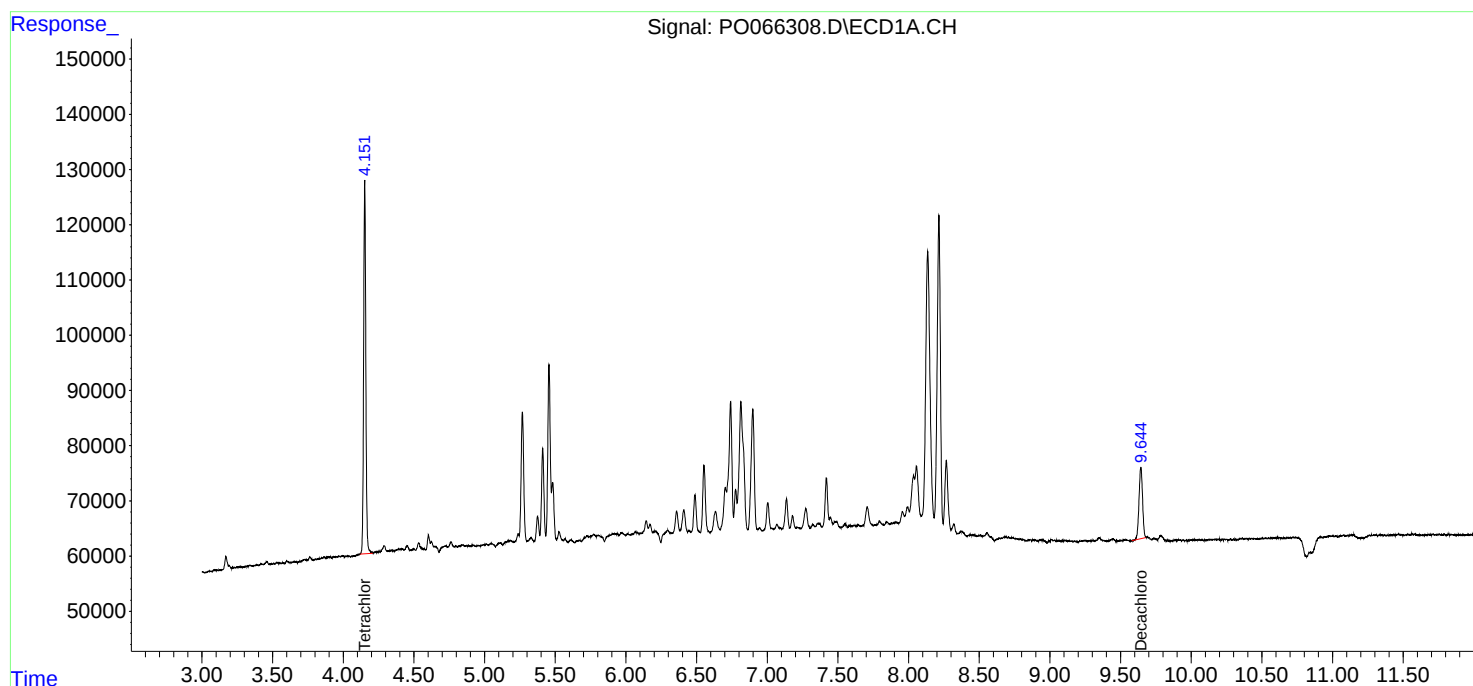


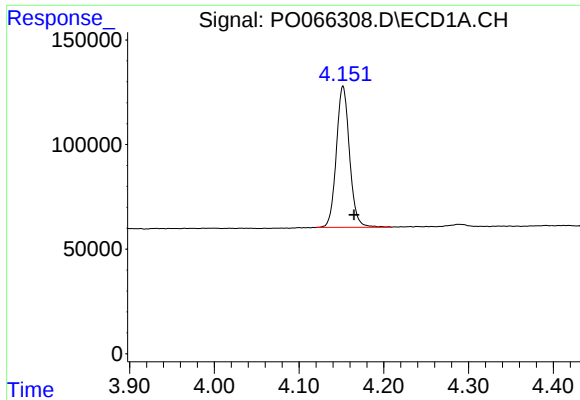

#1 Tetrachloro-m-xylene


R.T.: 4.152 min
Delta R.T.: -0.013 min
Response: 730249
Conc: 25.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
M030-9A

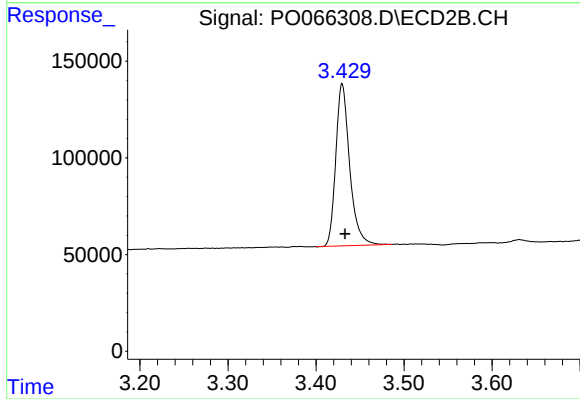


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 920374
Conc: 22.50 ng/ml

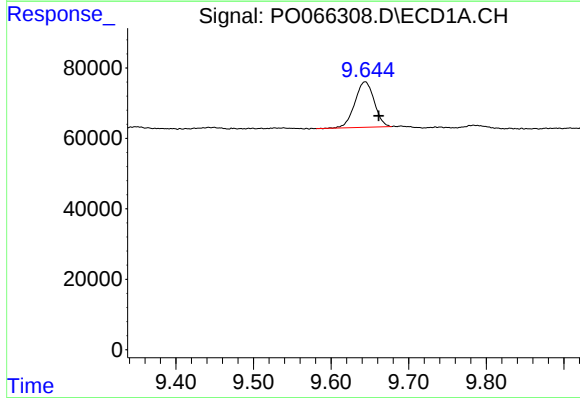

#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.018 min
Response: 224463
Conc: 5.70 ng/ml

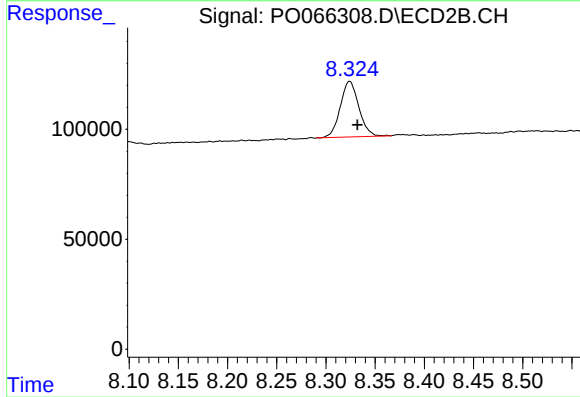

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.008 min
Response: 331812
Conc: 5.66 ng/ml