

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
Data File : P0066314.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 23:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:08:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.429	885402	1142690	30.394	27.936
2) SA Decachlor...	9.644	8.323	716705	1021848	18.187	17.434

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020520\
Data File : P0066314.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Feb 2020 23:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 05:08:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

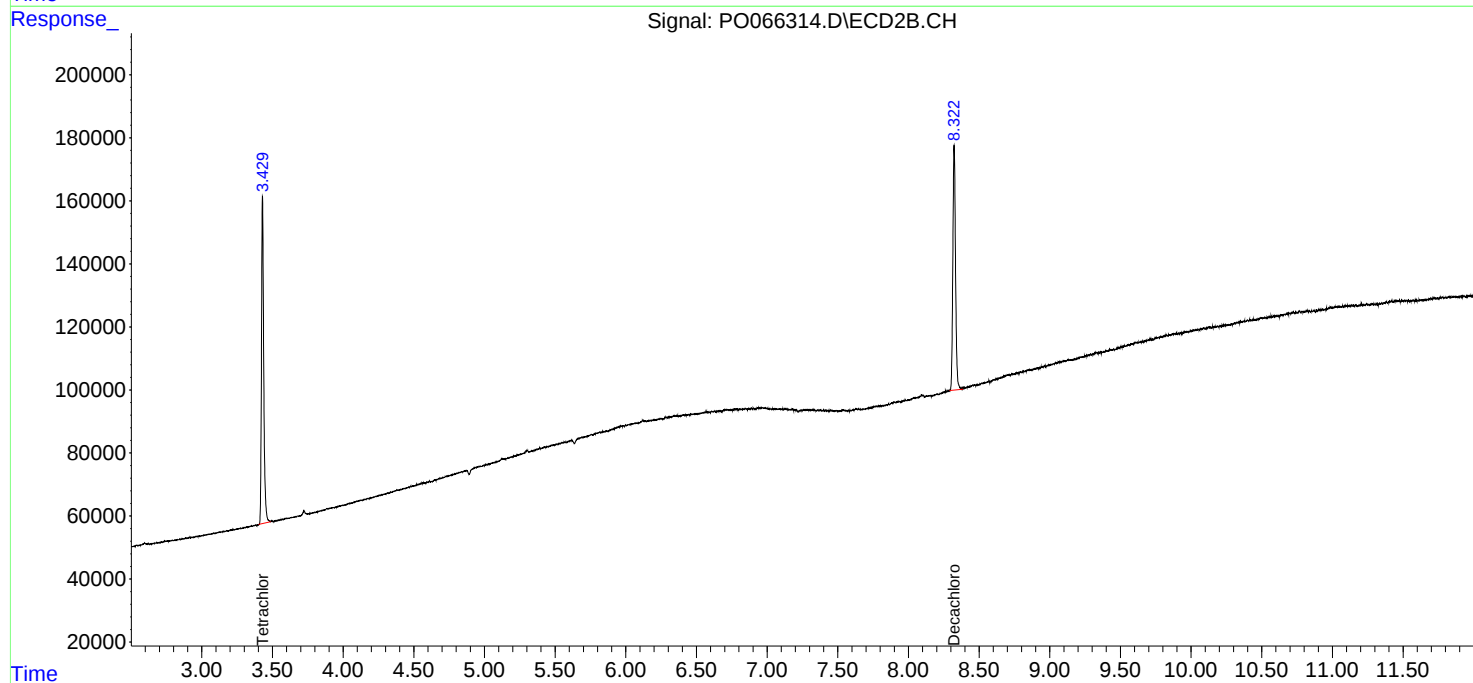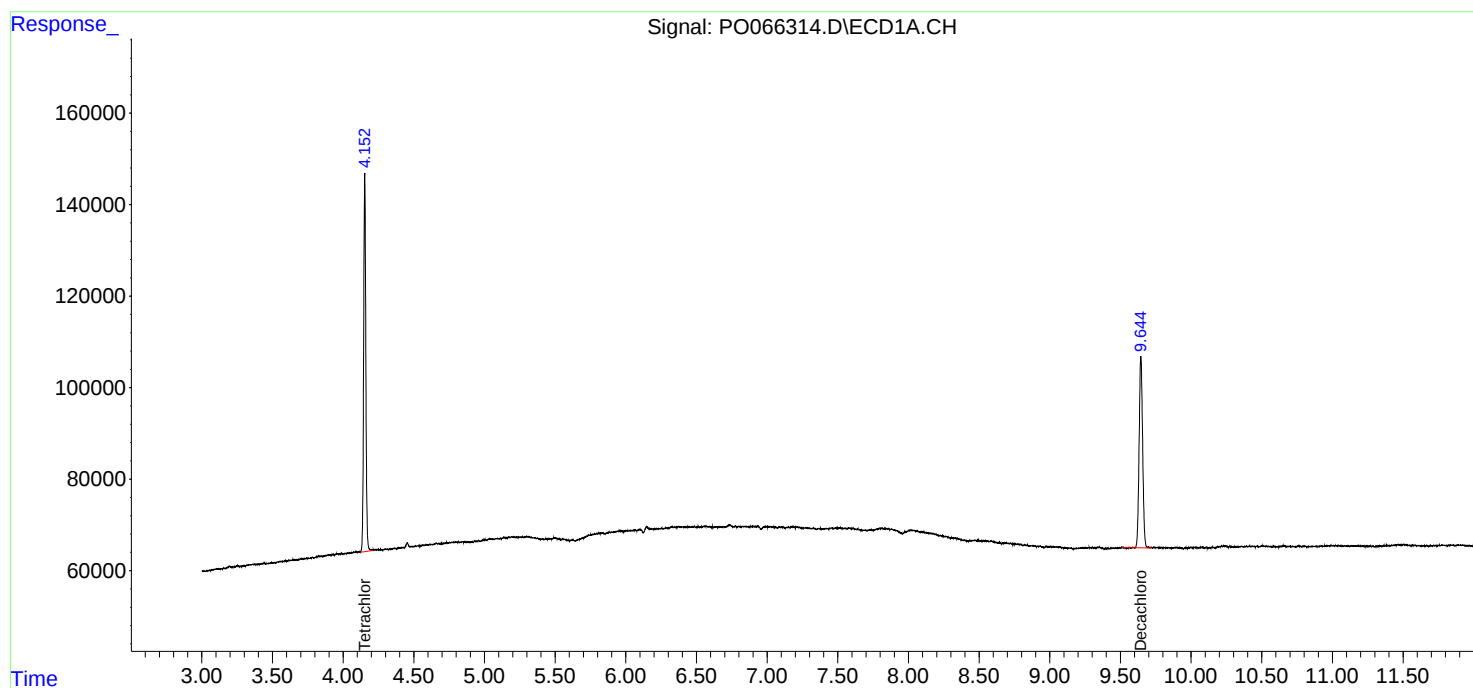


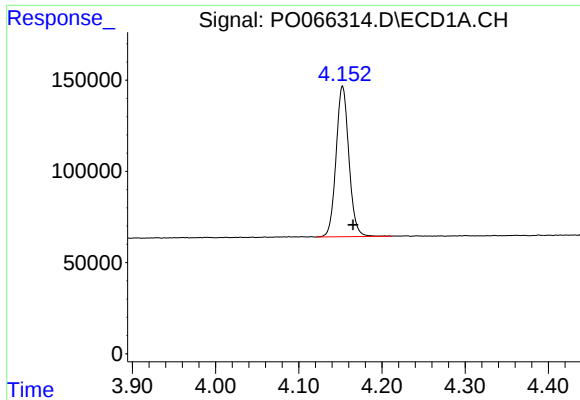

#1 Tetrachloro-m-xylene


R.T.: 4.153 min
Delta R.T.: -0.012 min
Response: 885402
Conc: 30.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

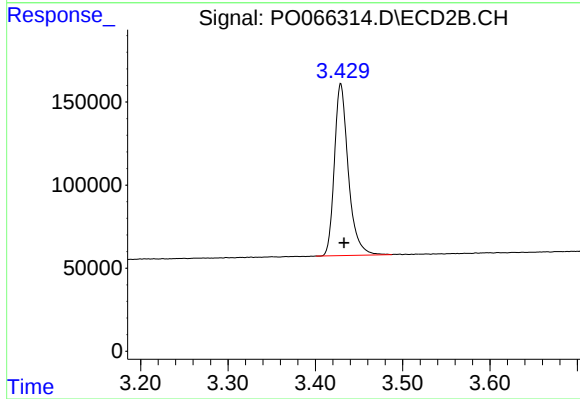


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: -0.004 min
Response: 1142690
Conc: 27.94 ng/ml

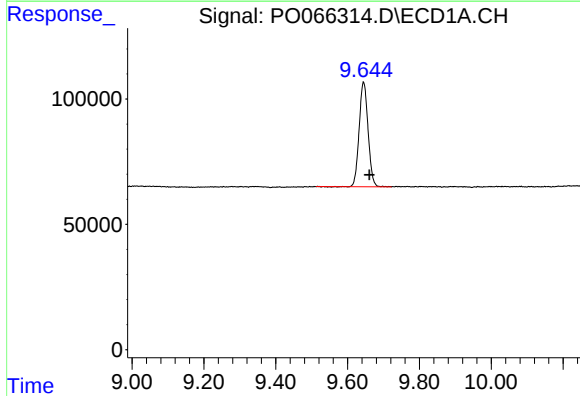

#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.017 min
Response: 716705
Conc: 18.19 ng/ml

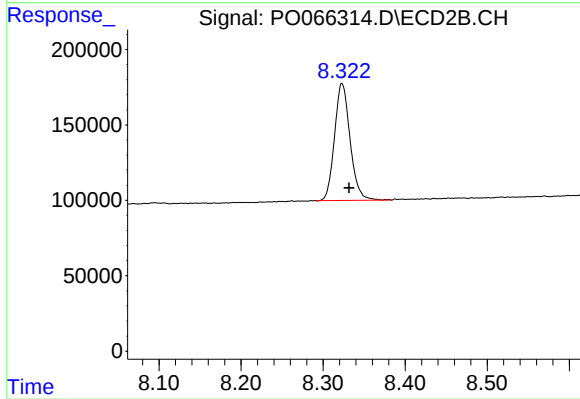

#2 Decachlorobiphenyl

R.T.: 8.323 min
Delta R.T.: -0.009 min
Response: 1021848
Conc: 17.43 ng/ml