

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
 Data File : PL064644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2021 09:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:42:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.108	68461281	56752168	22.489	23.825
28)	SA Decachlor...	8.165	9.273	67869554	50409606	21.537	24.621
Target Compounds							
4)	MA Heptachlor	0.000	5.302	0	7017285	N.D.	2.013 #
7)	B delta-BHC	0.000	5.222f	0	4171824	N.D.	1.354 #
23)	Chlordane-1	4.319f	0.000	5226454	0	47.547	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
Data File : PL064644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2021 09:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:42:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

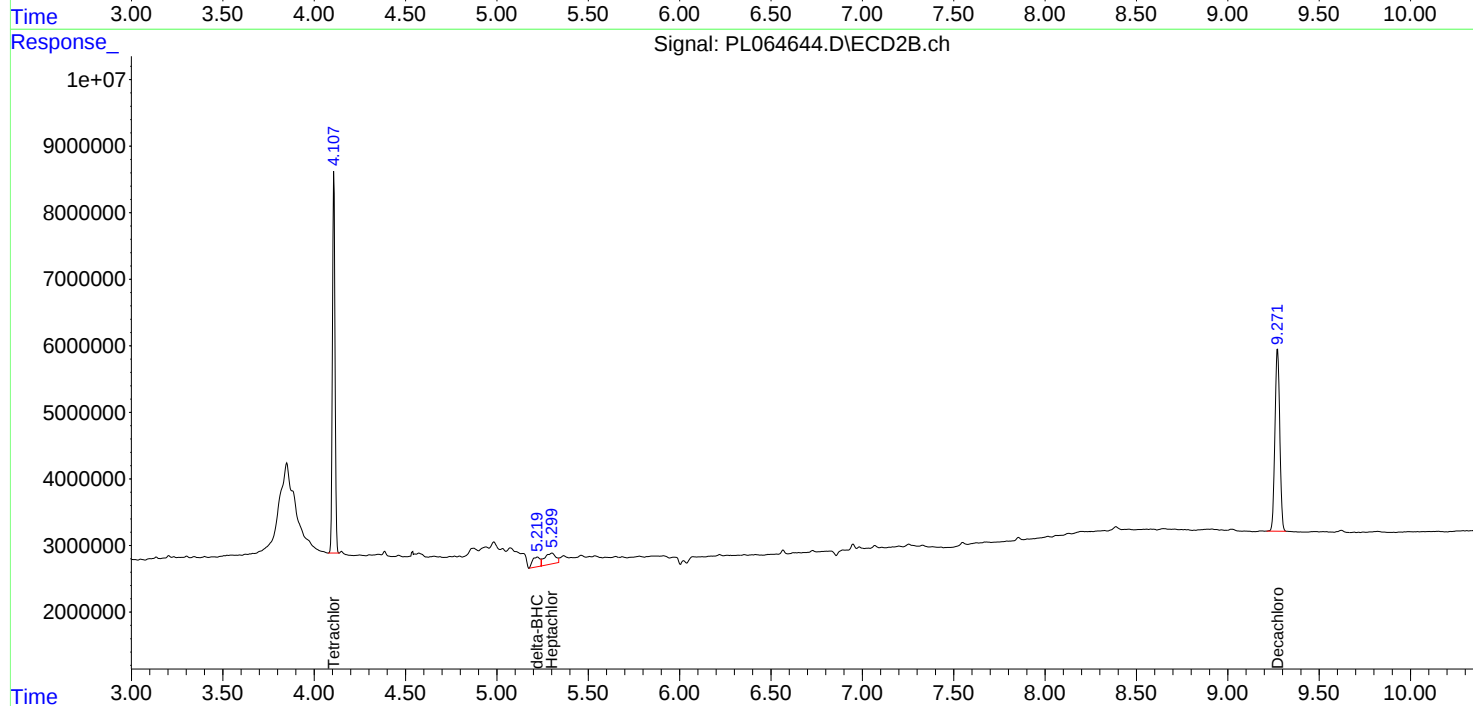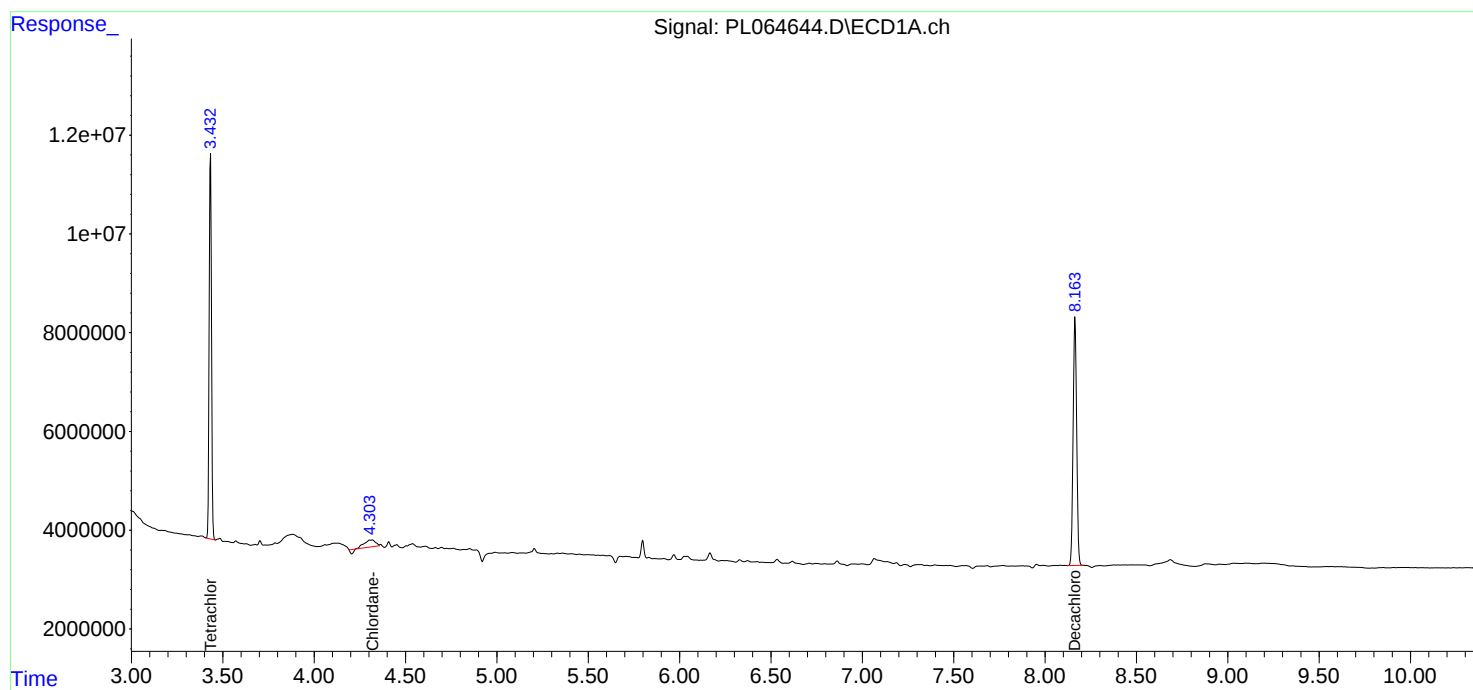


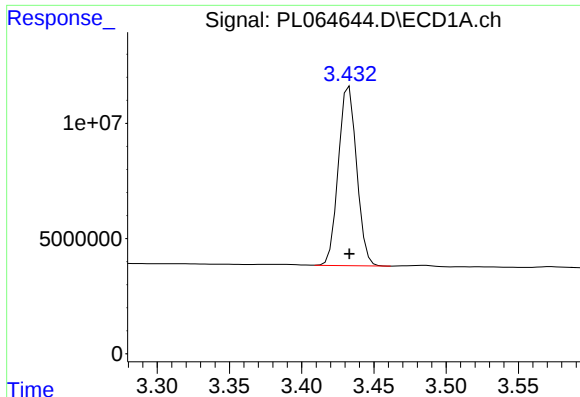

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 68461281
Conc: 22.49 ng/ml

Instrument :
ECD_O
ClientSampleId :

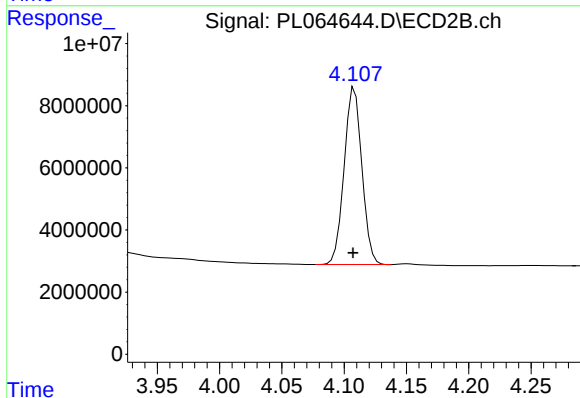


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 56752168
Conc: 23.83 ng/ml

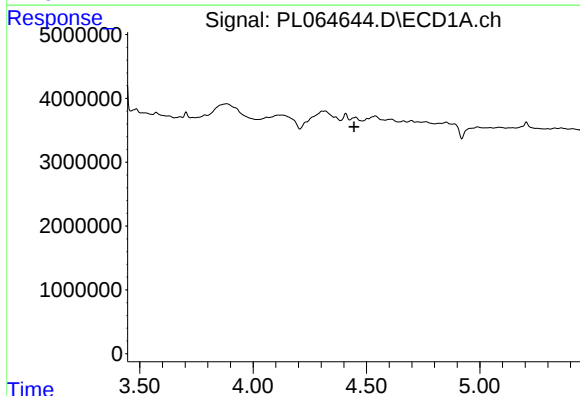


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

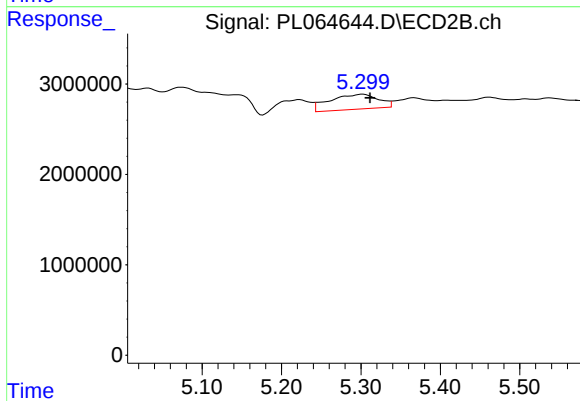

#4 Heptachlor


R.T.: 5.302 min
Delta R.T.: -0.009 min
Response: 7017285
Conc: 2.01 ng/ml

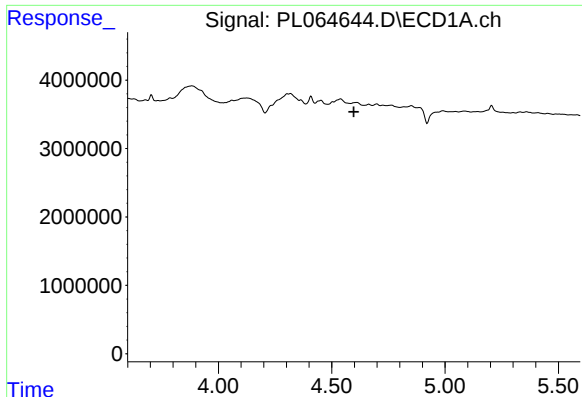

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

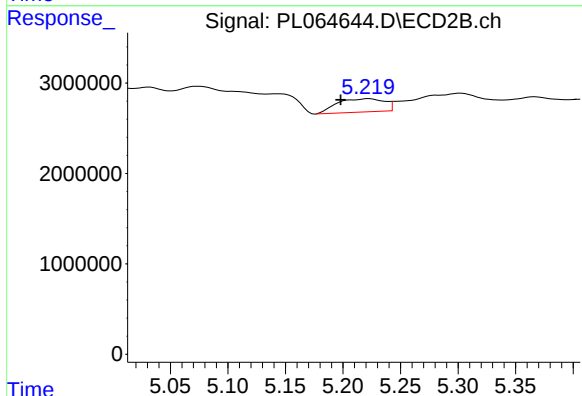


#7 delta-BHC

R.T.: 5.222 min
Delta R.T.: 0.024 min
Response: 4171824
Conc: 1.35 ng/ml

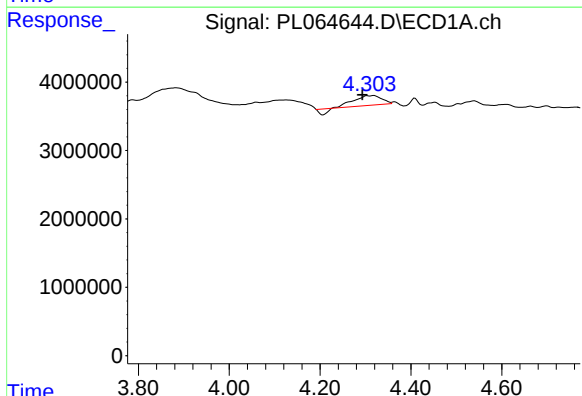


#23 Chlordane-1

R.T.: 4.319 min
Delta R.T.: 0.025 min
Response: 5226454
Conc: 47.55 ng/ml

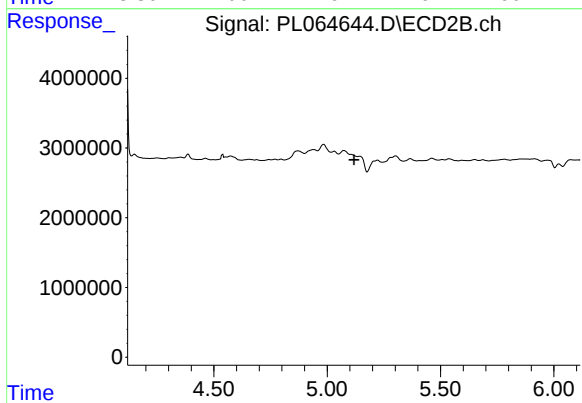

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

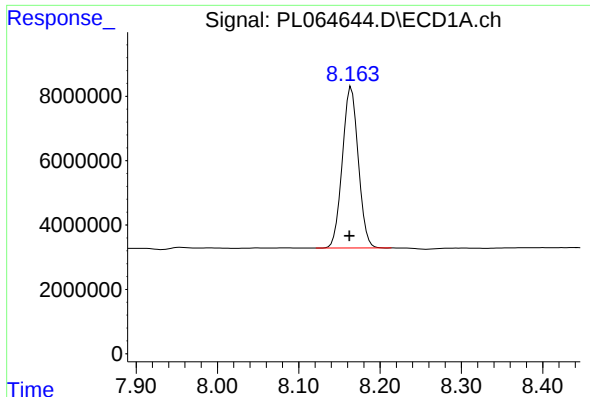

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.002 min
Response: 67869554
Conc: 21.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

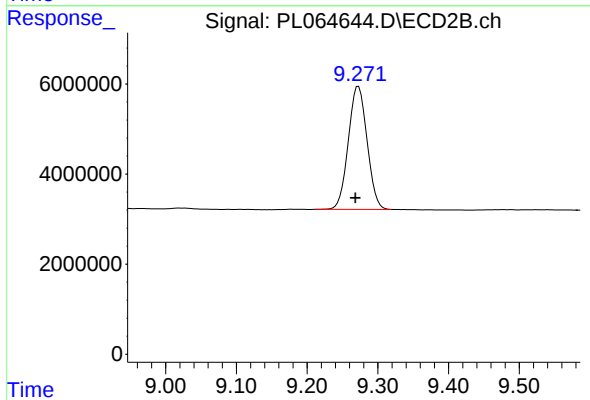

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.004 min
Response: 50409606
Conc: 24.62 ng/ml